
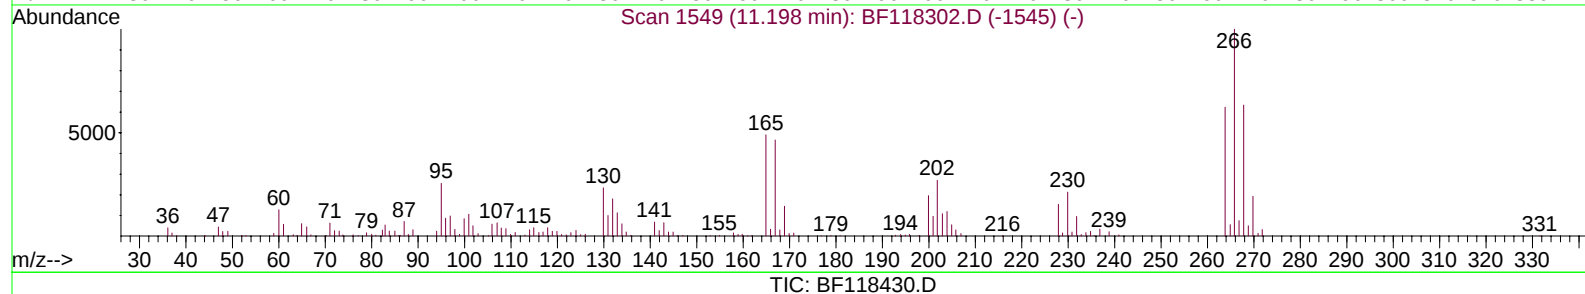
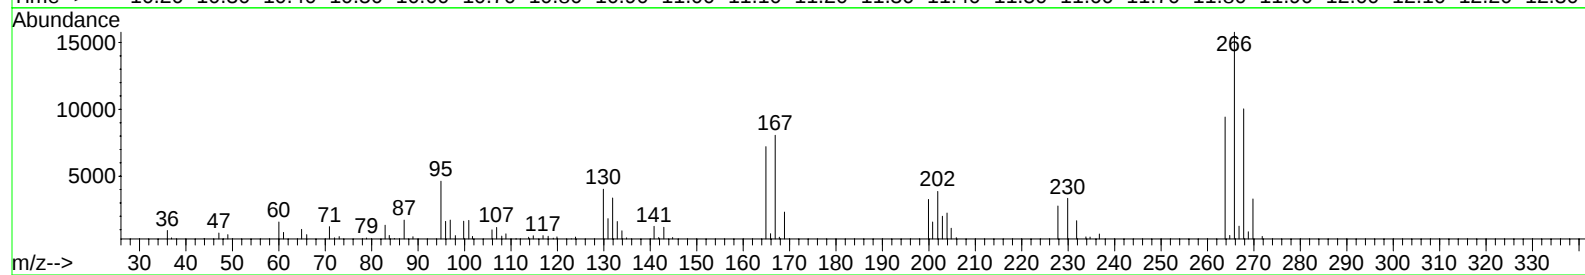


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF010220\
Data File : BF118430.D
Acq On : 2 Jan 2020 11:58
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 18:23:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF122419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 15:58:52 2019
Response via : Initial Calibration

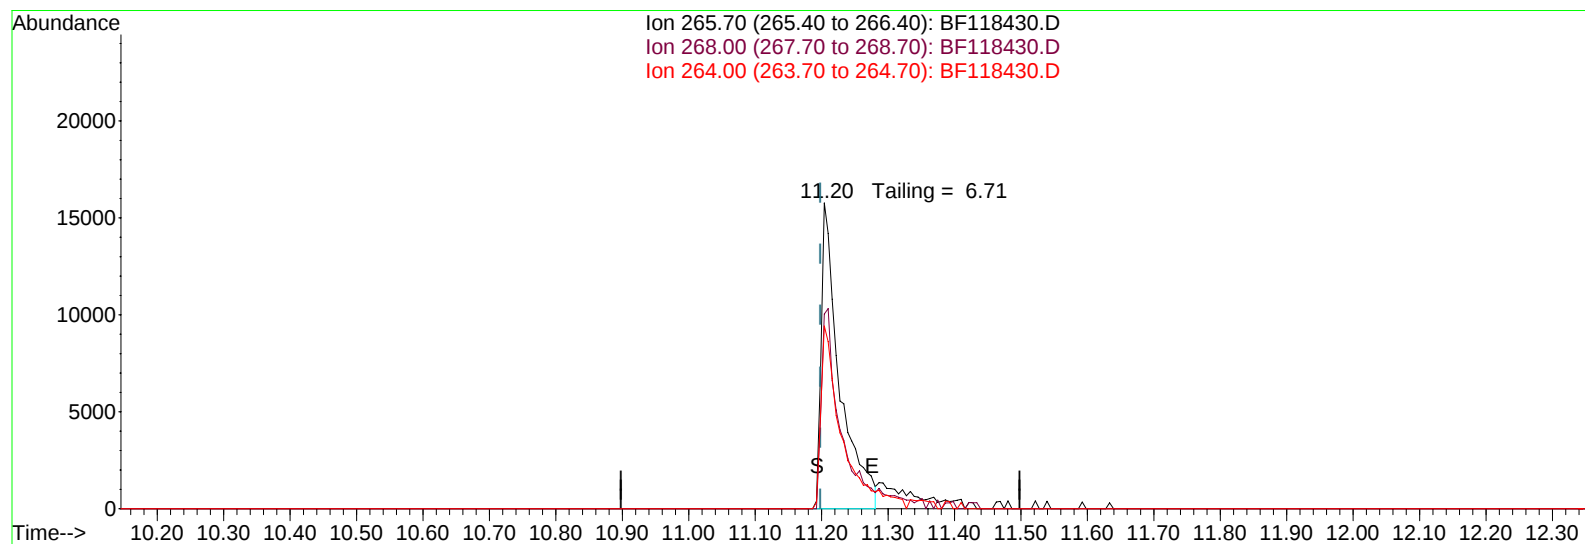

(70) Pentachlorophenol (C)




11.204min (+0.006) 15866.29ng

response 34360

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	63.67
264.00	62.40	59.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF010220\
Data File : BF118430.D
Acq On : 2 Jan 2020 11:58
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 18:23:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF122419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 15:58:52 2019
Response via : Initial Calibration

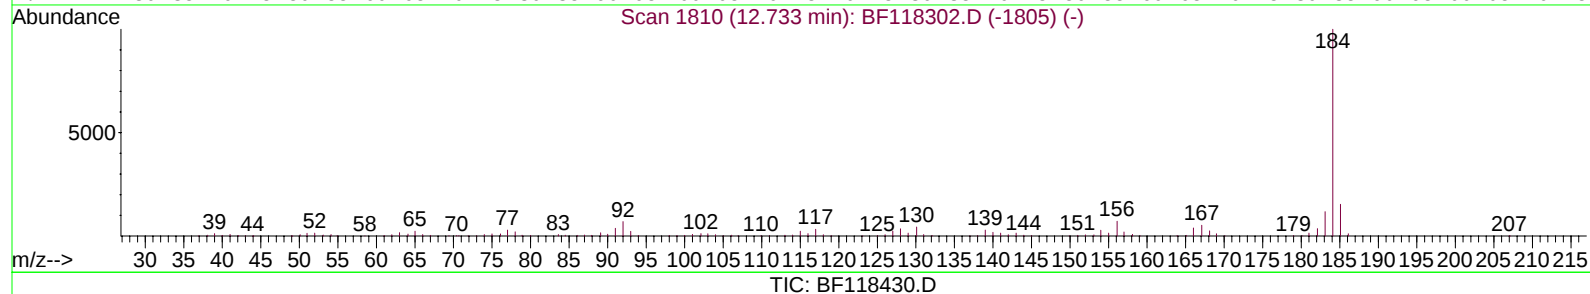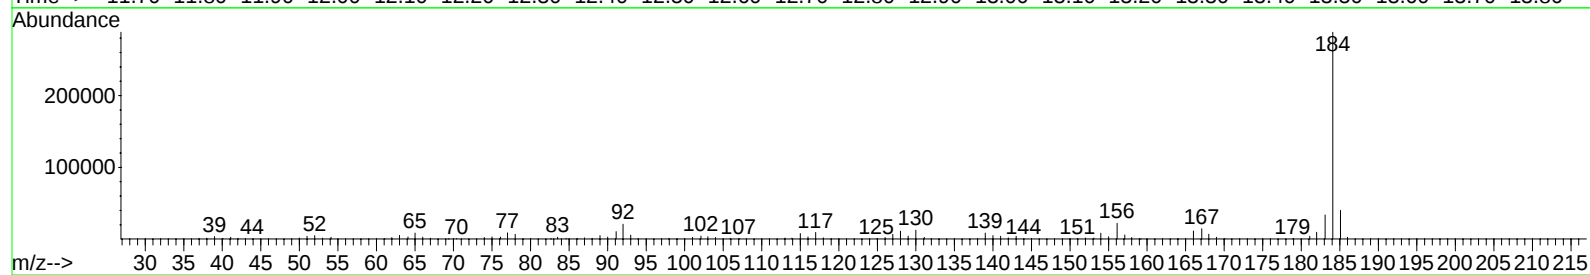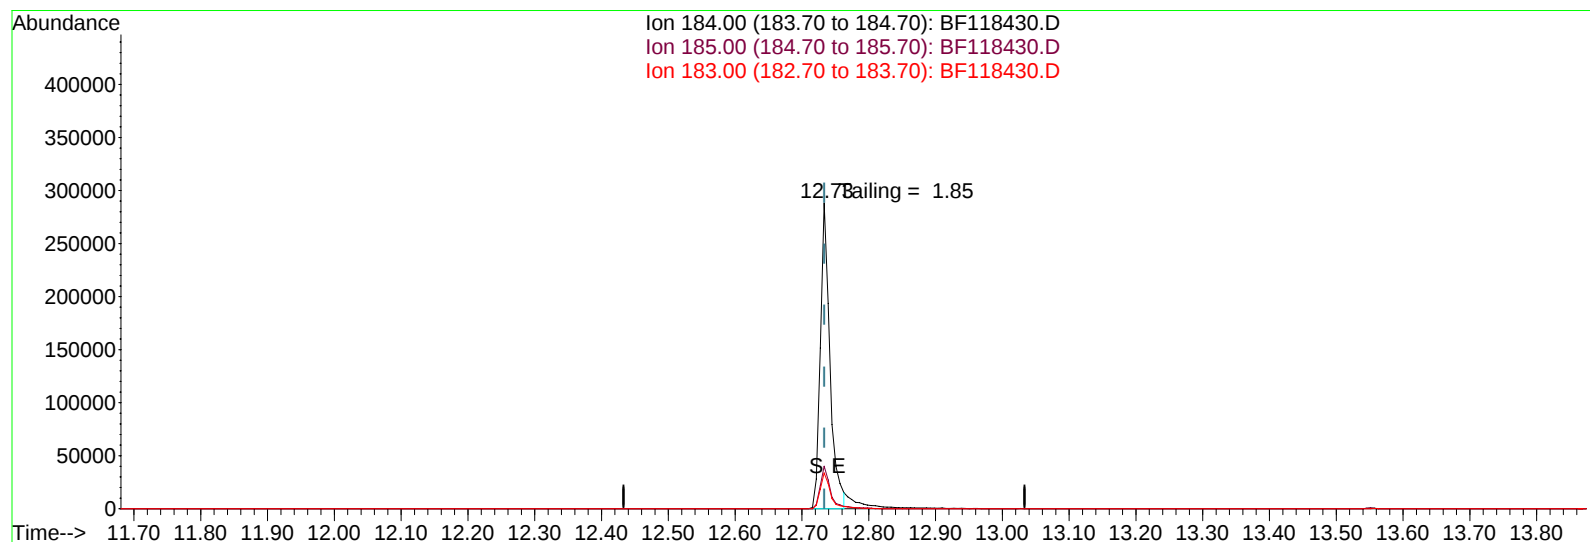

(77) Benzidine

12.733min (+0.000) 0.00ng

response 310405

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	13.91
183.00	11.80	11.72
0.00	0.00	0.00