


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010220\
 Data File : BF118430.D
 Acq On : 2 Jan 2020 11:58
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 15:58:52 2019

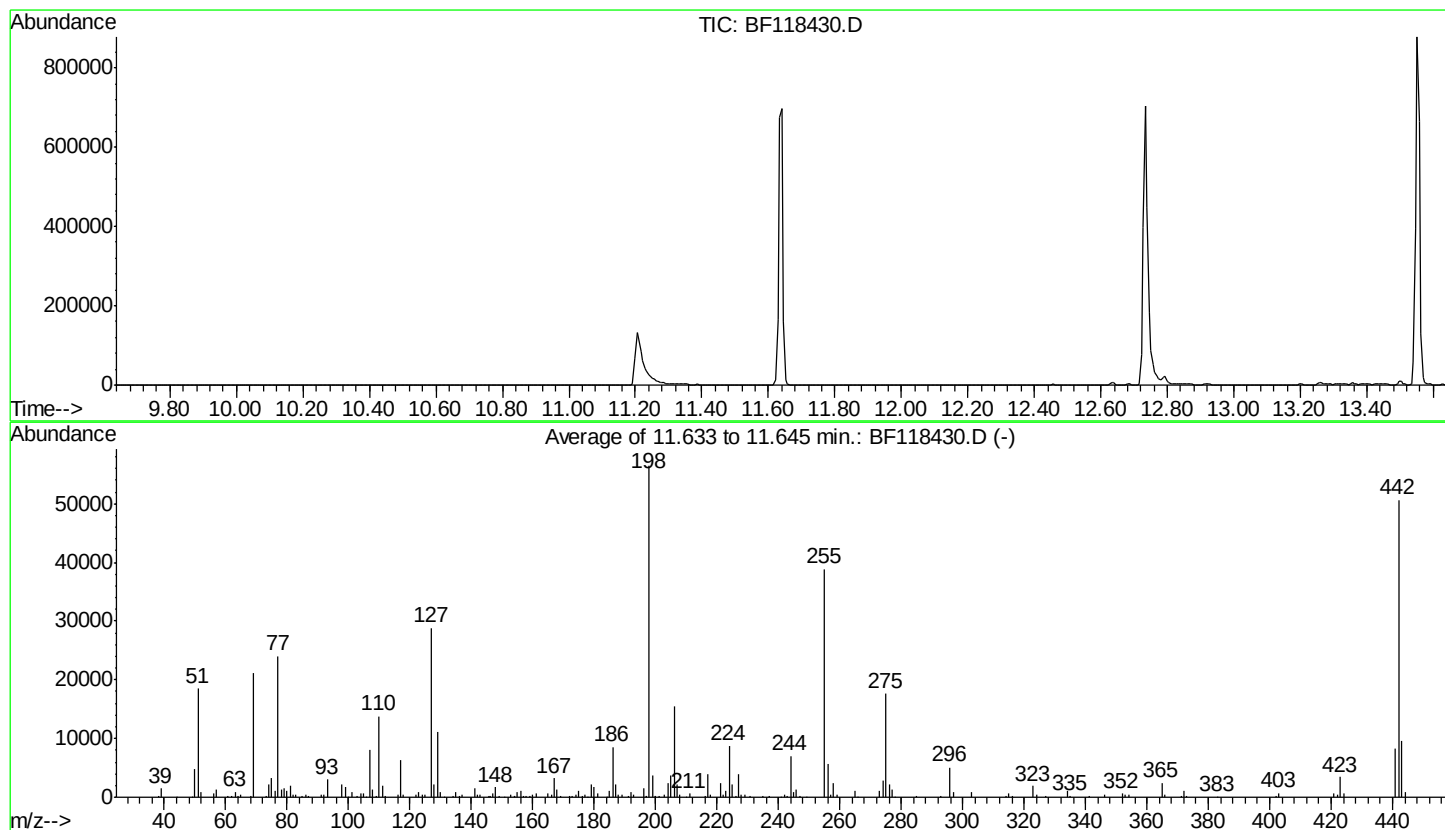

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	18499	PASS
68	69	0.00	2	1.3	269	PASS
69	198	0.00	100	37.5	21183	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.0	28831	PASS
197	198	0.00	2	0.5	274	PASS
198	198	100	100	100.0	56488	PASS
199	198	5	9	6.6	3712	PASS
275	198	10	60	31.1	17571	PASS
365	198	1	100	4.3	2440	PASS
441	198	0.01	100	14.7	8323	PASS
442	198	50	100	89.6	50637	PASS
443	442	15	24	18.9	9579	PASS