
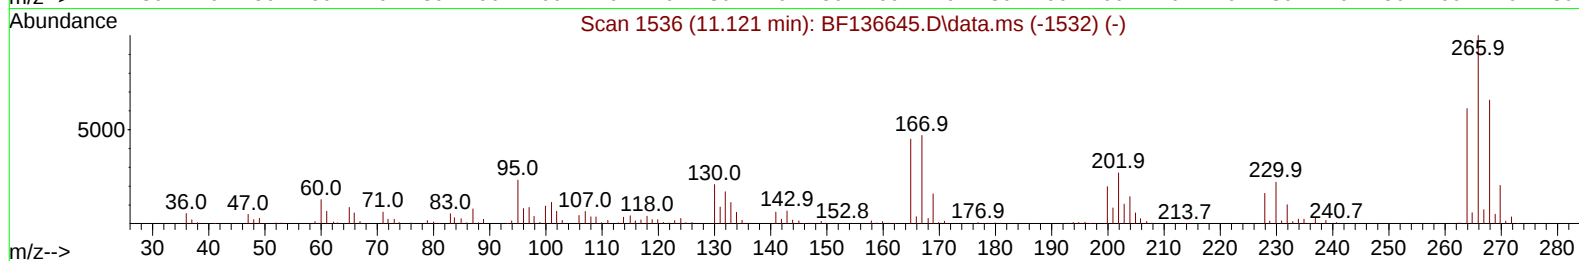
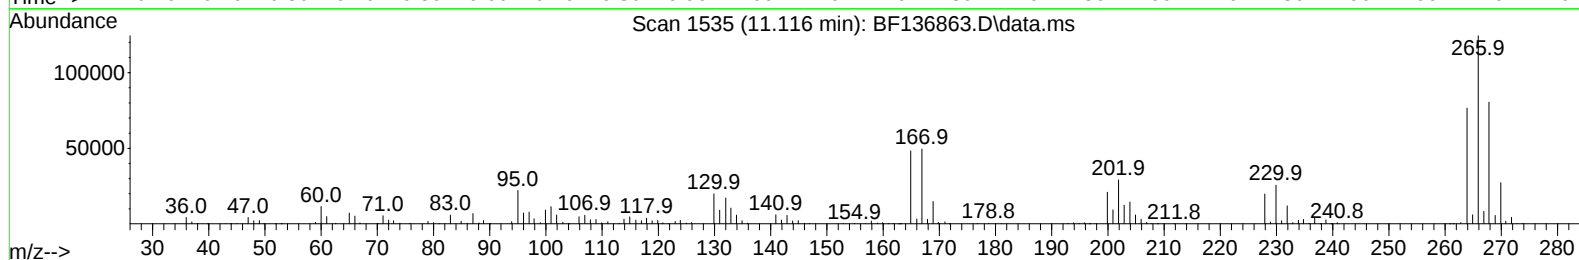


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010224\
Data File : BF136863.D
Acq On : 02 Jan 2024 10:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 12:21:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

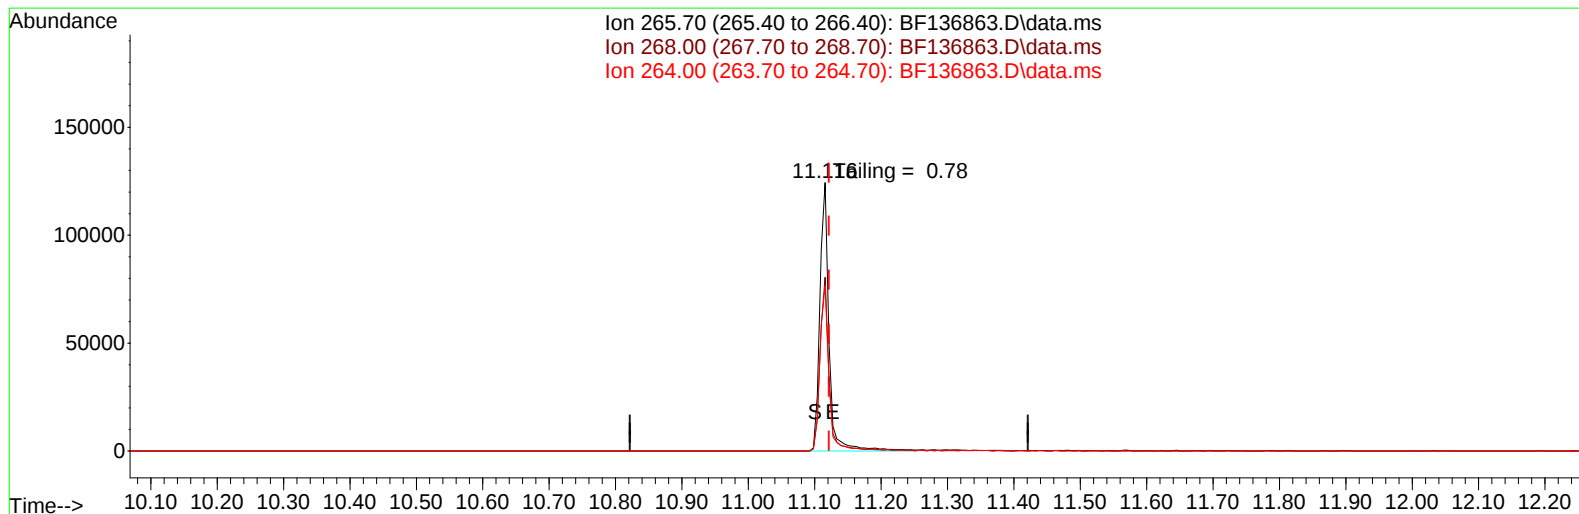

TIC: BF136863.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.006) 40234.39 ng

response 119533

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	64.70
264.00	61.20	61.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010224\
Data File : BF136863.D
Acq On : 02 Jan 2024 10:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 12:21:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

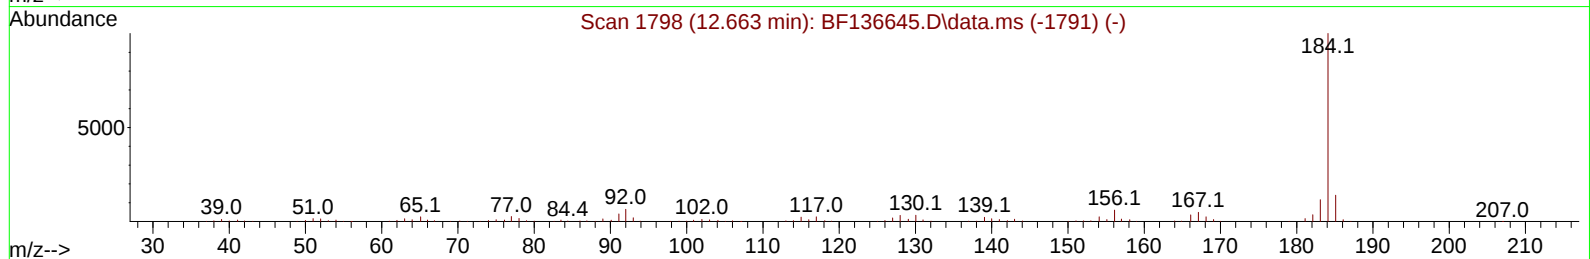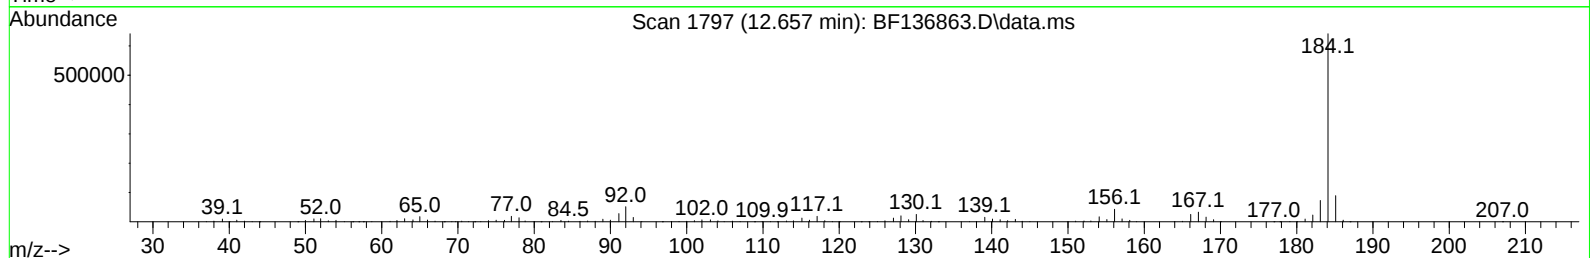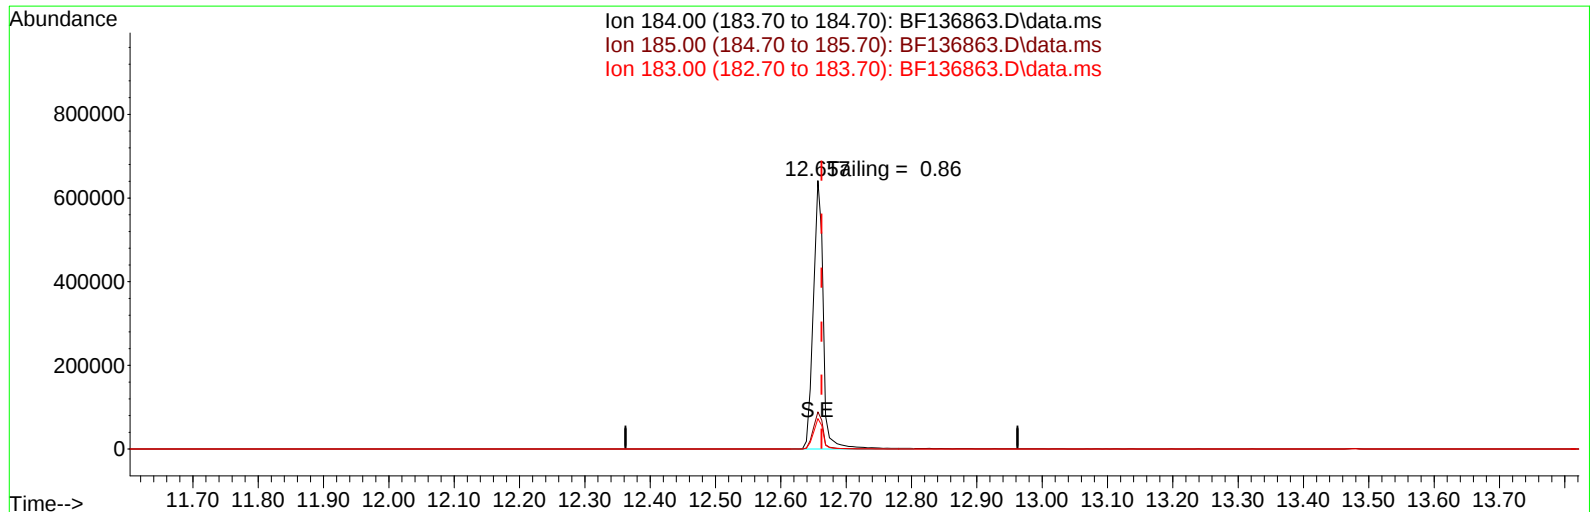

TIC: BF136863.D\data.ms

(77) Benzidine

12.657min (-0.006) 0.00 ng m

response 677873

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.86
183.00	11.60	11.34
0.00	0.00	0.00