
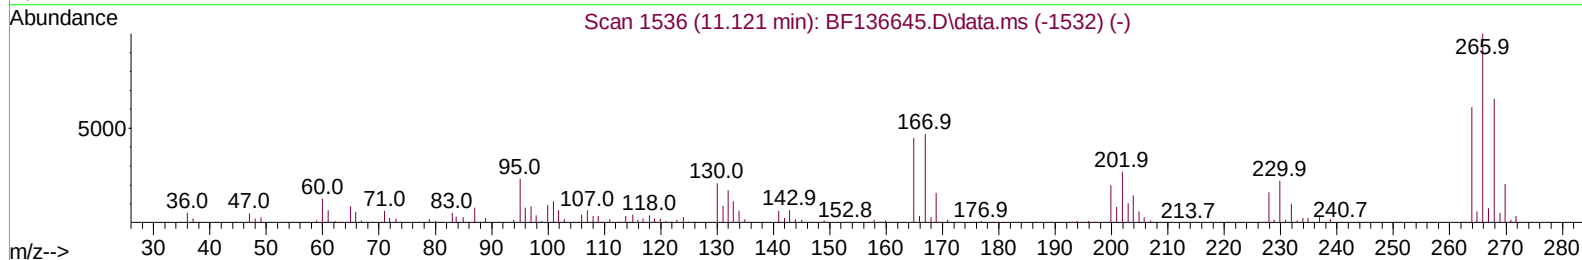
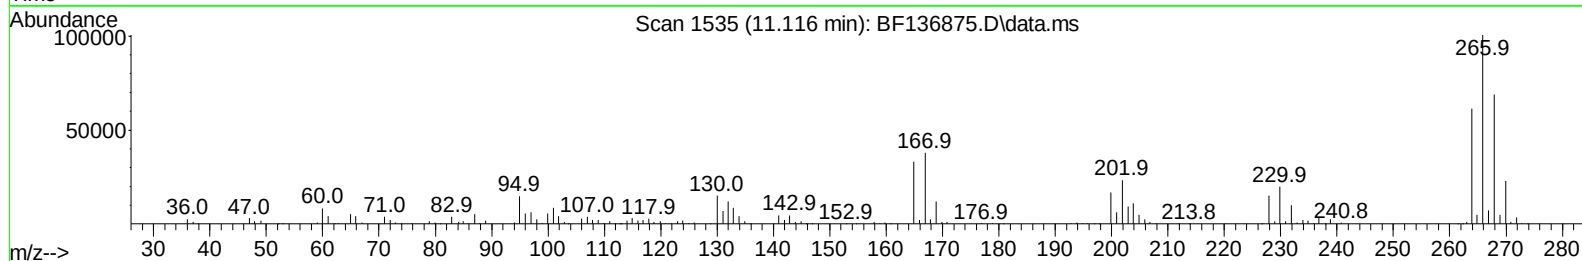


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010224\
Data File : BF136875.D
Acq On : 02 Jan 2024 17:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 01:51:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

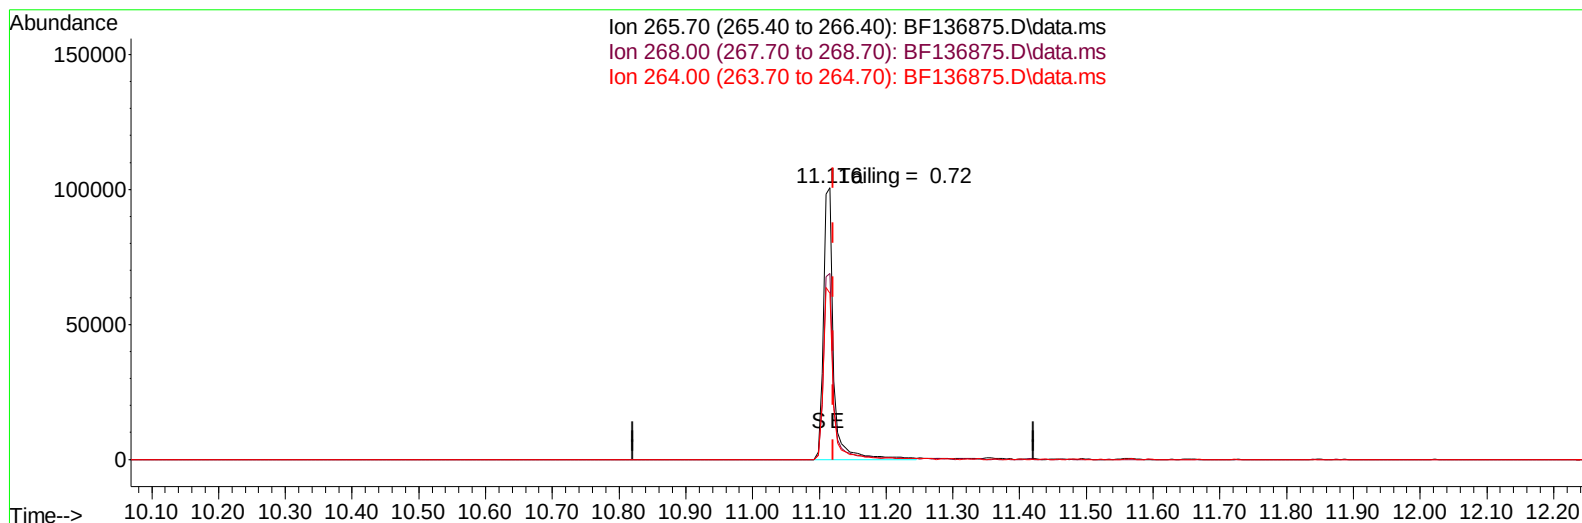

TIC: BF136875.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.006) 33469.73 ng

response 107352

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	68.47
264.00	61.20	61.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010224\
Data File : BF136875.D
Acq On : 02 Jan 2024 17:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 01:51:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

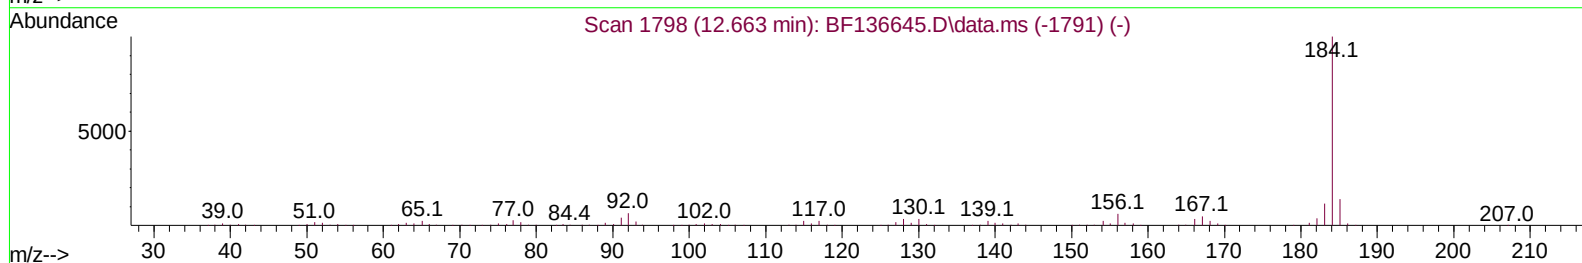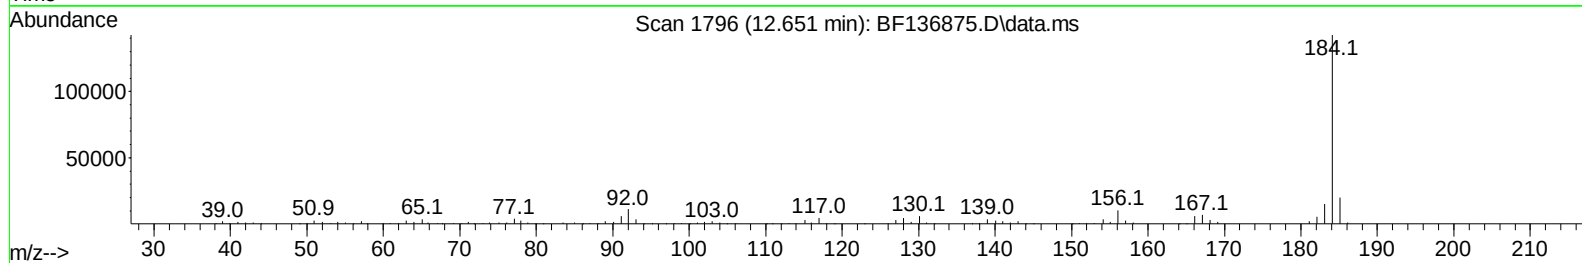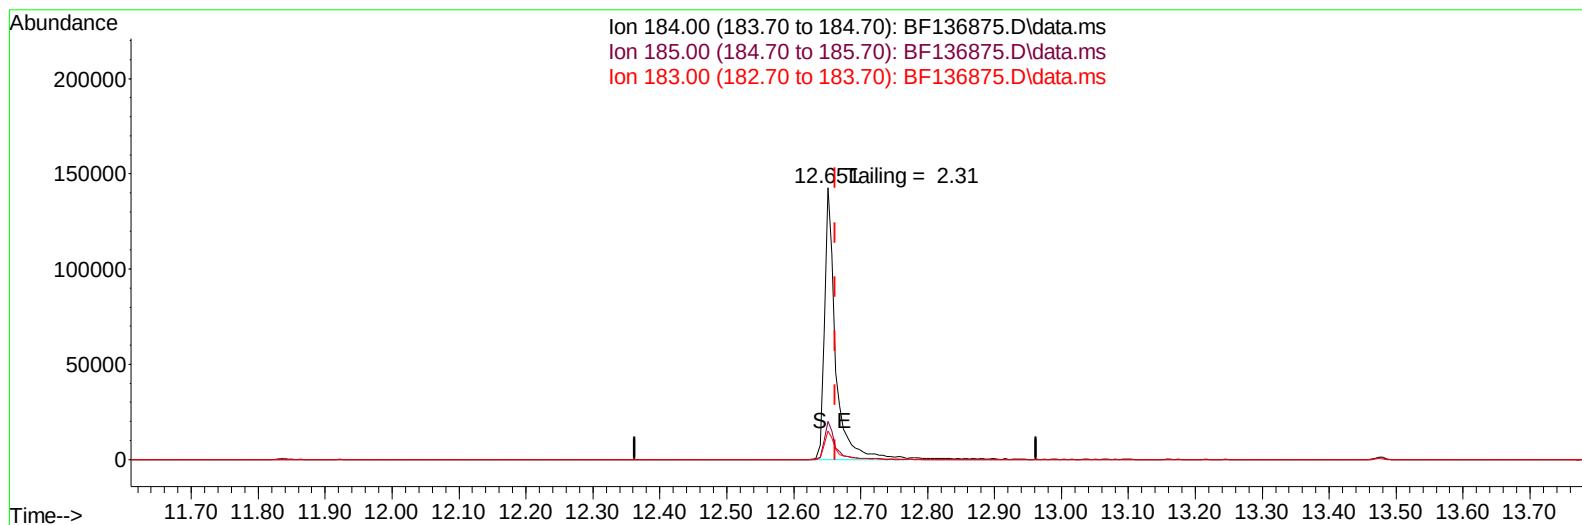

TIC: BF136875.D\data.ms

(77) Benzidine**12.651min (-0.012) 0.00 ng****response 166318**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.10
183.00	11.60	10.48
0.00	0.00	0.00