

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010224\
Data File : BF136865.D
Acq On : 02 Jan 2024 11:52
Operator : CG\JU
Sample : PB158048TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158048TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.052	500	504	514	rVB	26532	35321	1.30%	0.224%
2	5.434	564	569	572	rBV	2187803	2051551	75.43%	12.984%
3	6.428	733	738	741	rBV	1911753	2049289	75.35%	12.969%
4	6.781	794	798	801	rBV	512061	443482	16.31%	2.807%
5	7.346	888	894	897	rBV	1330395	1365992	50.22%	8.645%
6	8.057	1010	1015	1018	rBV	663635	599136	22.03%	3.792%
7	9.134	1192	1198	1201	rBV	2670055	2628953	96.66%	16.638%
8	9.810	1308	1313	1317	rBV	784820	690013	25.37%	4.367%
9	10.610	1444	1449	1452	rBV	1660898	1521850	55.95%	9.631%
10	11.304	1563	1567	1570	rBV	934604	739633	27.19%	4.681%
11	12.904	1834	1839	1842	rBV	2693402	2719873	100.00%	17.213%
12	13.957	2014	2018	2025	rVB	568439	525579	19.32%	3.326%
13	15.439	2265	2270	2283	rVB	323712	430454	15.83%	2.724%




Sum of corrected areas: 15801126

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010224\
Data File : BF136865.D
Acq On : 02 Jan 2024 11:52
Operator : CG\JU
Sample : PB158048TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158048TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

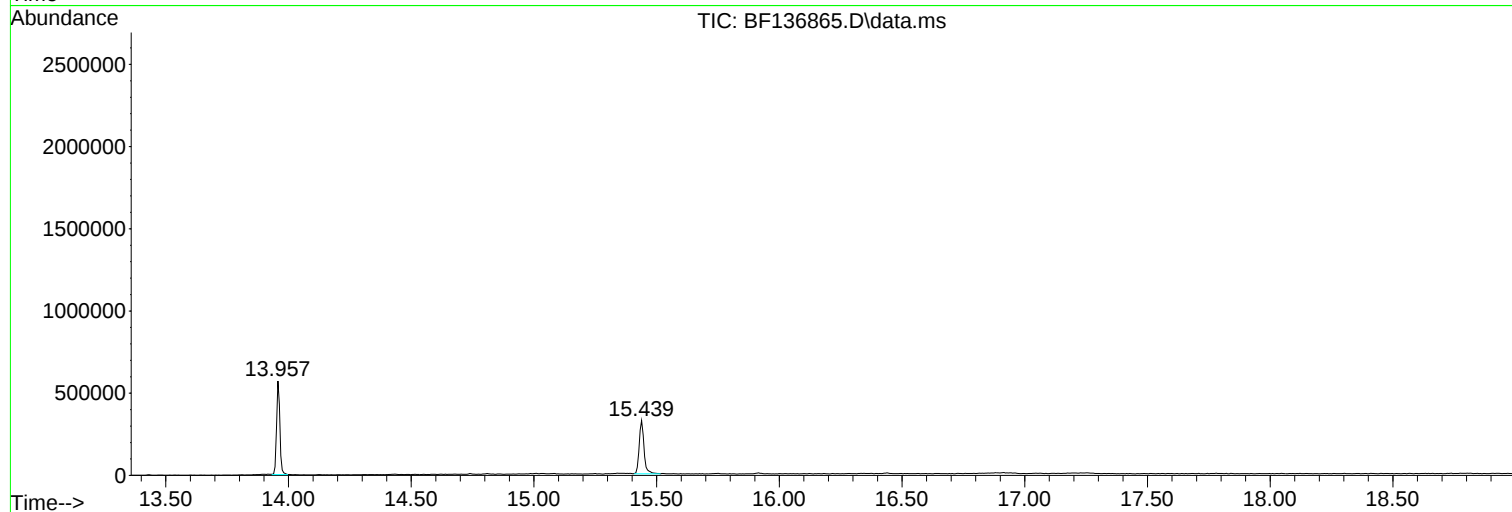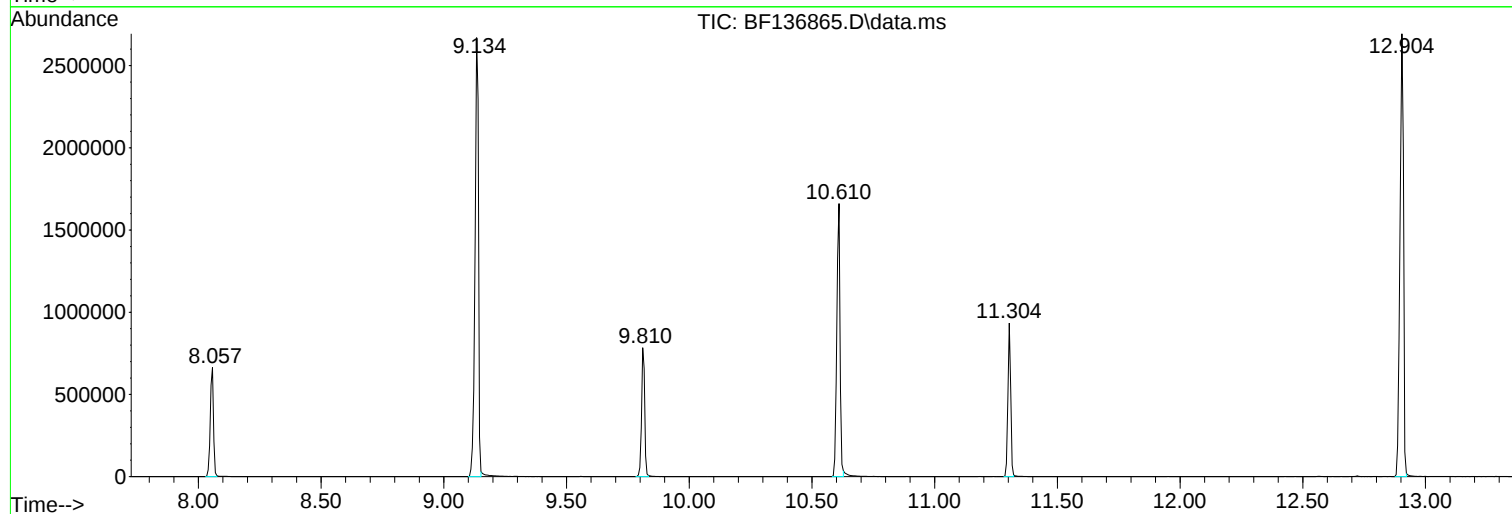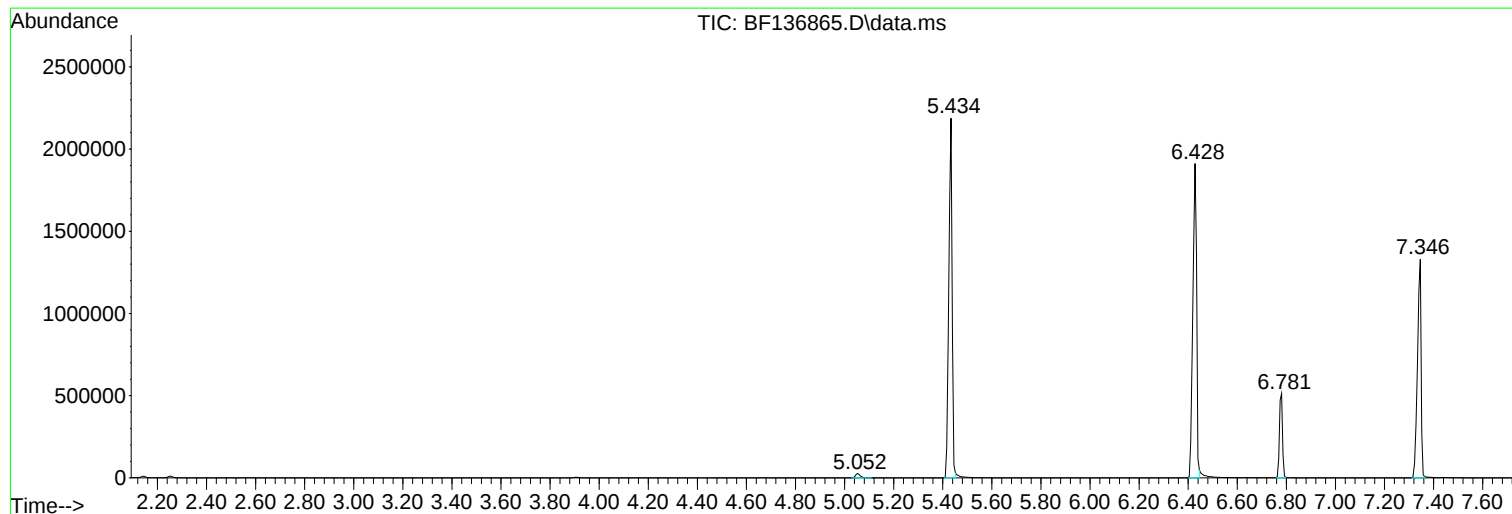

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010224\
Data File : BF136865.D
Acq On : 02 Jan 2024 11:52
Operator : CG\JU
Sample : PB158048TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158048TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010224\
Data File : BF136865.D
Acq On : 02 Jan 2024 11:52
Operator : CG\JU
Sample : PB158048TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158048TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------