
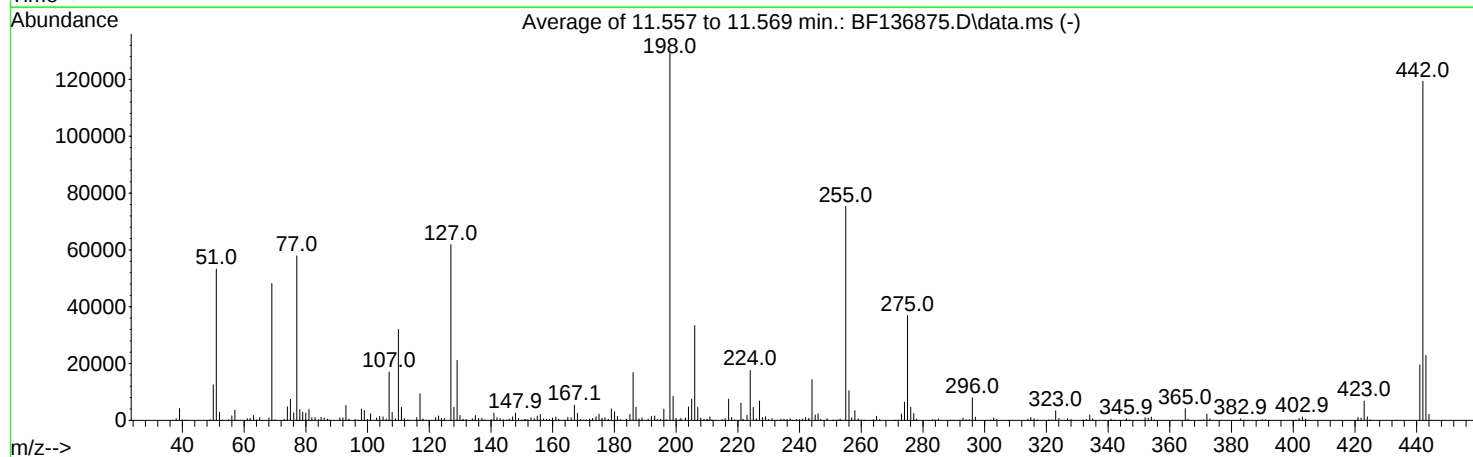


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010224\
Data File : BF136875.D
Acq On : 02 Jan 2024 17:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

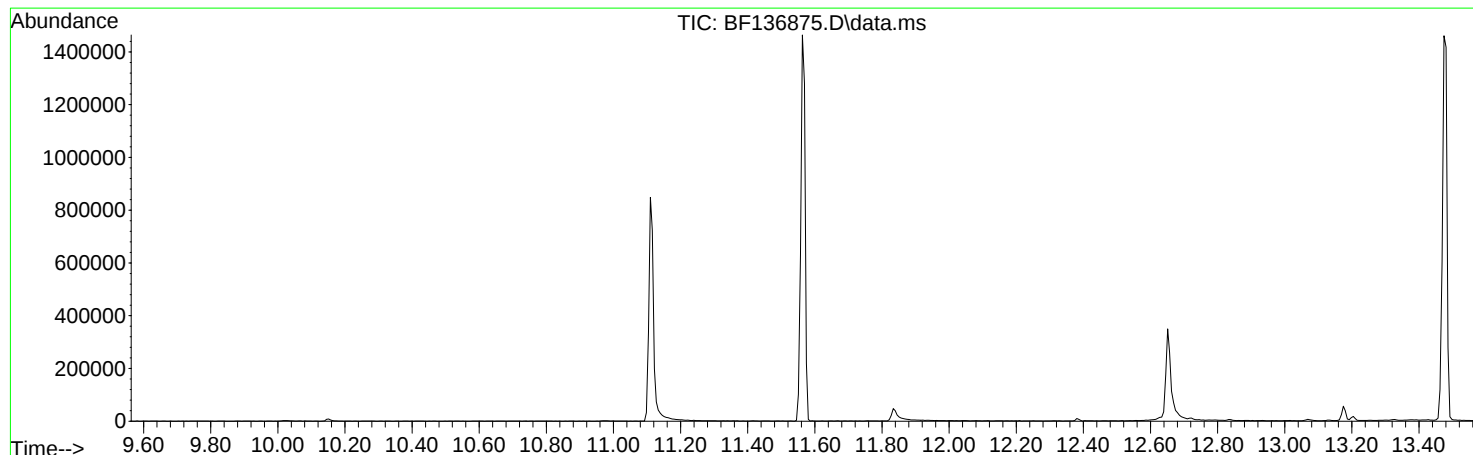




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	53264	PASS
68	69	0.00	2	1.6	792	PASS
69	198	0.00	100	37.2	48205	PASS
70	69	0.00	2	0.5	232	PASS
127	198	10	80	47.8	61856	PASS
197	198	0.00	2	0.2	204	PASS
198	198	100	100	100.0	129483	PASS
199	198	5	9	6.5	8438	PASS
275	198	10	60	28.5	36888	PASS
365	198	1	100	3.2	4157	PASS
441	198	0.01	100	15.1	19536	PASS
442	442	50	100	100.0	119323	PASS
443	442	15	24	19.2	22879	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010224\
Data File : BF136875.D
Acq On : 02 Jan 2024 17:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 03 01:51:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

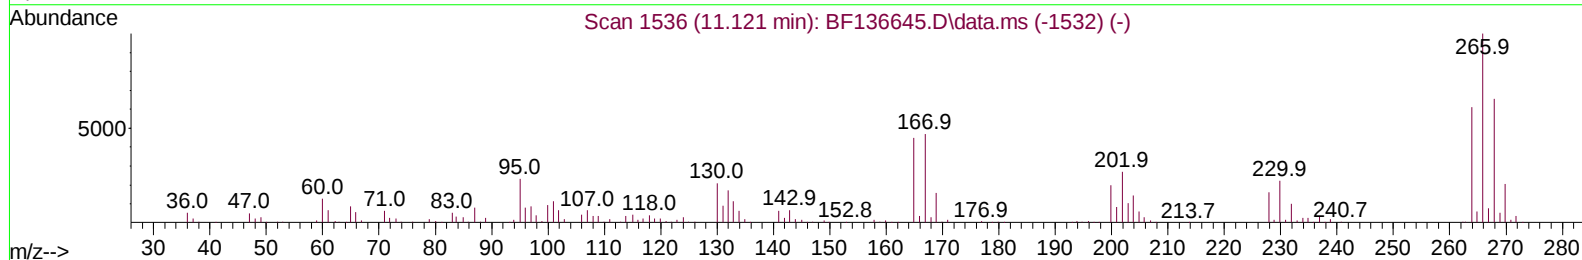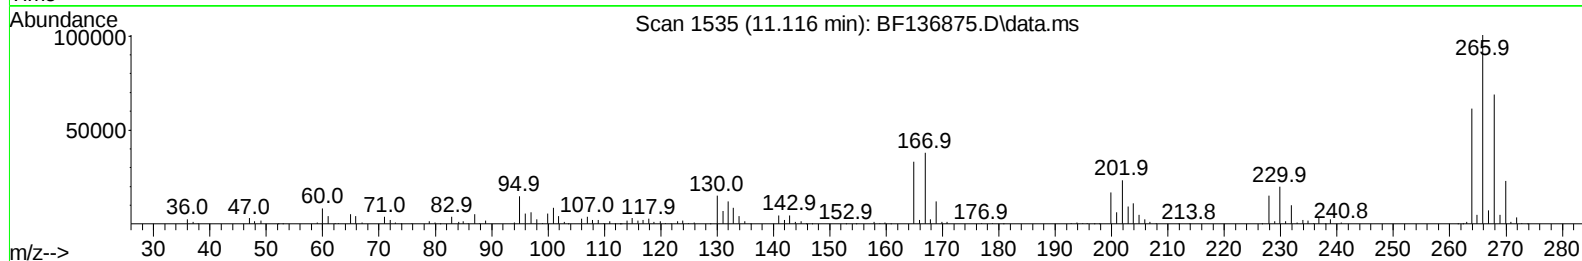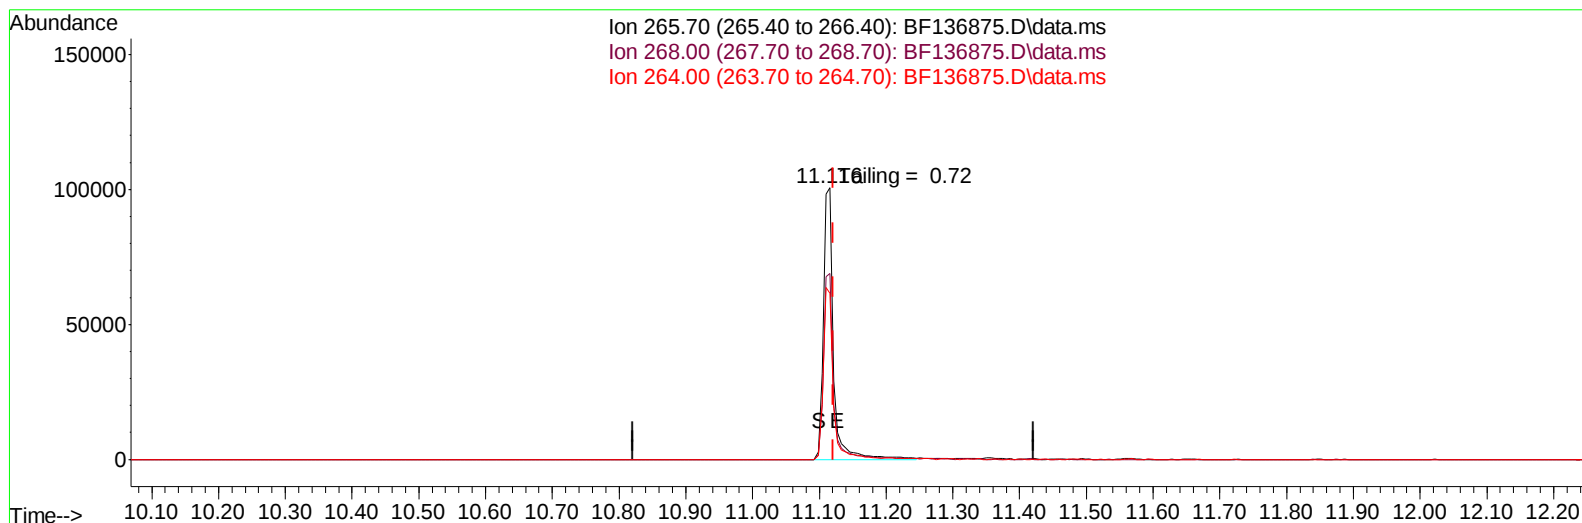

TIC: BF136875.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.006) 33469.73 ng




response 107352

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	68.47
264.00	61.20	61.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010224\
Data File : BF136875.D
Acq On : 02 Jan 2024 17:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 03 01:51:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

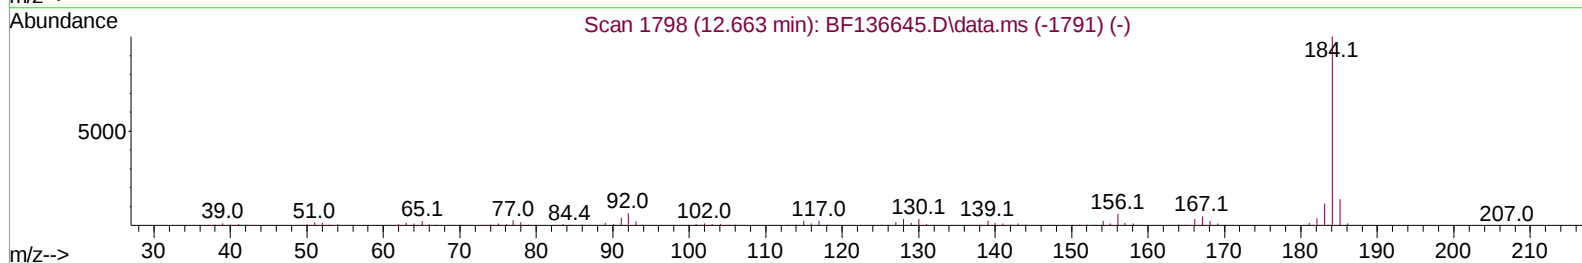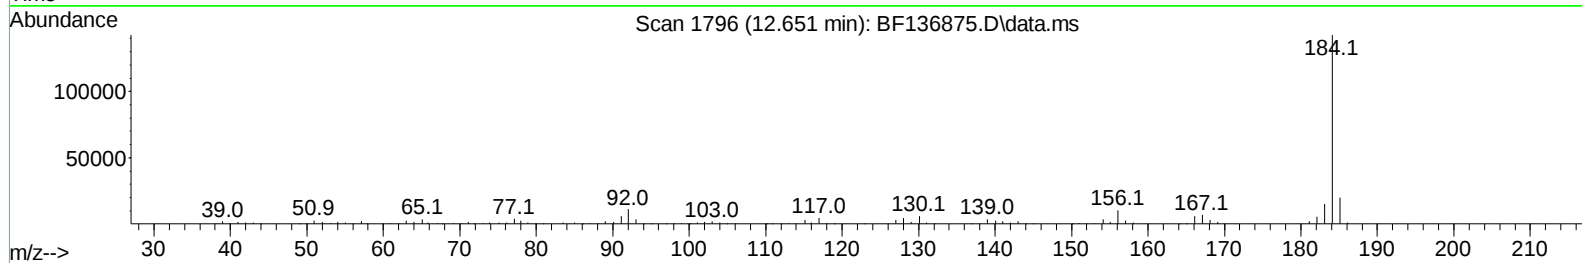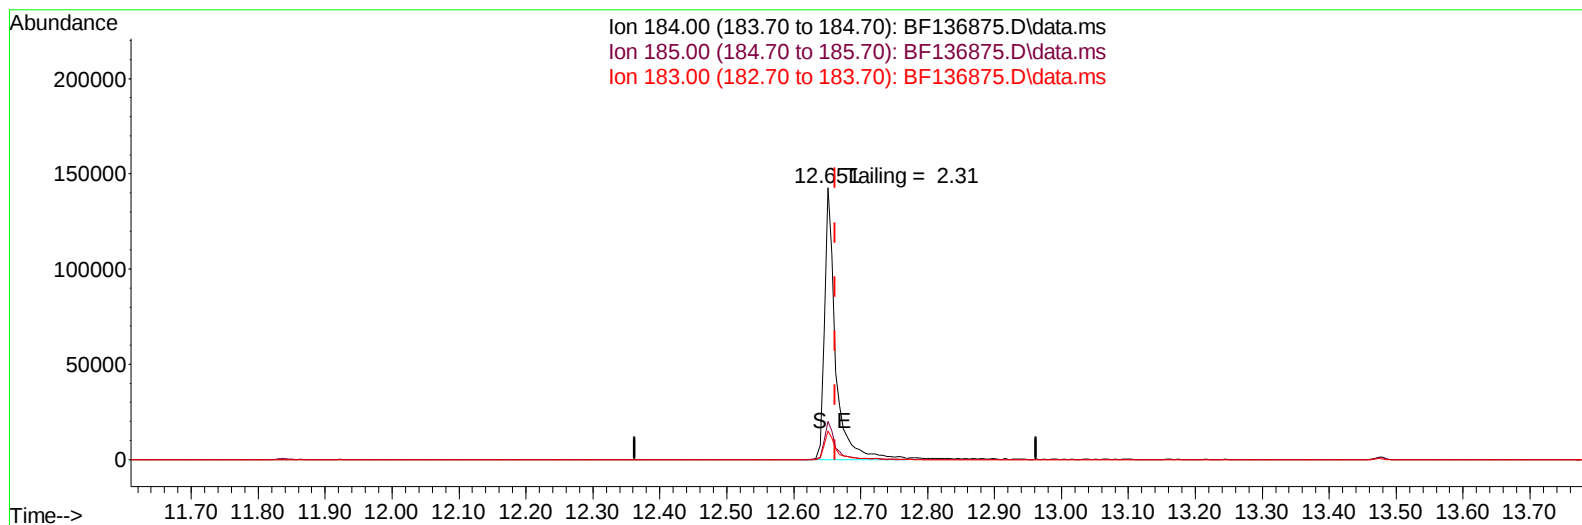

TIC: BF136875.D\data.ms

(77) Benzidine

12.651min (-0.012) 0.00 ng

response 166318

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.10
183.00	11.60	10.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/2/2024	BNA_F	<u>BF136875.D</u>
Compound Name	Response	Retention Time
DDT	290283	13.48
DDD	13065	13.175
DDE	574	12.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13639	303922	4.49

Instrument :
BNA_F
ClientSampleId :
DFTPP