
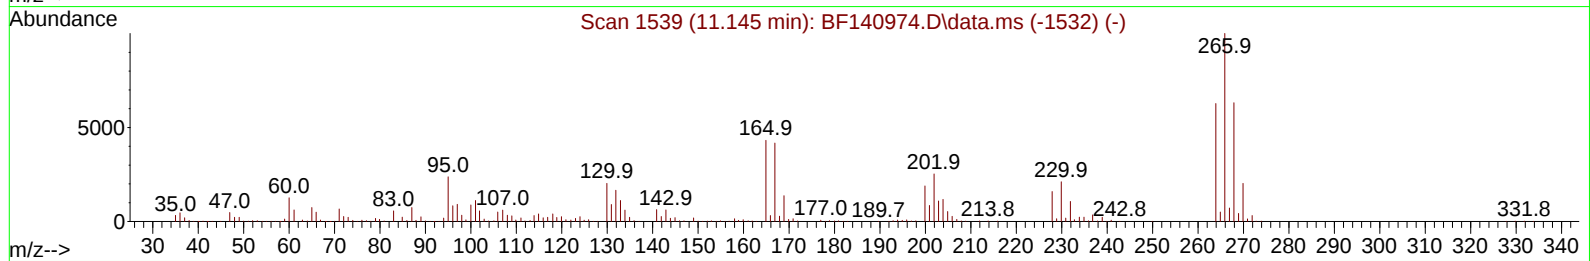
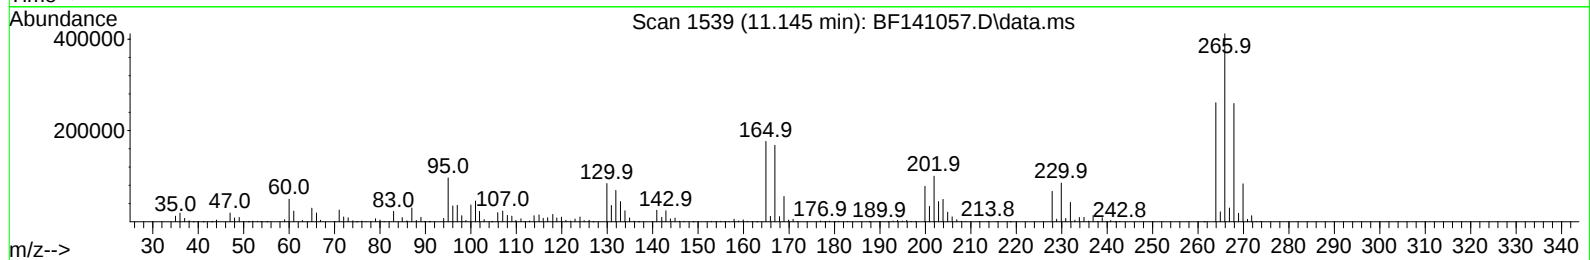


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010225\
Data File : BF141057.D
Acq On : 02 Jan 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 10:33:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

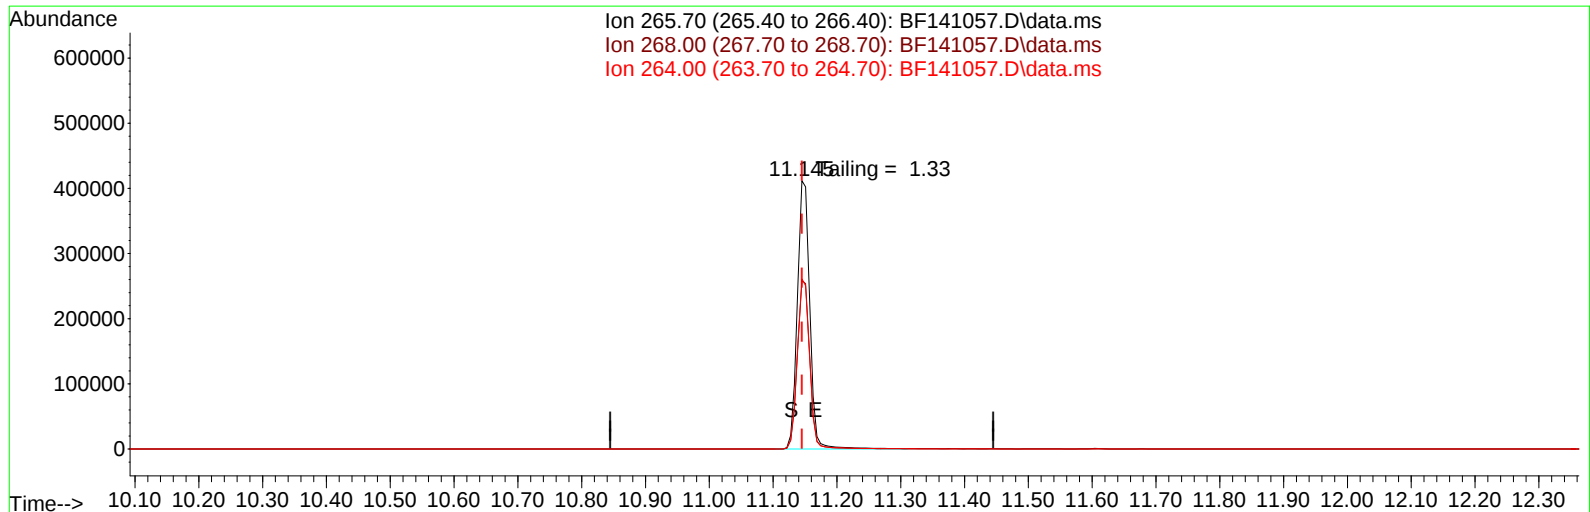

TIC: BF141057.D\data.ms

(70) Pentachlorophenol (C)




11.145min (+ 0.000) 172590.47 ng

response 561020

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.90
264.00	62.80	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010225\
Data File : BF141057.D
Acq On : 02 Jan 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 10:33:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

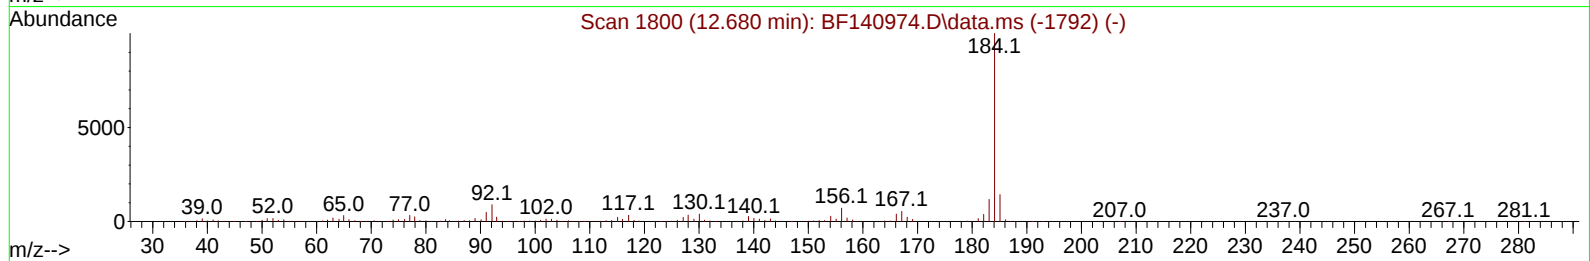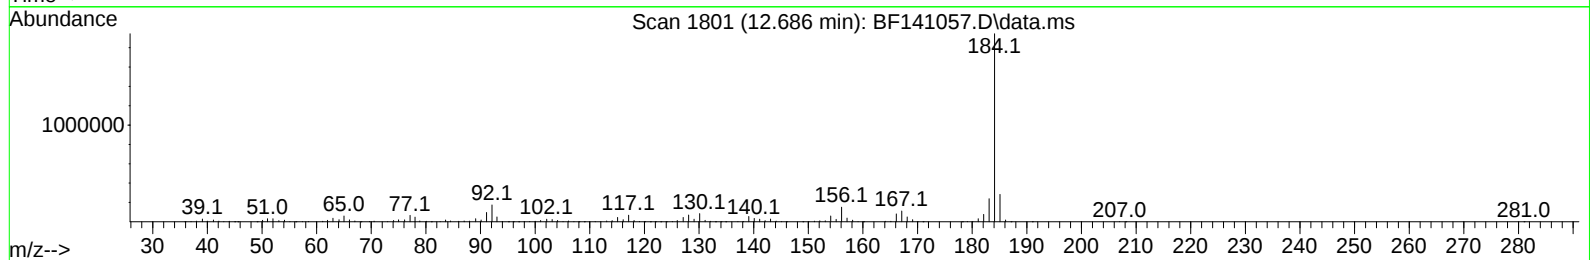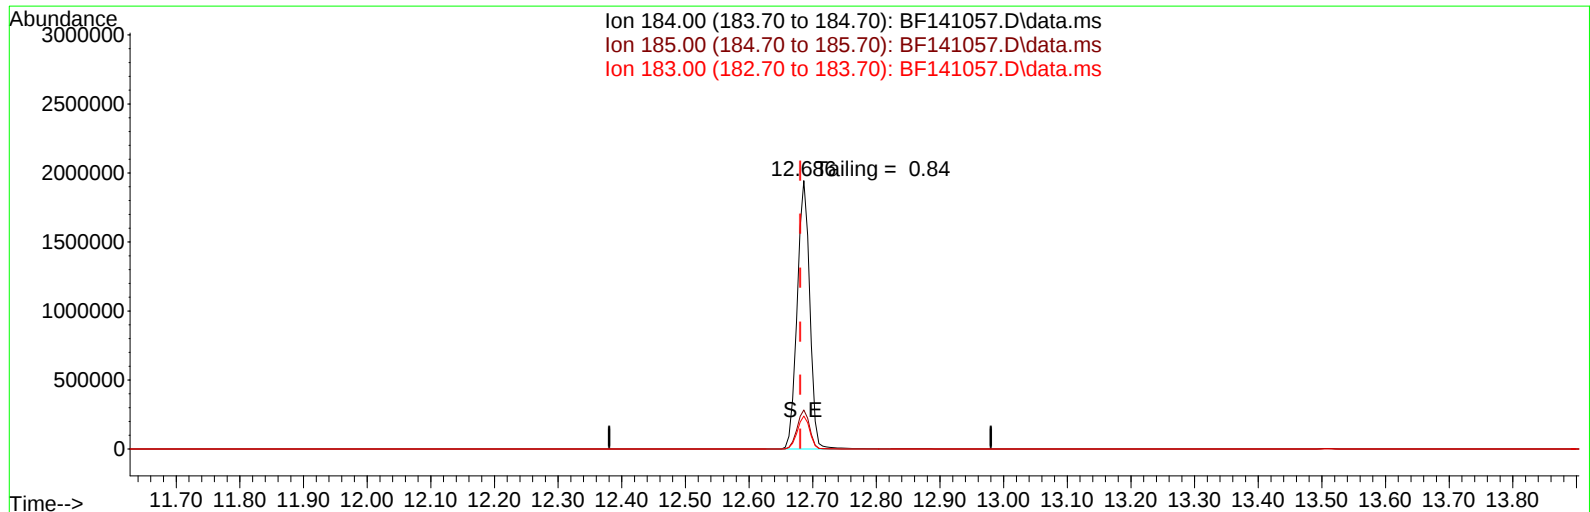

TIC: BF141057.D\data.ms

(77) Benzidine**12.686min (+ 0.006) 290659.11 ng****response 2684400**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.57
183.00	11.70	12.27
0.00	0.00	0.00