


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010225\
Data File : BF141057.D
Acq On : 02 Jan 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 27 00:31:16 2024

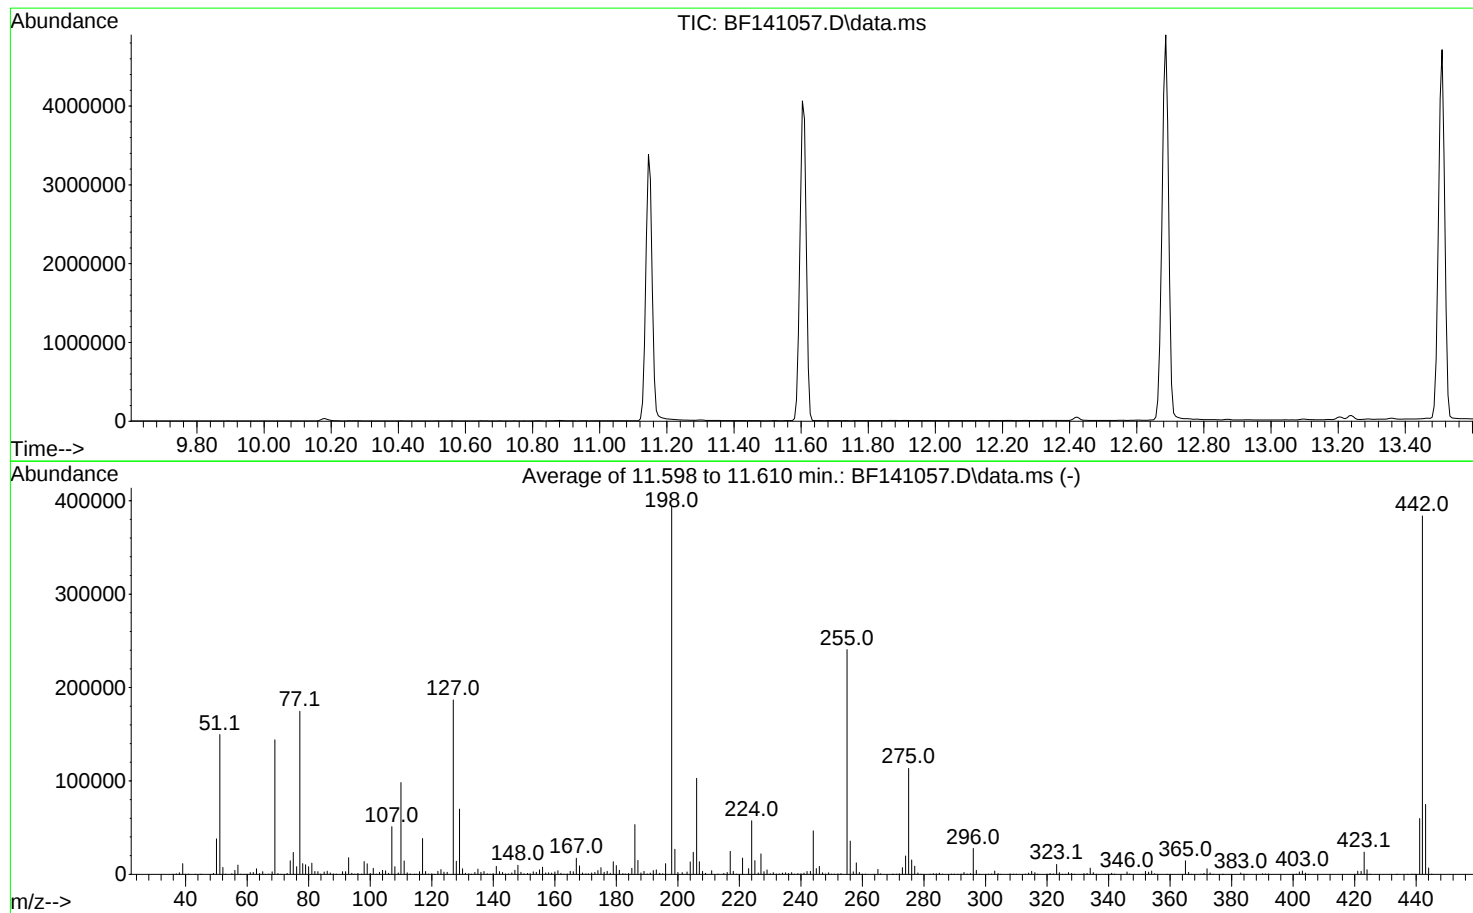

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	149696	PASS
68	69	0.00	2	1.9	2792	PASS
69	198	0.00	100	36.6	144016	PASS
70	69	0.00	2	0.6	826	PASS
127	198	10	80	47.4	186773	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	393792	PASS
199	198	5	9	6.8	26899	PASS
275	198	10	60	28.8	113405	PASS
365	198	1	100	3.7	14513	PASS
441	198	0.01	100	15.2	59736	PASS
442	442	50	100	100.0	383637	PASS
443	442	15	24	19.5	74931	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/2/2025	BNA_F	<u>BF141057.D</u>
Compound Name	Response	Retention Time
DDT	1175216	13.51
DDD	21206	13.239
DDE	1544	12.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22750	1197966	1.90

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010225\
Data File : BF141057.D
Acq On : 02 Jan 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 02 10:33:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

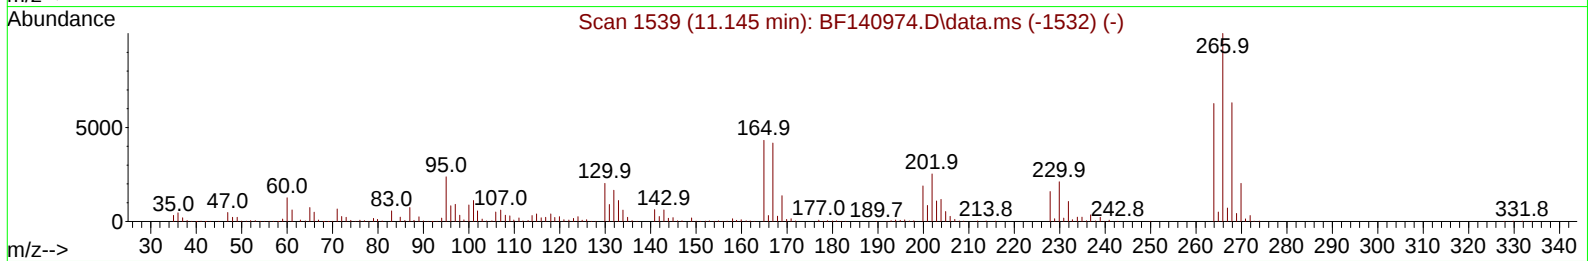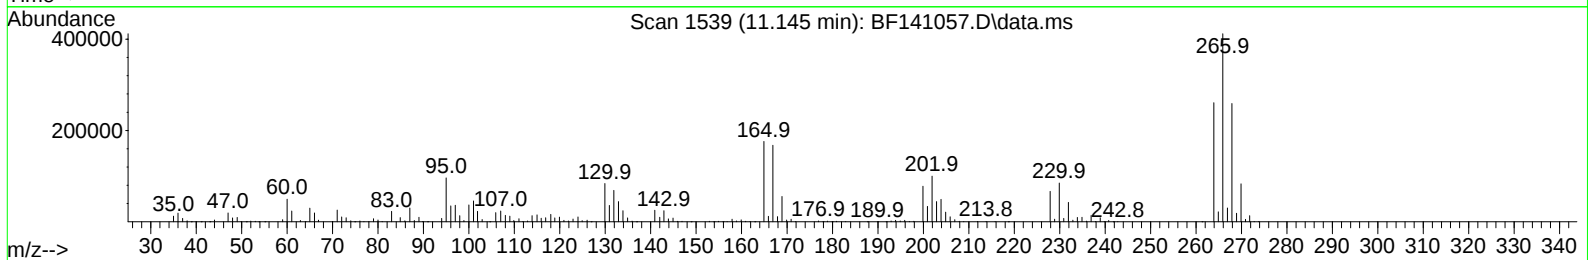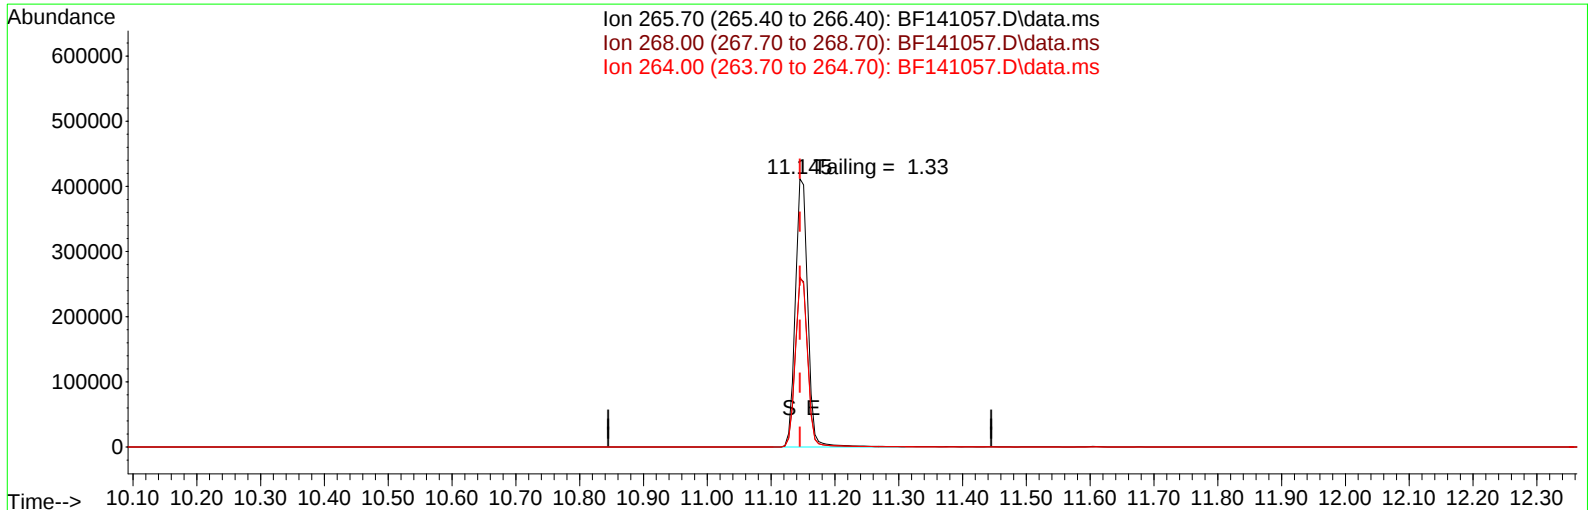

TIC: BF141057.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.000) 172590.47 ng




response 561020

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.90
264.00	62.80	63.38
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010225\  
Data File : BF141057.D  
Acq On    : 02 Jan 2025  09:07  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 02 10:33:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

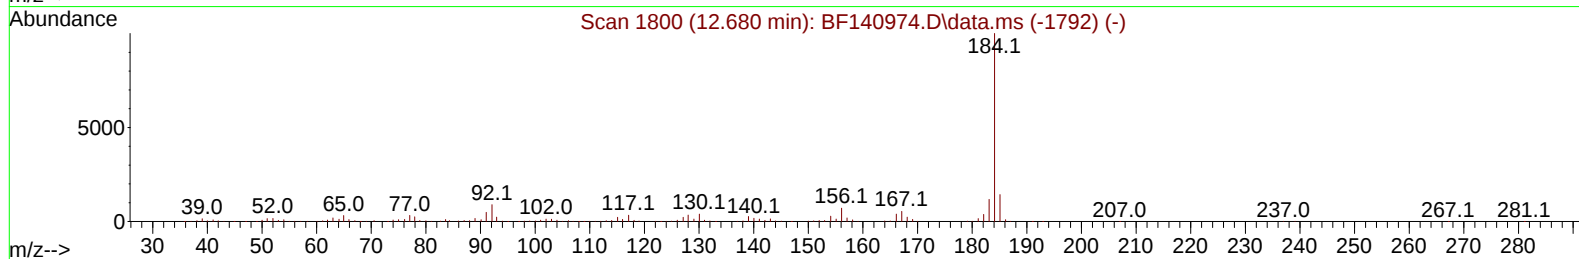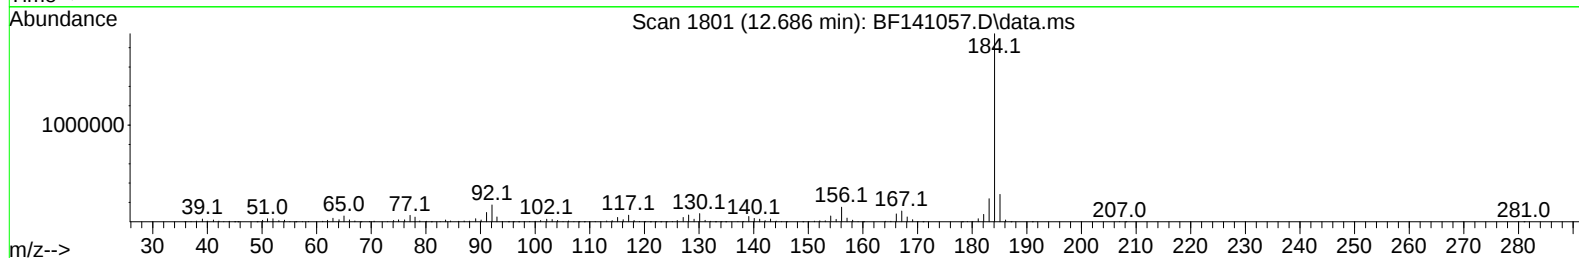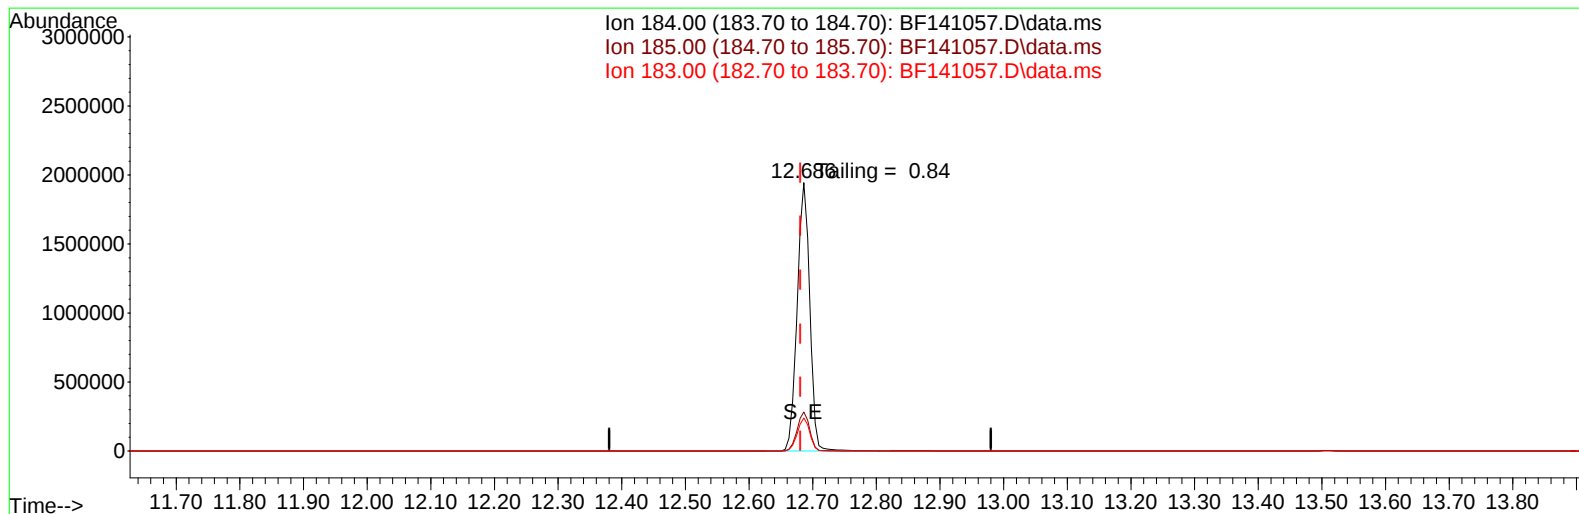

TIC: BF141057.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 290659.11 ng

```
response      2684400
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.57
183.00	11.70	12.27
0.00	0.00	0.00