
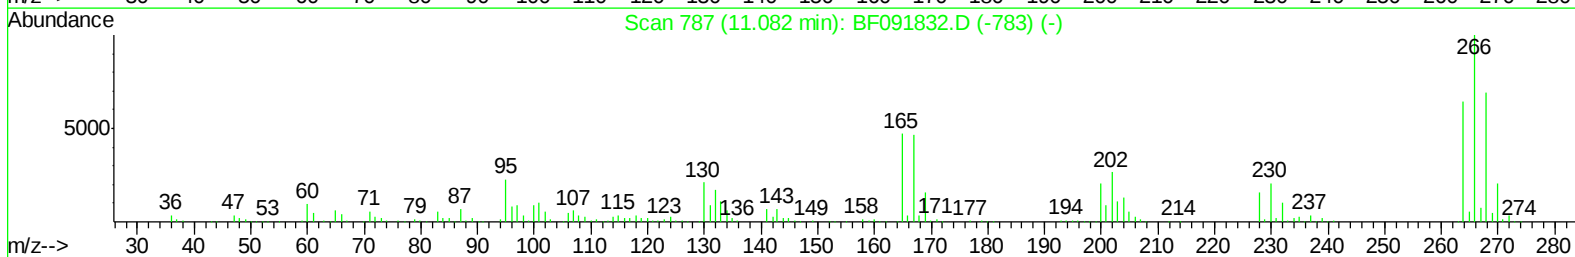
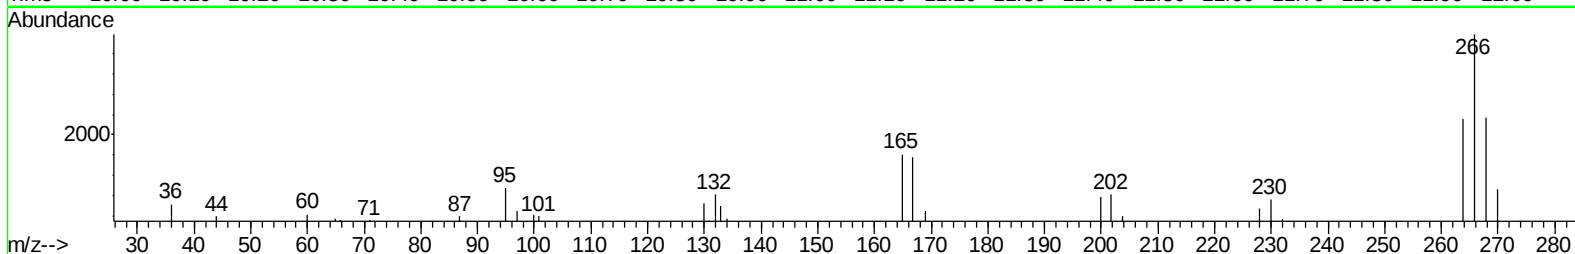


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010317\
Data File : BF092058.D
Acq On : 3 Jan 2017 13:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 03:45:06 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 17:32:10 2016
Response via : Initial Calibration

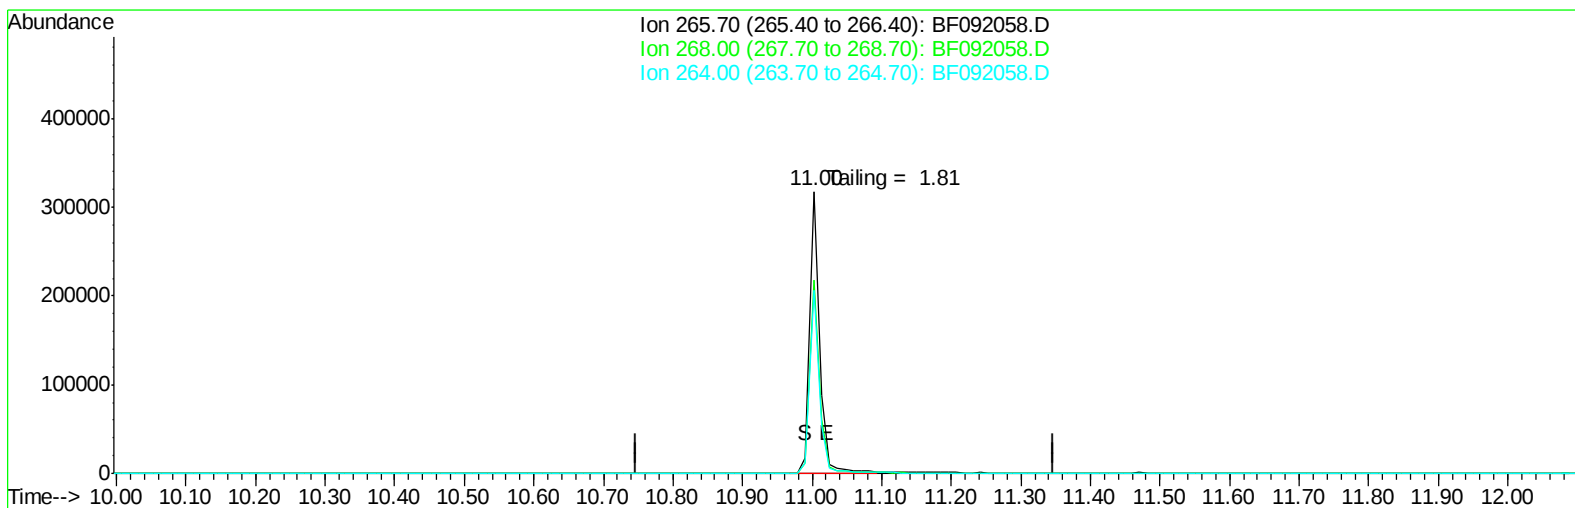

TIC: BF092058.D

(69) Pentachlorophenol (C)




11.048min (-11.048) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	66.60	0.00#
264.00	62.90	0.00#
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010317\  
Data File : BF092058.D  
Acq On    : 3 Jan 2017 13:13  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Jan 04 03:45:06 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 17:32:10 2016
Response via : Initial Calibration

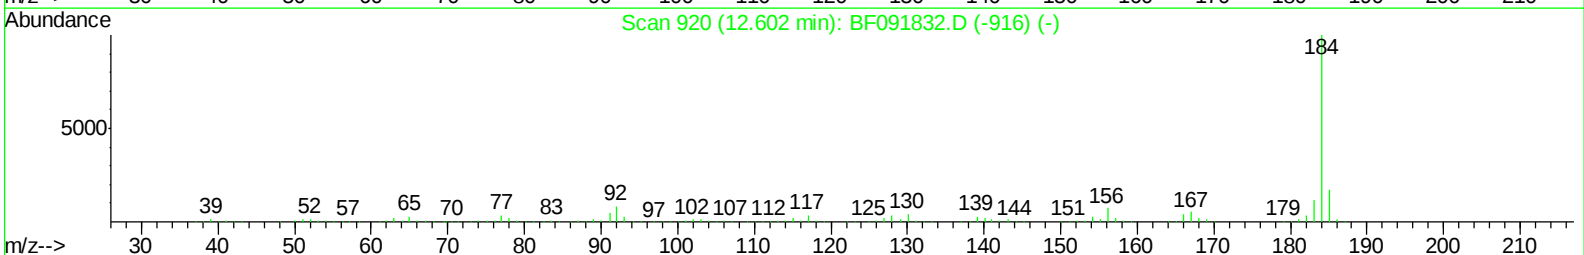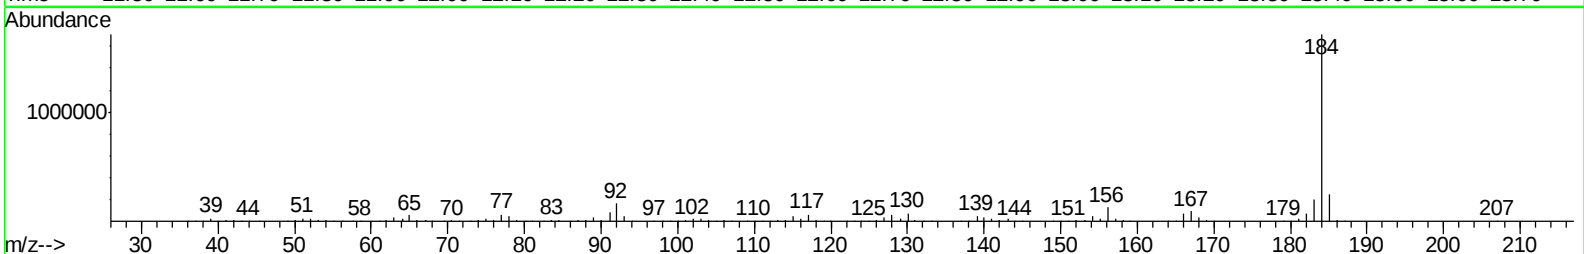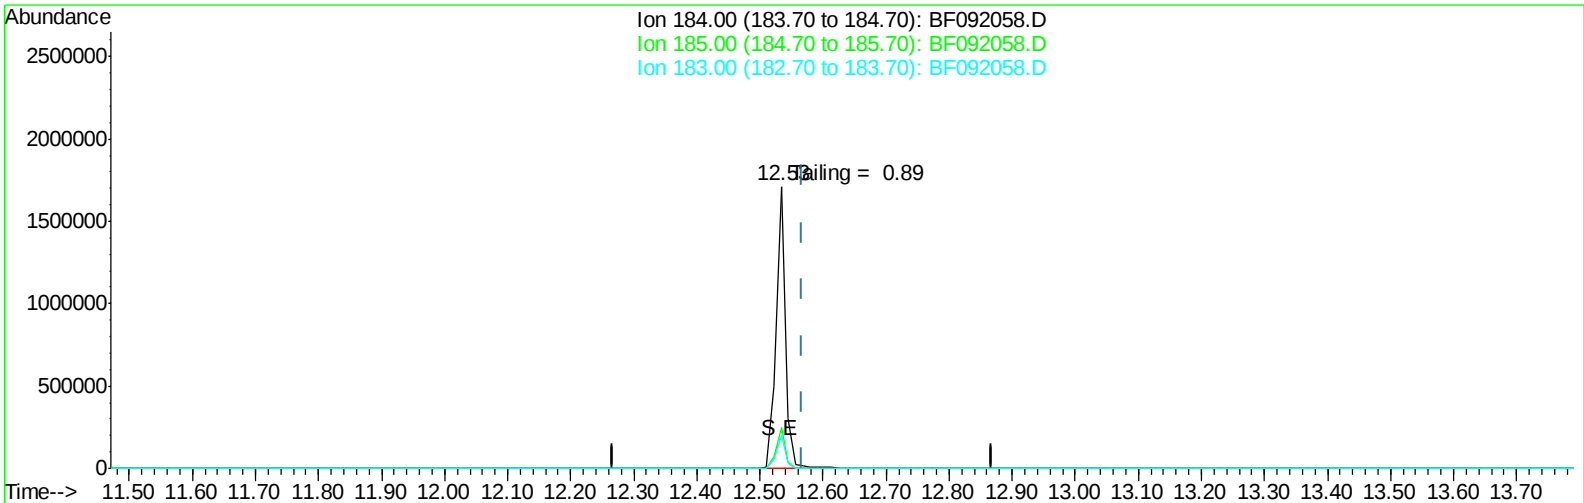

TIC: BF092058.D

(76) Benzidine

12.534min (-0.034) 0.00ng

response 1794347

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.75
183.00	11.50	11.69
0.00	0.00	0.00