


Data Path : Z:\HPCHEM1\BNA F\DATA\BF010317\
 Data File : BF092058.D
 Acq On : 3 Jan 2017 13:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 28 17:32:10 2016

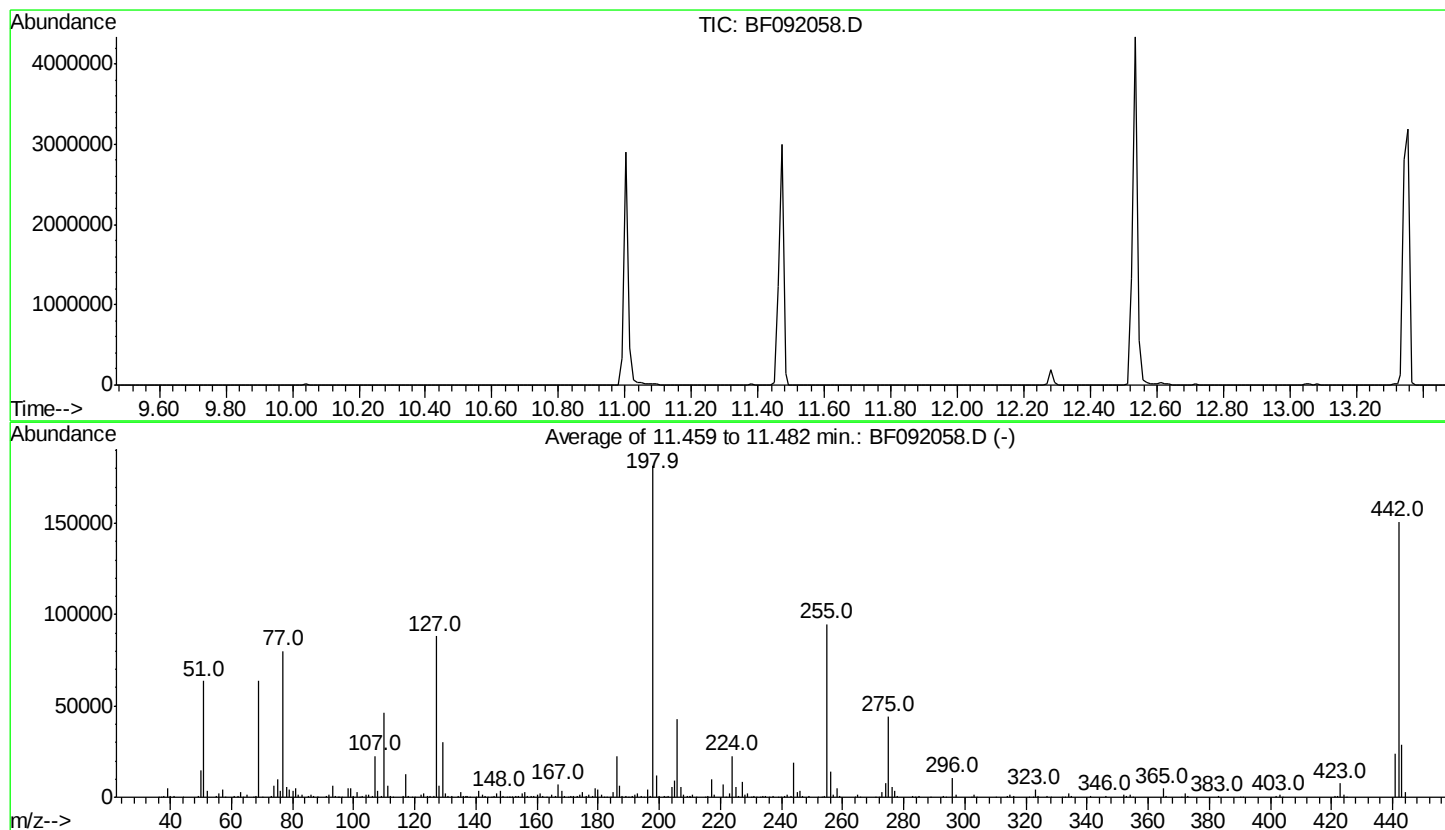

AutoFind: Scans 820, 821, 822; Background Corrected with Scan 816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	63580	PASS
68	69	0.00	2	1.5	962	PASS
69	198	0.00	100	35.3	64027	PASS
70	69	0.00	2	0.6	373	PASS
127	198	10	80	48.6	88290	PASS
197	198	0.00	2	0.5	928	PASS
198	198	100	100	100.0	181610	PASS
199	198	5	9	6.8	12272	PASS
275	198	10	60	24.2	43909	PASS
365	198	1	100	2.6	4691	PASS
441	442	0.01	24	15.7	23630	PASS
442	198	50	100	83.0	150797	PASS
443	442	15	24	18.9	28511	PASS