
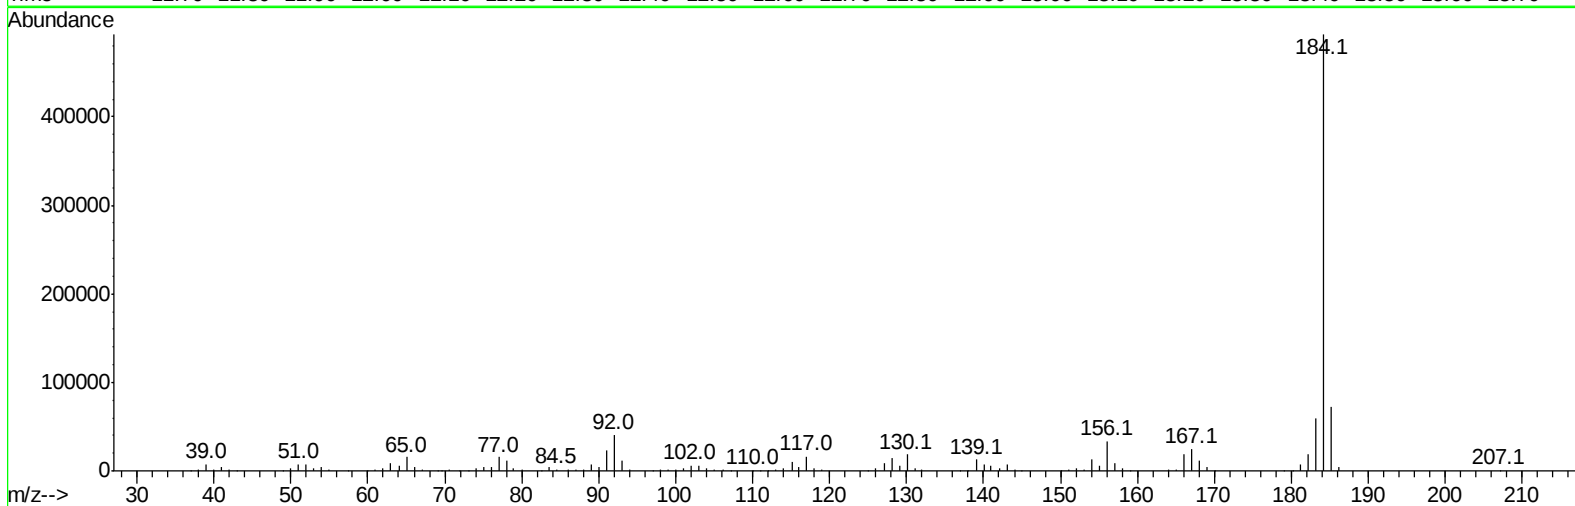


Data Path : Z:\HPCHEM1\BNA F\Data\BF010318\
Data File : BF101854.D
Acq On : 3 Jan 2018 11:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 08:42:47 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 13:21:45 2017
Response via : Initial Calibration

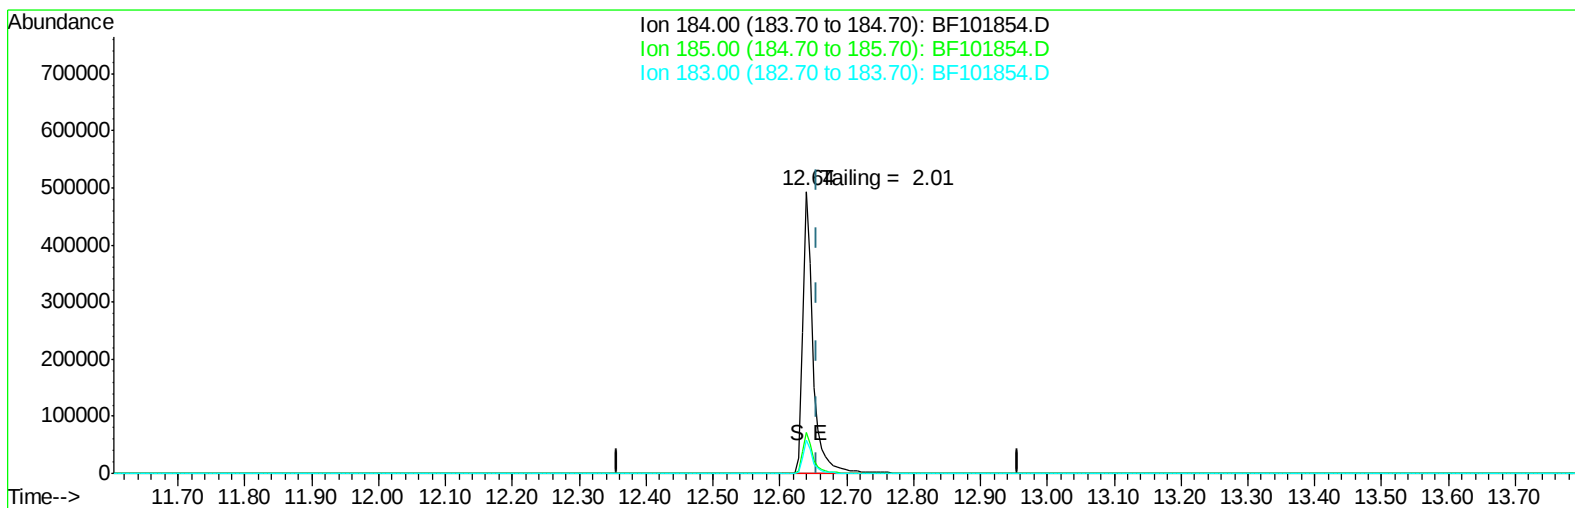

TIC: BF101854.D

(76) Benzidine



12.639min (-0.017) 17085.94ng

response 538334

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.74
183.00	11.60	11.95
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF010318\
Data File : BF101854.D
Acq On : 3 Jan 2018 11:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 08:42:47 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 13:21:45 2017
Response via : Initial Calibration

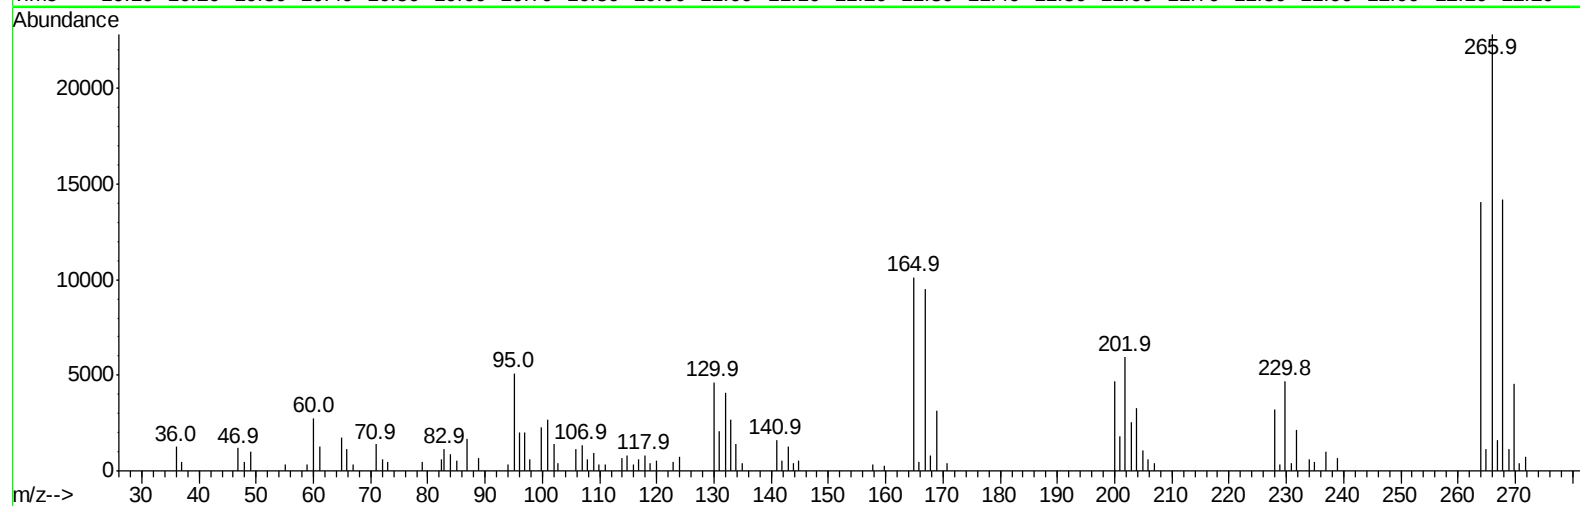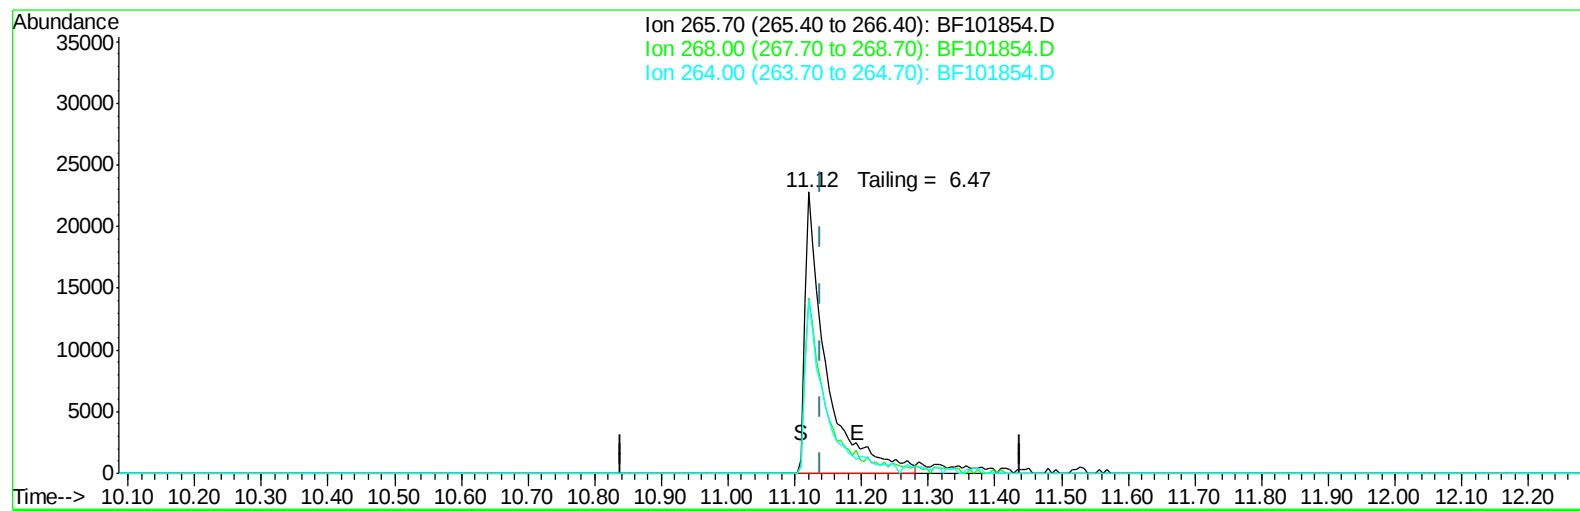

TIC: BF101854.D

(69) Pentachlorophenol (C)

11.122min (-0.017) 27602.77ng

response 49628

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.32
264.00	61.90	61.60
0.00	0.00	0.00