


Data Path : Z:\HPCHEM1\BNA F\Data\BF010318\
Data File : BF101880.D
Acq On : 4 Jan 2018 1:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 08:44:27 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 13:21:45 2017
Response via : Initial Calibration

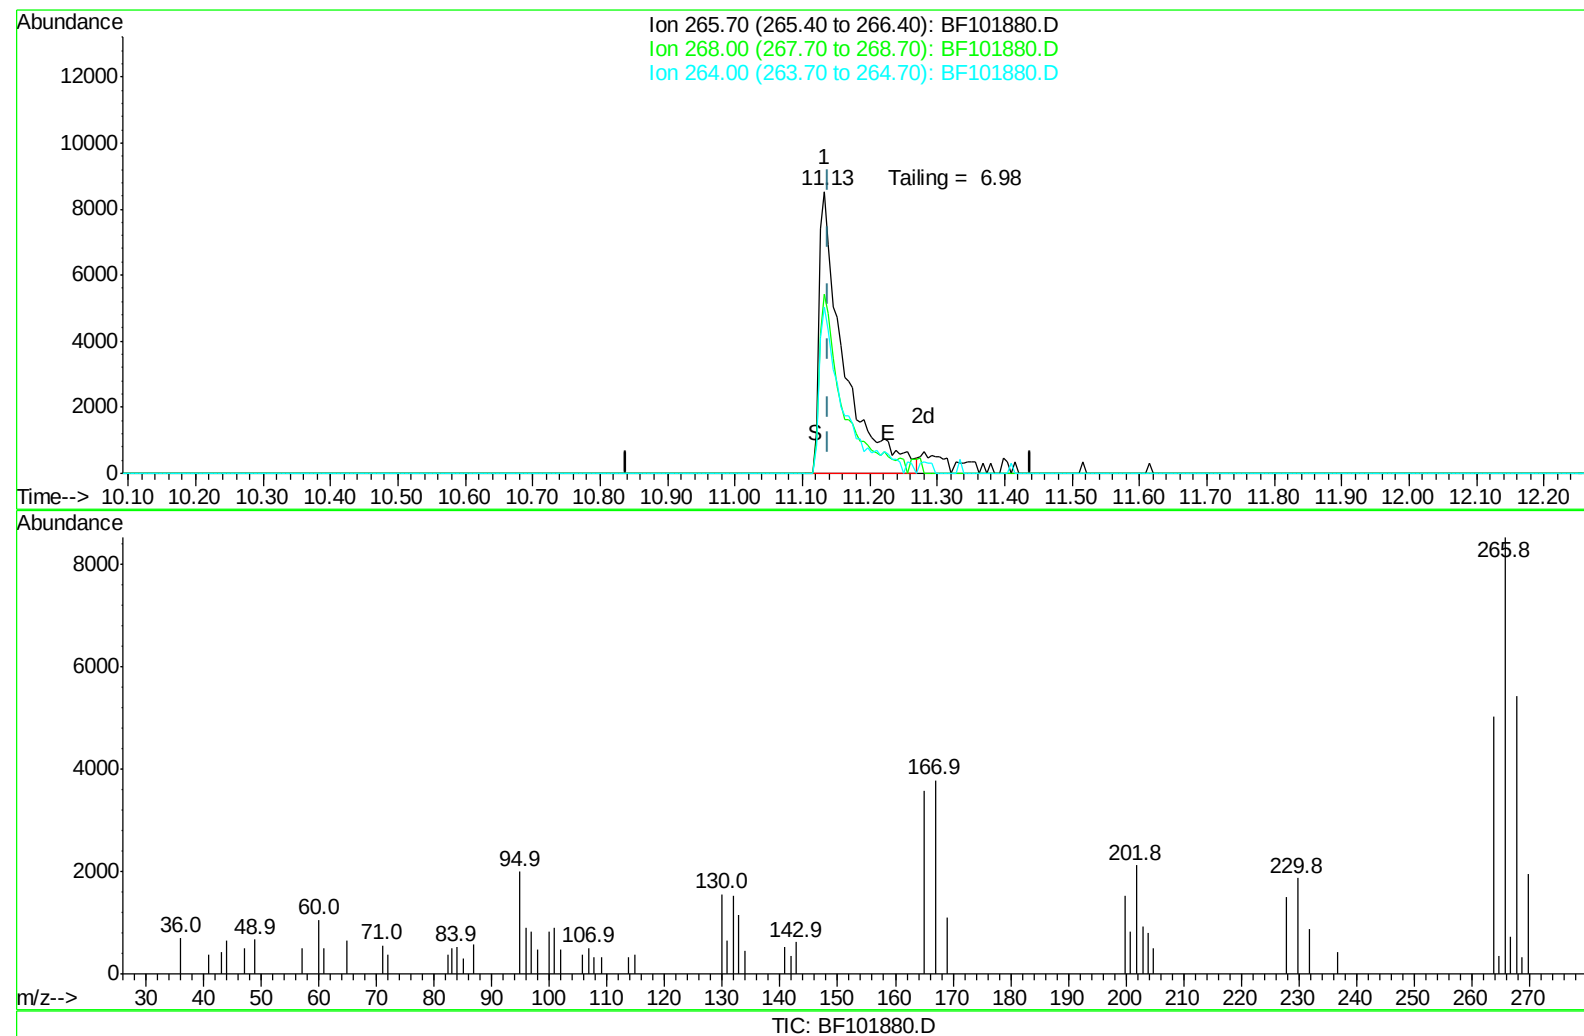

(69) Pentachlorophenol (C)



11.133min (-0.006) 0.00ng

response 21461

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.68
264.00	61.90	59.06
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF010318\
Data File : BF101880.D
Acq On : 4 Jan 2018 1:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 08:44:27 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 13:21:45 2017
Response via : Initial Calibration

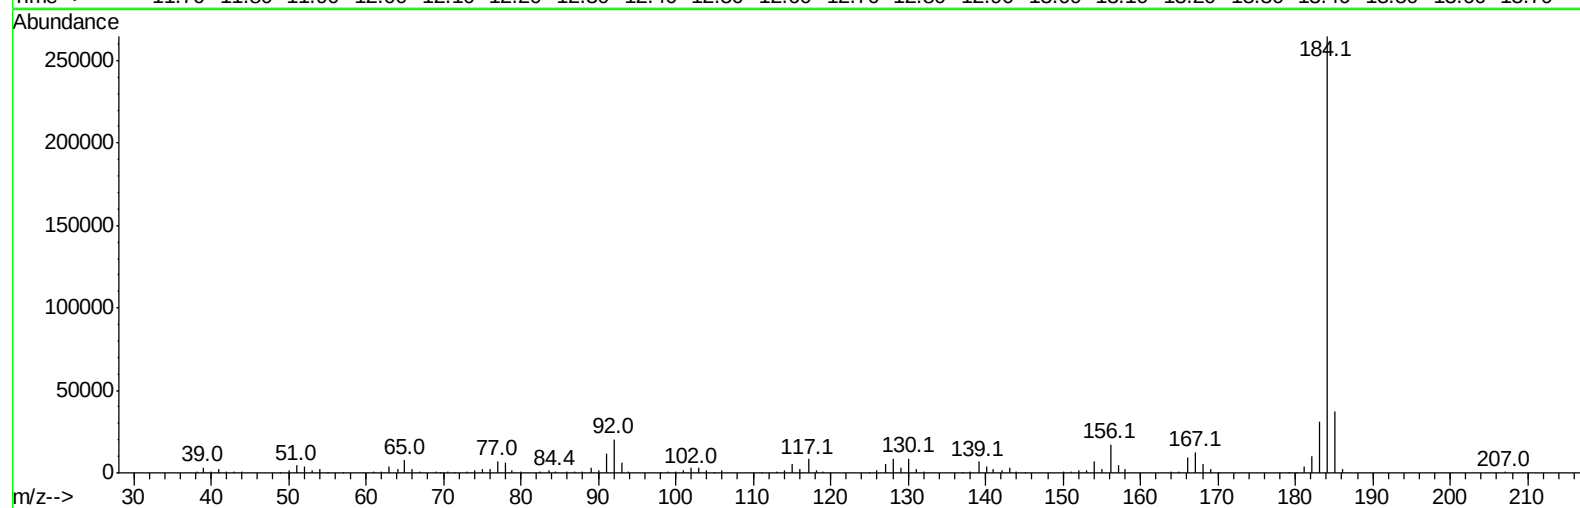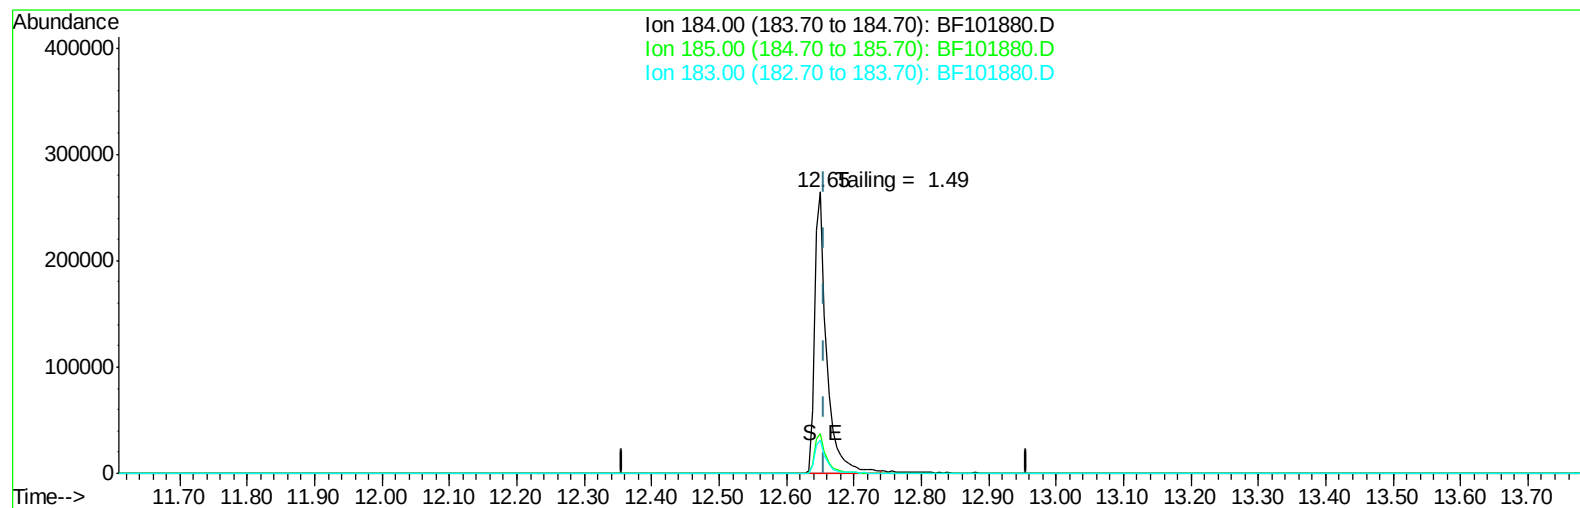

TIC: BF101880.D

(76) Benzidine

12.651min (-0.006) 55262.86ng

response 324431

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.01
183.00	11.60	11.64
0.00	0.00	0.00