


Data Path : Z:\HPCHEM1\BNA_F\Data\BF010318\
 Data File : BF101880.D
 Acq On : 4 Jan 2018 1:21
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 29 13:21:45 2017

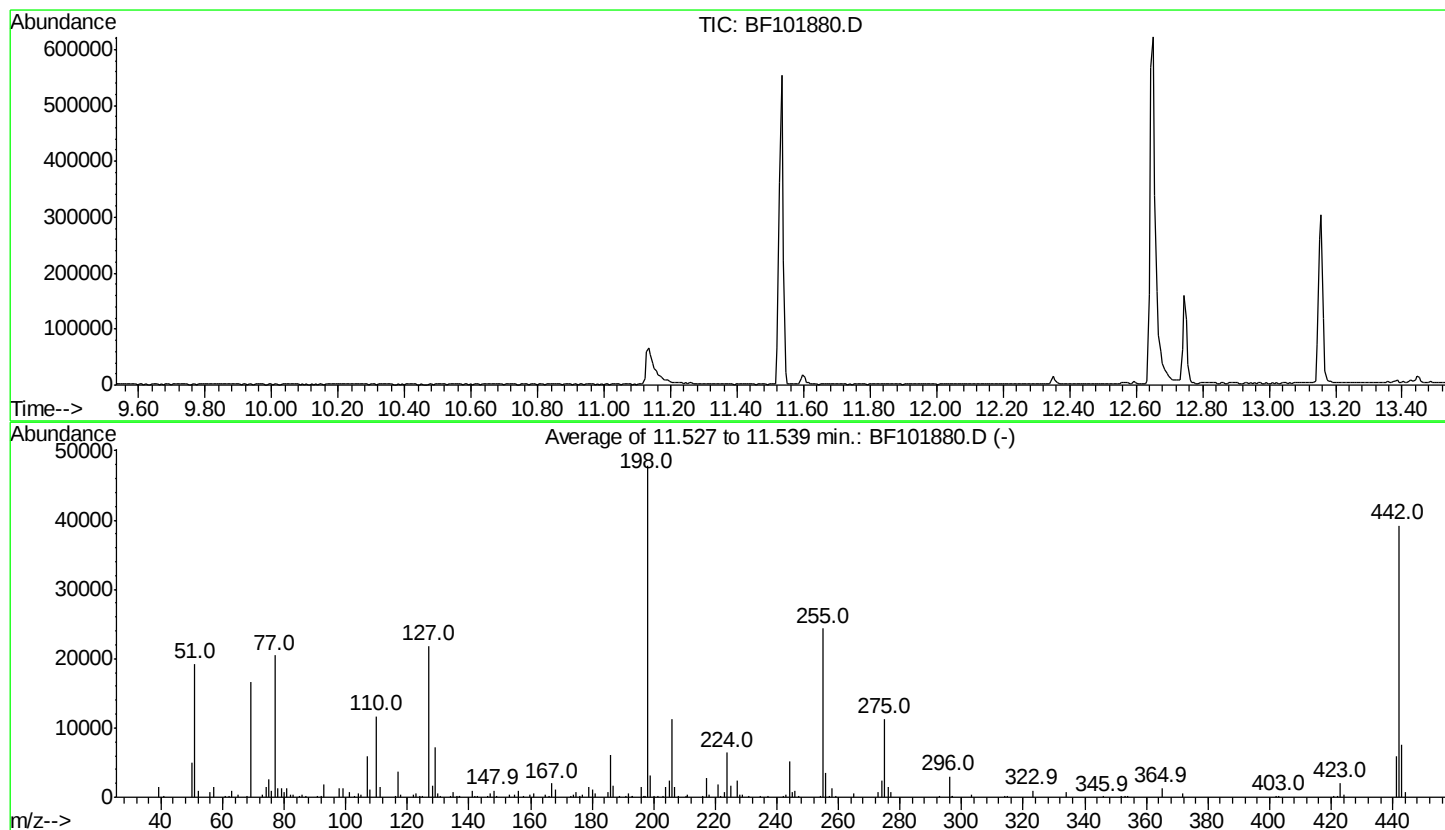

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	19227	PASS
68	69	0.00	2	1.5	244	PASS
69	198	0.00	100	34.8	16675	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.7	21878	PASS
197	198	0.00	2	0.4	192	PASS
198	198	100	100	100.0	47864	PASS
199	198	5	9	6.5	3133	PASS
275	198	10	60	23.6	11290	PASS
365	198	1	100	2.7	1305	PASS
441	443	0.01	100	77.1	5866	PASS
442	198	50	100	82.0	39240	PASS
443	442	15	24	19.4	7609	PASS