
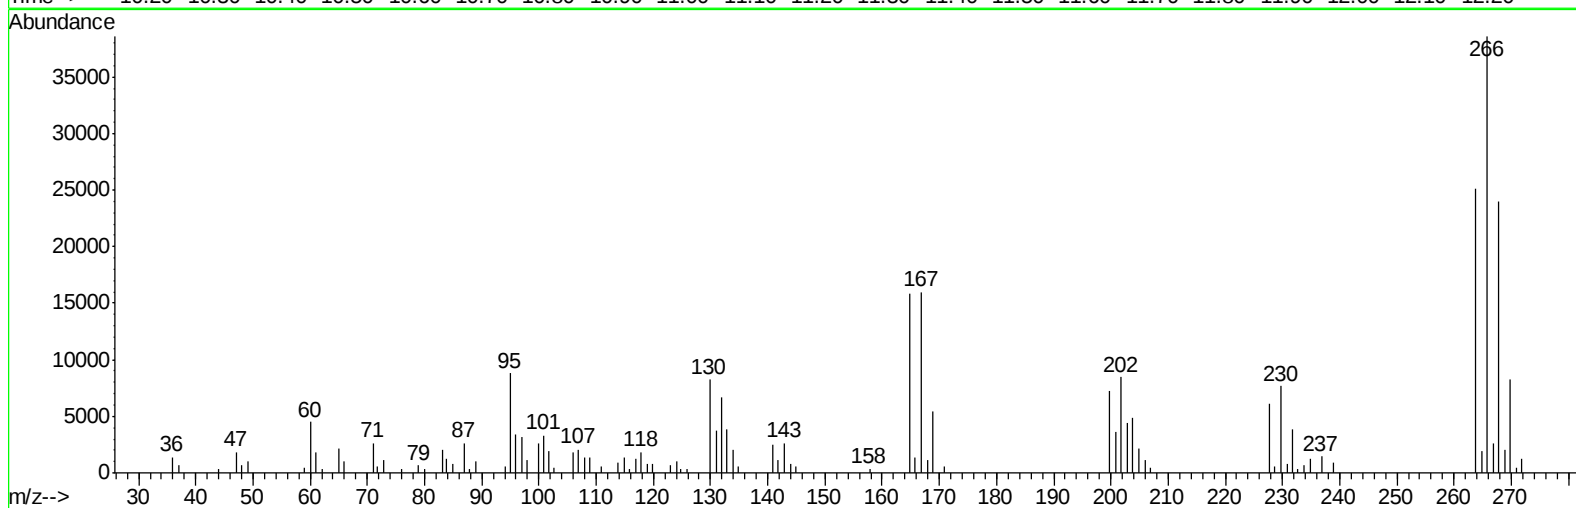


Data File : BF118462.D
Acq On : 3 Jan 2020 16:19
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 01:42:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 15:58:52 2019
Response via : Initial Calibration

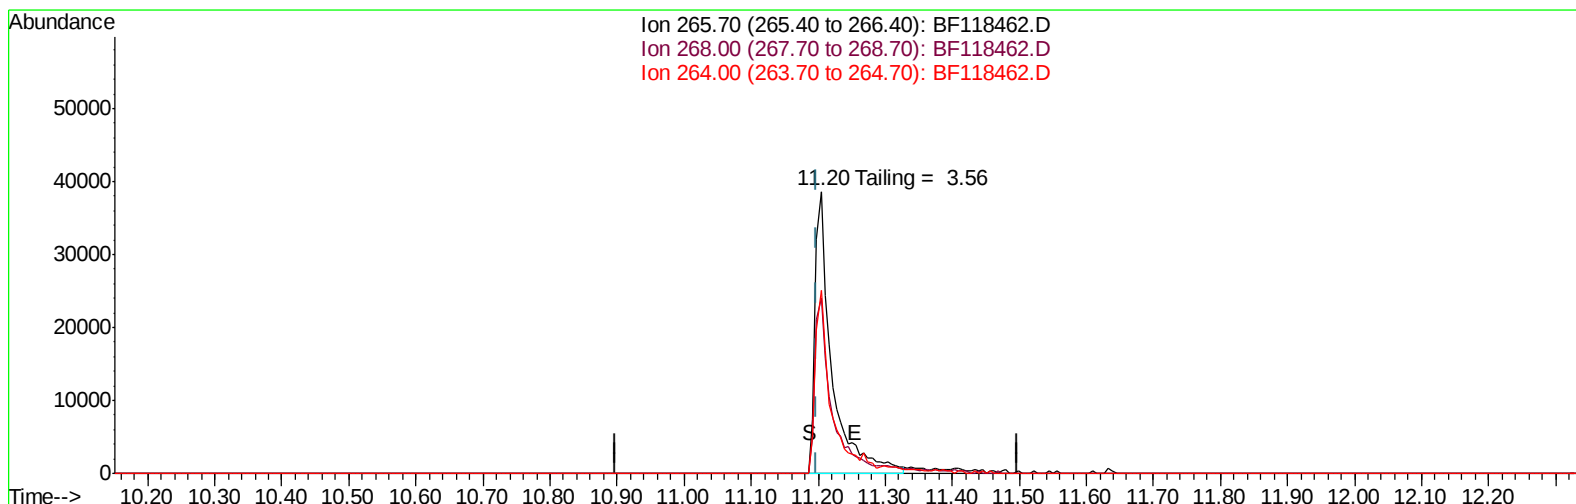

TIC: BF118462.D

(70) Pentachlorophenol (C)



11.204min (+0.006) 21508.76ng

response 65442

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	62.31
264.00	62.40	65.04
0.00	0.00	0.00

Data File : BF118462.D
Acq On : 3 Jan 2020 16:19
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 01:42:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 15:58:52 2019
Response via : Initial Calibration

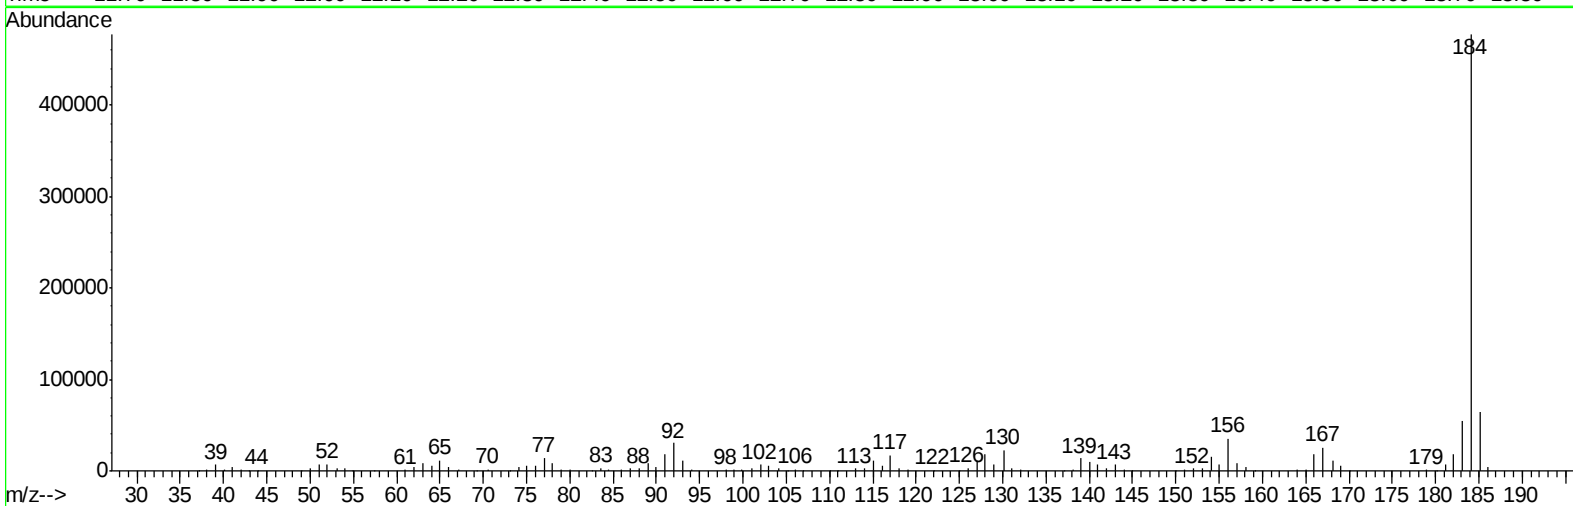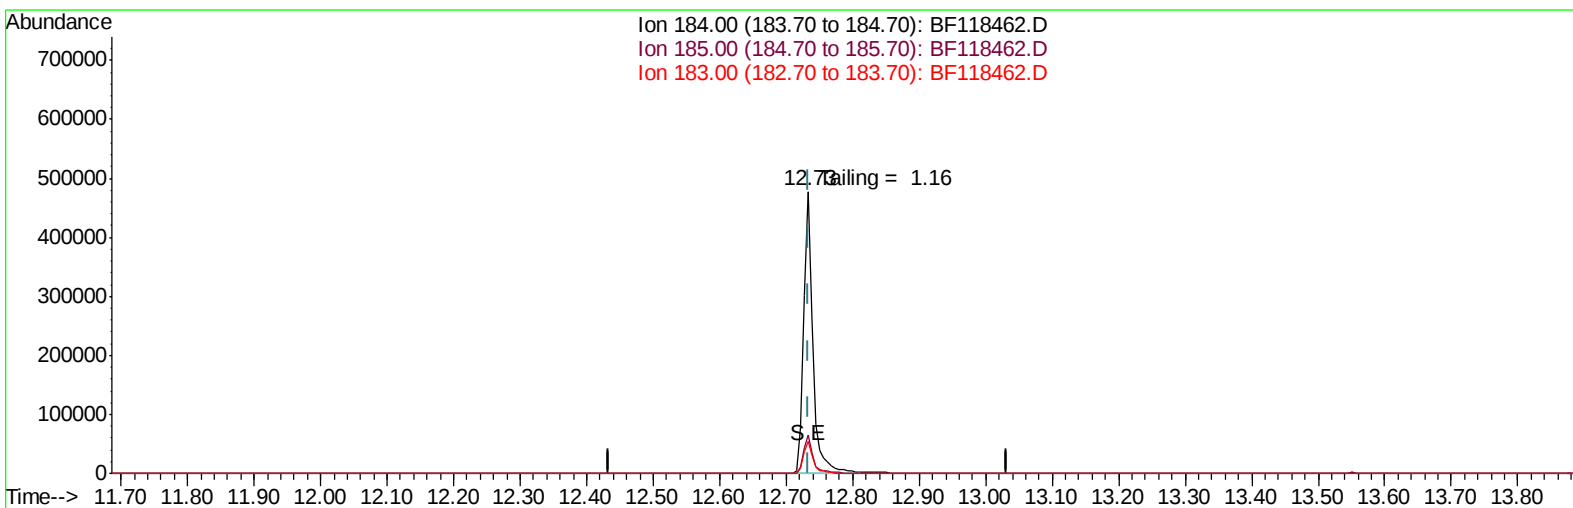

TIC: BF118462.D

(77) Benzidine

12.733min (-0.000) 0.00ng m

response 472096

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	13.64
183.00	11.80	11.50
0.00	0.00	0.00