


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010320\
 Data File : BF118454.D
 Acq On : 3 Jan 2020 11:40
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 15:58:52 2019

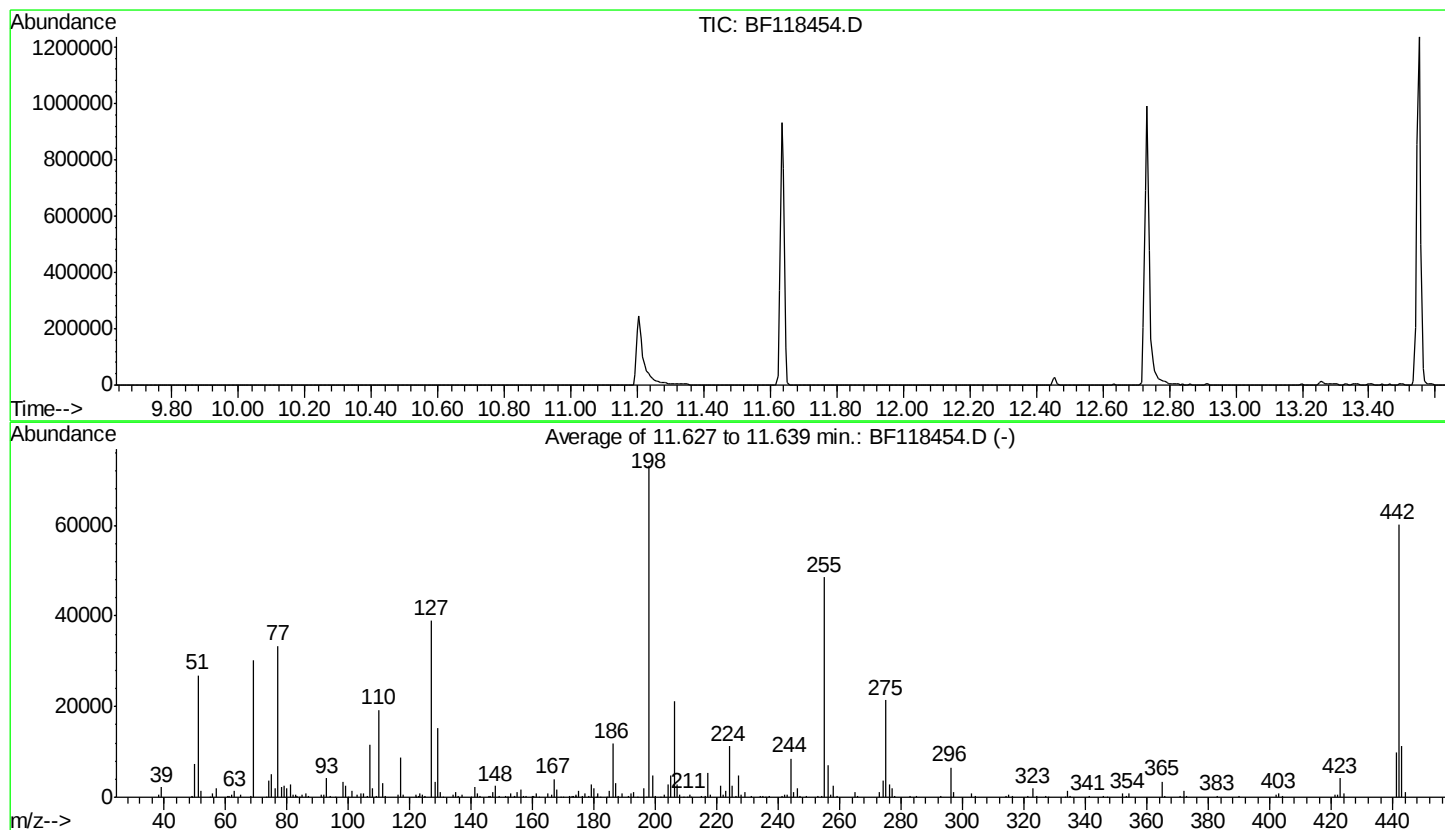

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	26877	PASS
68	69	0.00	2	1.3	407	PASS
69	198	0.00	100	41.2	30162	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.3	38984	PASS
197	198	0.00	2	0.2	133	PASS
198	198	100	100	100.0	73192	PASS
199	198	5	9	6.7	4929	PASS
275	198	10	60	29.3	21475	PASS
365	198	1	100	4.8	3480	PASS
441	198	0.01	100	13.4	9818	PASS
442	198	50	100	82.2	60181	PASS
443	442	15	24	18.7	11240	PASS