


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010320\
 Data File : BF118462.D
 Acq On : 3 Jan 2020 16:19
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 15:58:52 2019

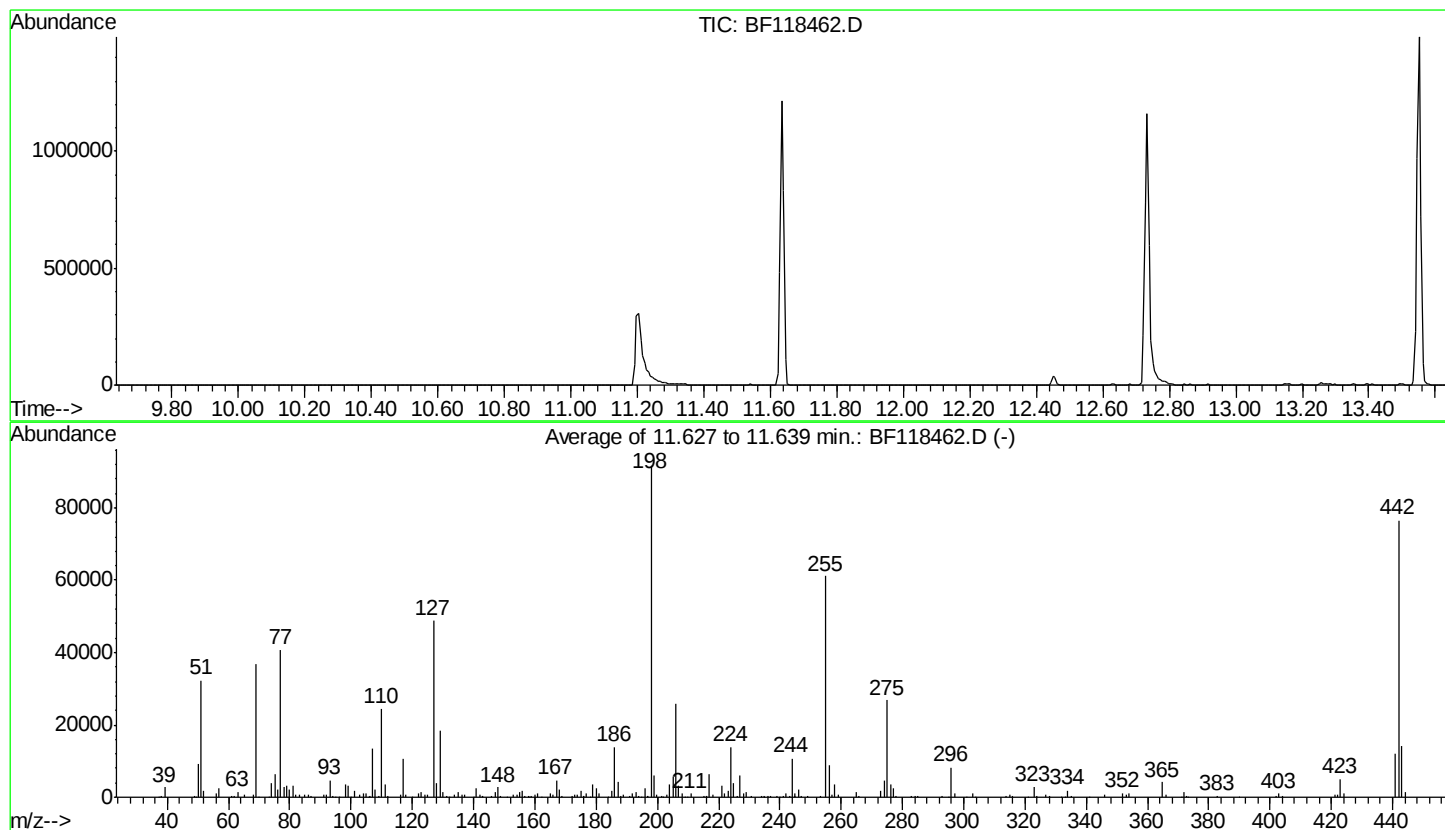

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	32376	PASS
68	69	0.00	2	1.9	704	PASS
69	198	0.00	100	40.2	36829	PASS
70	69	0.00	2	0.4	149	PASS
127	198	10	80	53.2	48744	PASS
197	198	0.00	2	0.4	411	PASS
198	198	100	100	100.0	91653	PASS
199	198	5	9	6.4	5908	PASS
275	198	10	60	29.2	26774	PASS
365	198	1	100	4.5	4094	PASS
441	198	0.01	100	13.1	12050	PASS
442	198	50	100	83.5	76504	PASS
443	442	15	24	18.5	14154	PASS