

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
 Data File : BF136914.D
 Acq On : 03 Jan 2024 18:44
 Operator : CG\JU
 Sample : 05900-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jan 04 03:40:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.781	152	58828	20.000	ng	-0.01
21) Naphthalene-d8	8.057	136	230766	20.000	ng	-0.01
39) Acenaphthene-d10	9.810	164	118856	20.000	ng	-0.02
64) Phenanthrene-d10	11.304	188	208246	20.000	ng	-0.01
76) Chrysene-d12	13.963	240	121379	20.000	ng	# 0.00
86) Perylene-d12	15.445	264	140198	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	376875	99.958	ng	0.00
7) Phenol-d6	6.434	99	481734	98.606	ng	0.00
23) Nitrobenzene-d5	7.345	82	302428	67.062	ng	-0.01
42) 2,4,6-Tribromophenol	10.610	330	130913	93.523	ng	-0.01
45) 2-Fluorobiphenyl	9.133	172	616674	69.783	ng	-0.02
79) Terphenyl-d14	12.898	244	507188	58.394	ng	-0.02
Target Compounds						Qvalue
19) n-Nitroso-di-n-propyla...	7.339	70	39783	13.433	ng	# 74
25) Isophorone	7.345	82	301444	36.735	ng	# 65
31) Naphthalene	8.075	128	33442	2.638	ng	98
37) 2-Methylnaphthalene	8.769	142	27165	3.329	ng	95
38) 1-Methylnaphthalene	8.869	142	19133	2.390	ng	98
50) Dimethylphthalate	9.810	163	21813	2.513	ng	# 1
51) 2,6-Dinitrotoluene	9.810	165	15461	7.847	ng	# 30
57) 2,4-Dinitrotoluene	9.810	165	15461	6.045	ng	# 21
67) 4-Bromophenyl-phenylether	10.610	248	7862	3.399	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136914.D
Acq On : 03 Jan 2024 18:44
Operator : CG\JU
Sample : 05900-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :


Quant Time: Jan 04 03:40:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

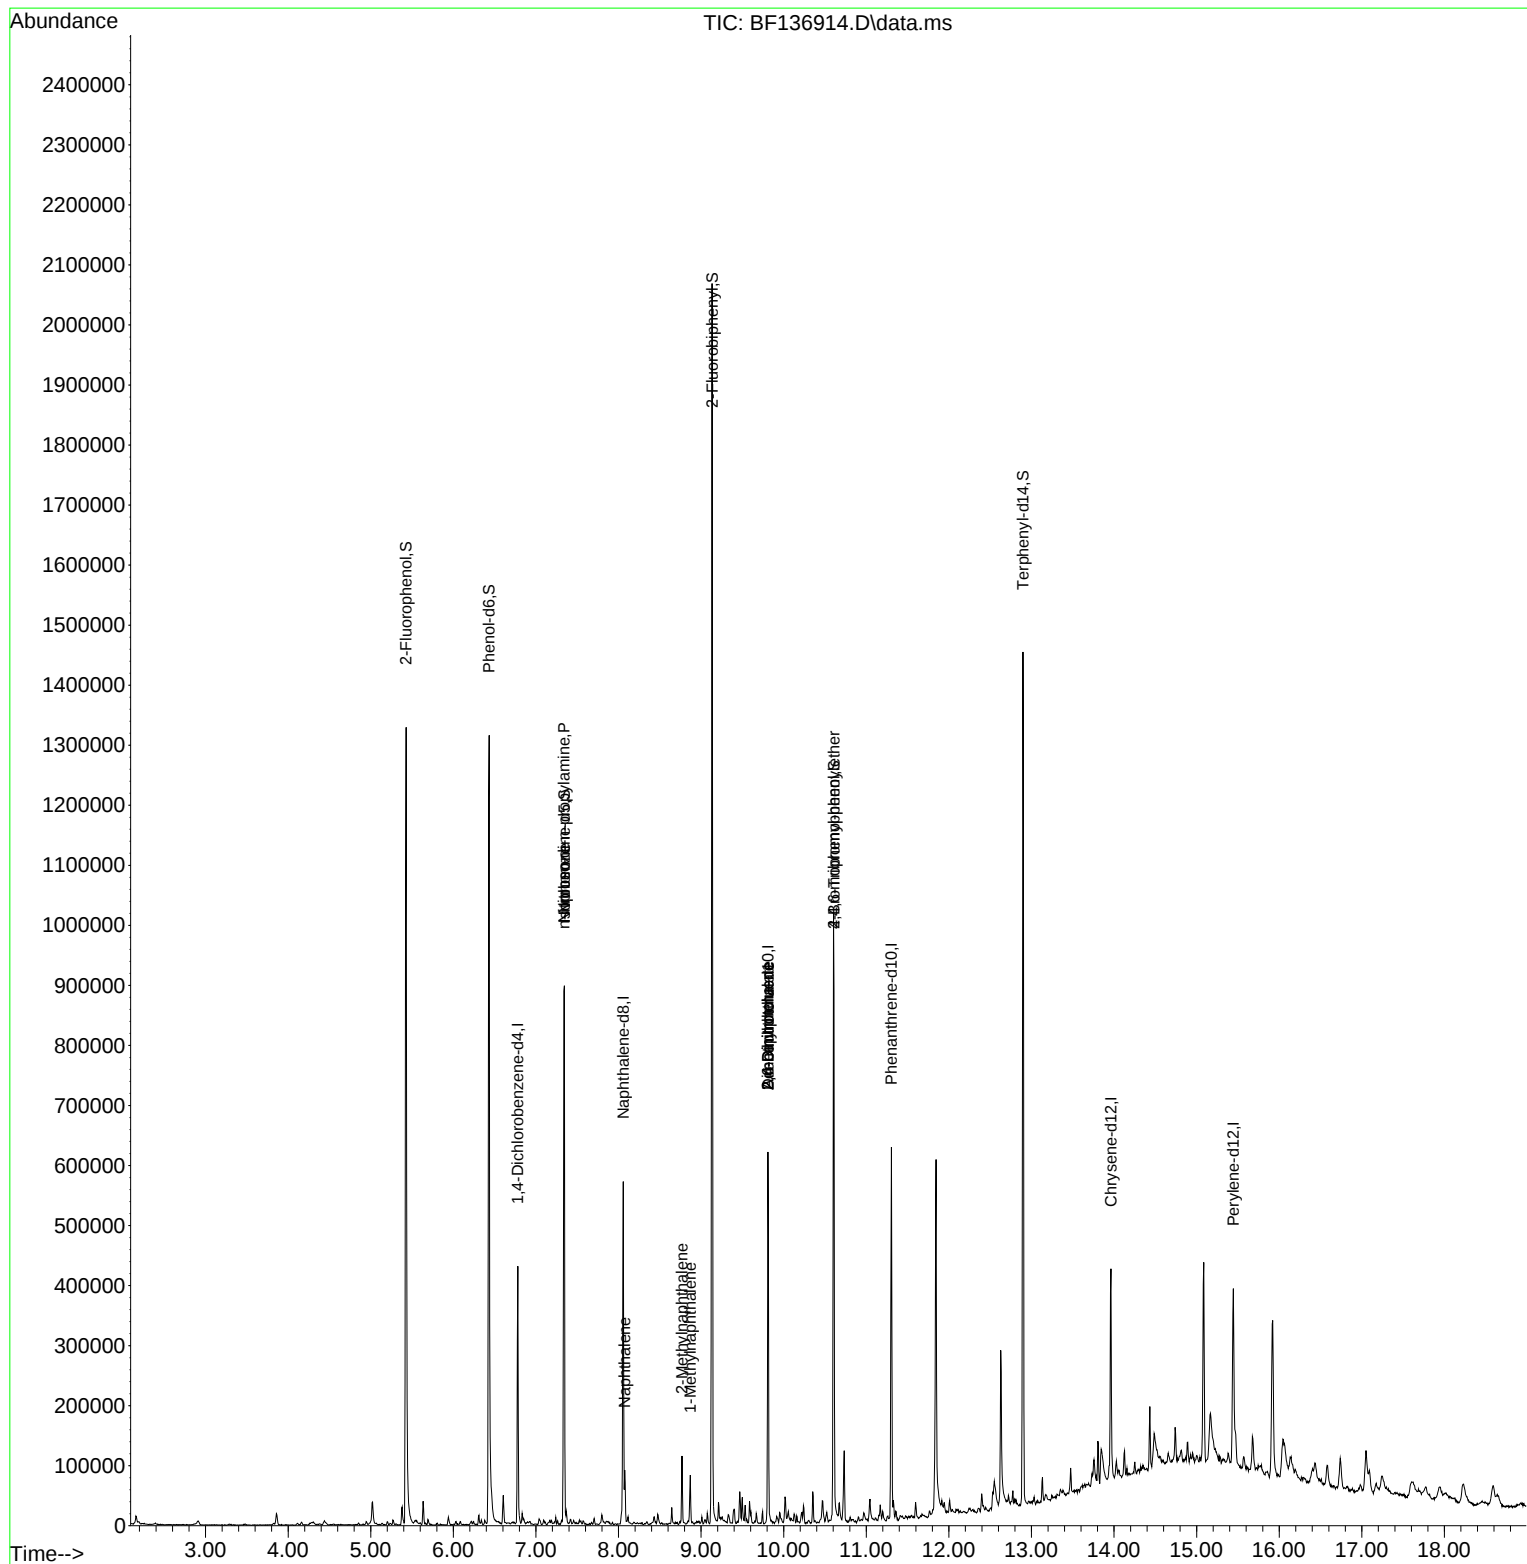






#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.781 min Scan# 79
 Delta R.T. -0.011 min
 Lab File: BF136914.D
 Acq: 03 Jan 2024 18:44

Instrument :
 BNA_F
 ClientSampleId :



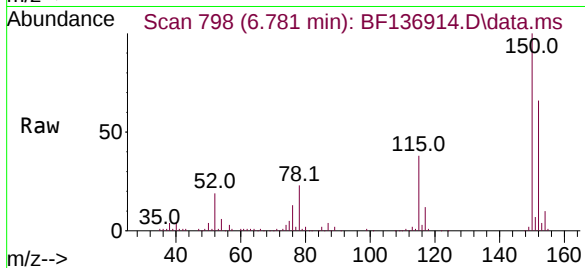



Tgt Ion:152 Resp: 58828
 Ion Ratio Lower Upper
 152 100
 150 152.3 127.0 190.6
 115 57.8 49.0 73.4

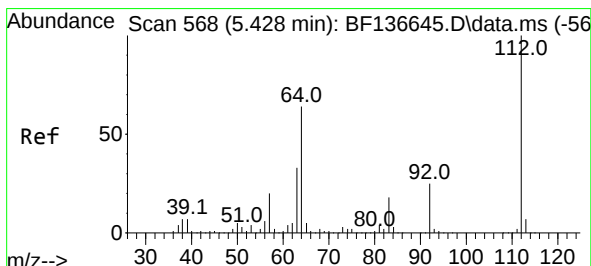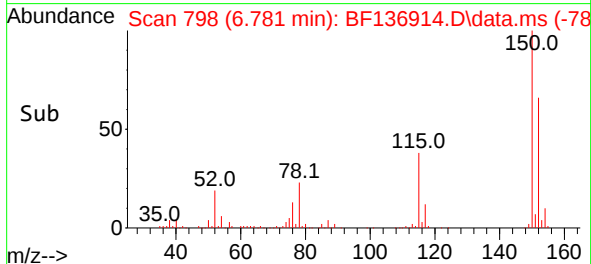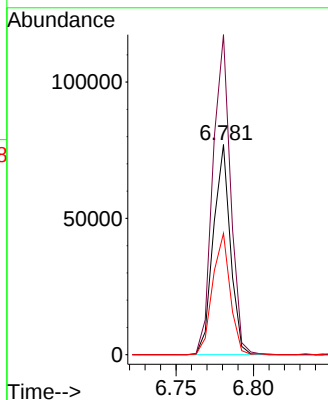

#5
 2-Fluorophenol
 Concen: 99.958 ng
 RT: 5.428 min Scan# 568
 Delta R.T. 0.000 min
 Lab File: BF136914.D
 Acq: 03 Jan 2024 18:44

Tgt Ion:112 Resp: 376875
 Ion Ratio Lower Upper
 112 100
 64 60.4 51.1 76.7
 63 30.2 26.1 39.1


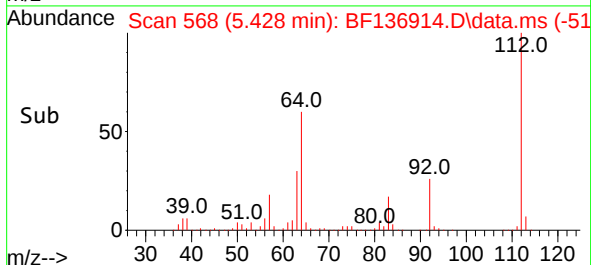
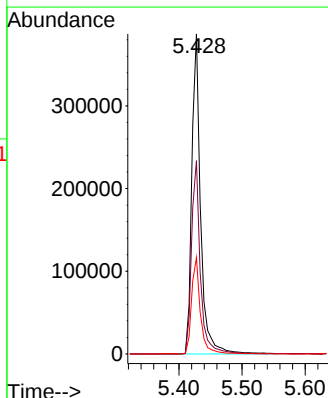
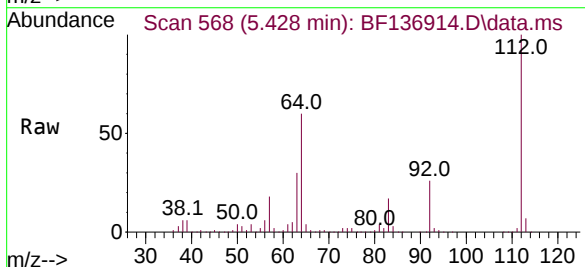


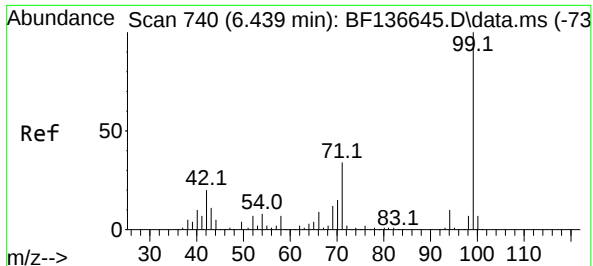

#7
Phenol-d6
Concen: 98.606 ng
RT: 6.434 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF136914.D
Acq: 03 Jan 2024 18:44




Instrument :
BNA_F
ClientSampleId :


Tgt Ion: 99 Resp: 481734
Ion Ratio Lower Upper
99 100
42 18.2 16.1 24.1
71 31.8 27.4 41.2

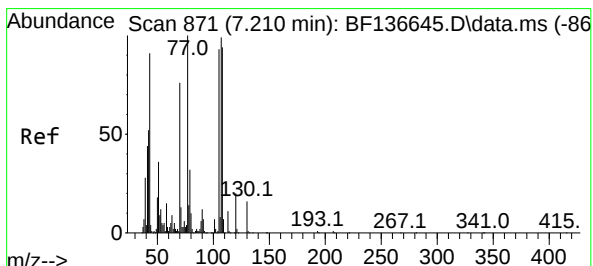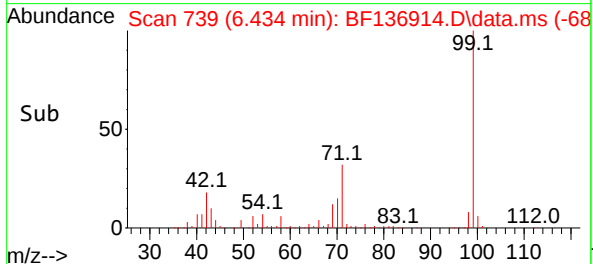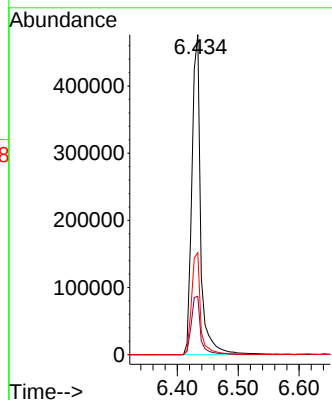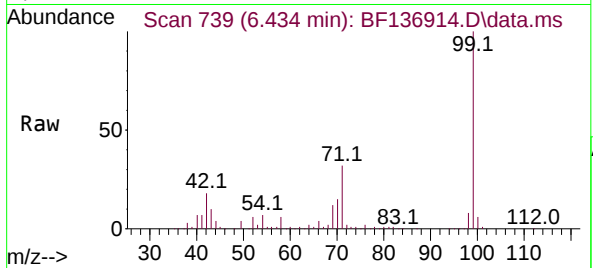

#19
n-Nitroso-di-n-propylamine
Concen: 13.433 ng
RT: 7.339 min Scan# 893
Delta R.T. 0.129 min
Lab File: BF136914.D
Acq: 03 Jan 2024 18:44


Tgt Ion: 70 Resp: 39783
Ion Ratio Lower Upper
70 100
42 51.4 54.2 81.4#
101 0.0 7.6 11.4#
130 1.6 17.1 25.7#

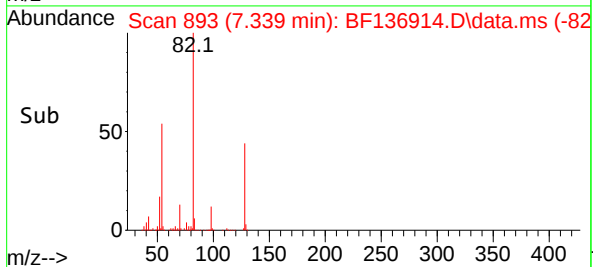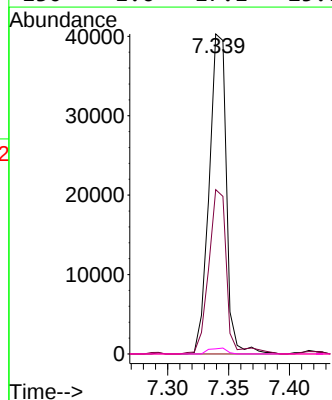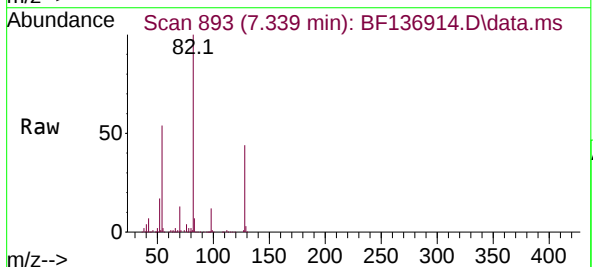



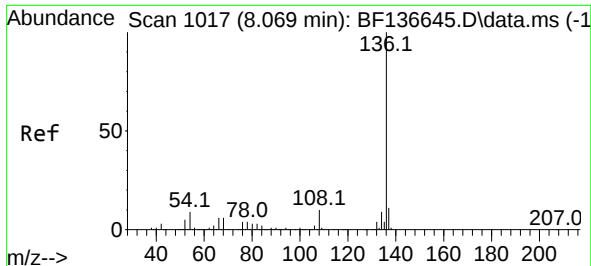


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.057 min Scan# 1015
Delta R.T. -0.012 min
Lab File: BF136914.D
Acq: 03 Jan 2024 18:44

Instrument :
BNA_F
ClientSampleId :







Tgt Ion:	136	Resp:	230766
Ion	Ratio	Lower	Upper
136	100		
137	10.4	9.0	13.4
54	7.7	7.2	10.8
68	5.5	4.9	7.3

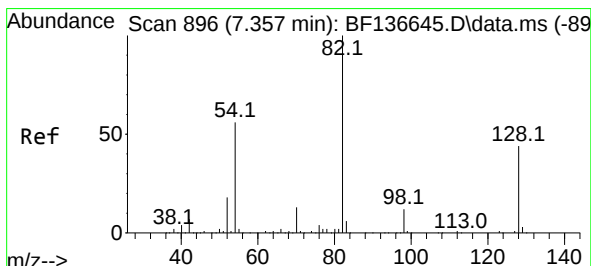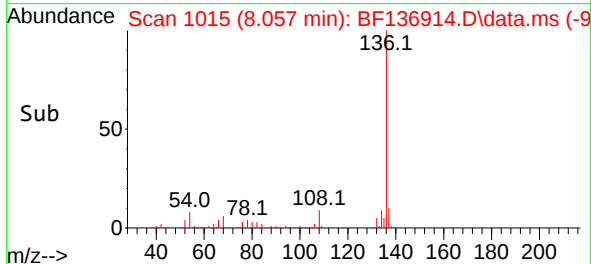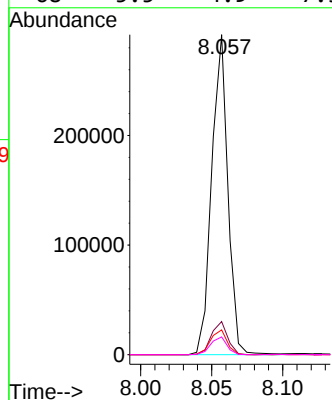

#23
Nitrobenzene-d5
Concen: 67.062 ng
RT: 7.345 min Scan# 894
Delta R.T. -0.012 min
Lab File: BF136914.D
Acq: 03 Jan 2024 18:44

Tgt Ion:	82	Resp:	302428
Ion	Ratio	Lower	Upper
82	100		
128	47.3	35.3	52.9
54	51.2	44.5	66.7


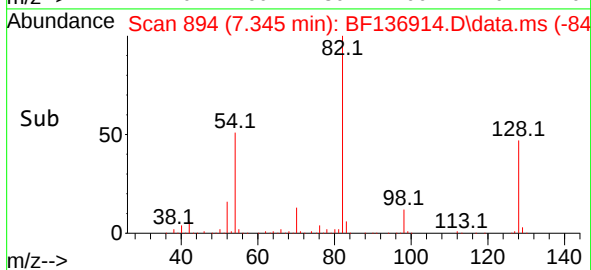
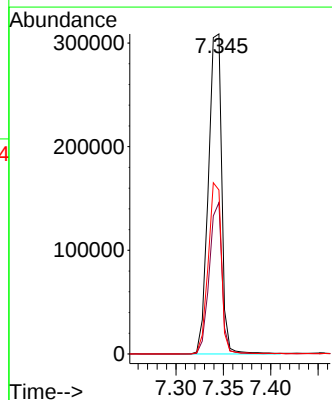
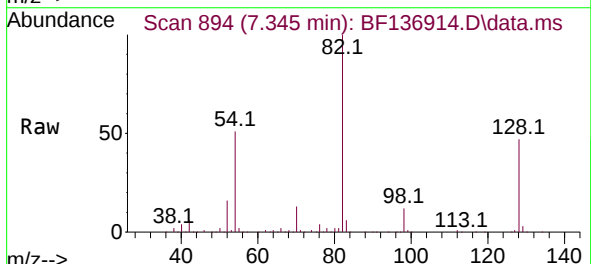


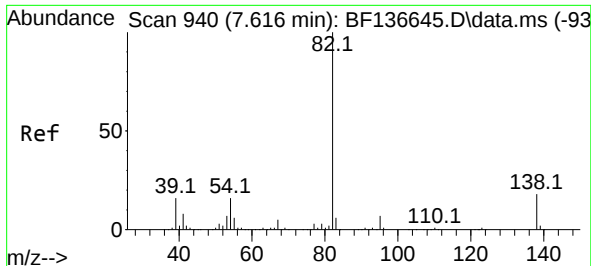

#25
Isophorone
Concen: 36.735 ng
RT: 7.345 min Scan# 894
Delta R.T. -0.271 min
Lab File: BF136914.D
Acq: 03 Jan 2024 18:44




Instrument :
BNA_F
ClientSampleId :


Tgt Ion: 82 Resp: 301444
Ion Ratio Lower Upper
82 100
95 0.0 5.5 8.3#
138 0.0 14.5 21.7#

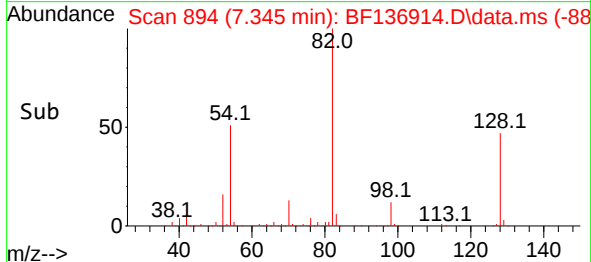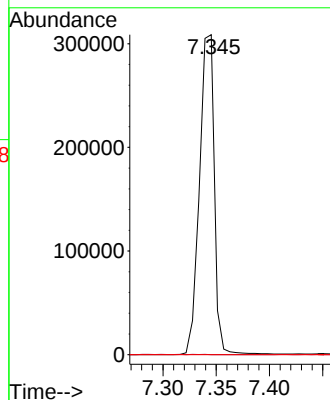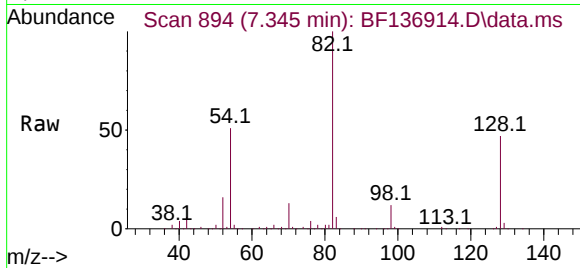

#31
Naphthalene
Concen: 2.638 ng
RT: 8.075 min Scan# 1018
Delta R.T. -0.018 min
Lab File: BF136914.D
Acq: 03 Jan 2024 18:44

Tgt Ion:128 Resp: 33442
Ion Ratio Lower Upper
128 100
129 10.4 8.7 13.1
127 14.7 10.8 16.2

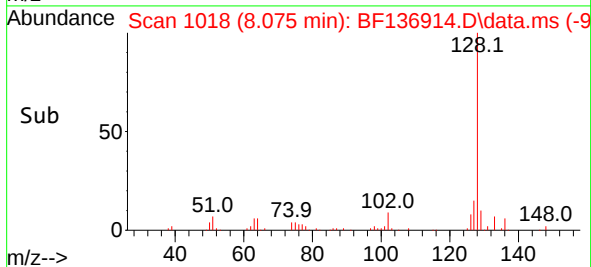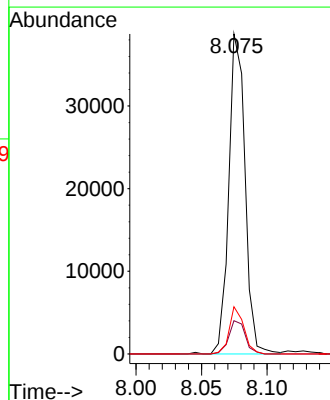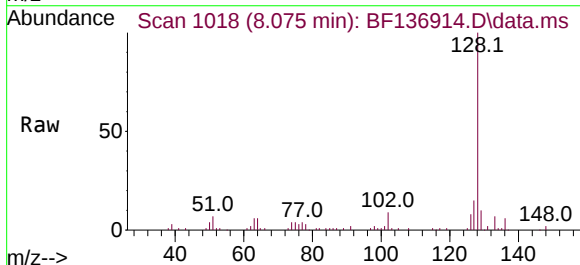

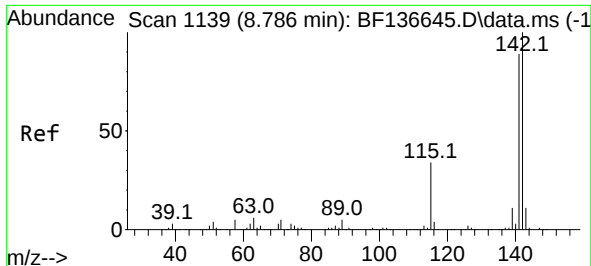

#37

2-Methylnaphthalene

Concen: 3.329 ng

RT: 8.769 min Scan# 1136

Delta R.T. -0.018 min

Lab File: BF136914.D

Acq: 03 Jan 2024 18:44

Instrument :

BNA_F





ClientSampleId :

Tgt Ion:142 Resp: 27165

Ion Ratio Lower Upper

142 100

141 83.9 71.1 106.7

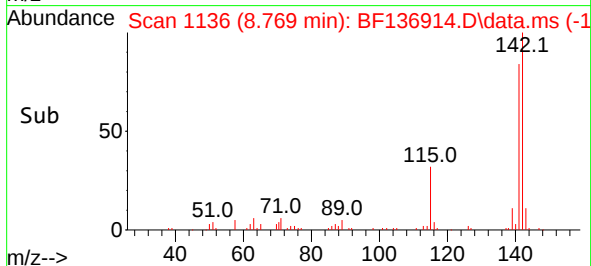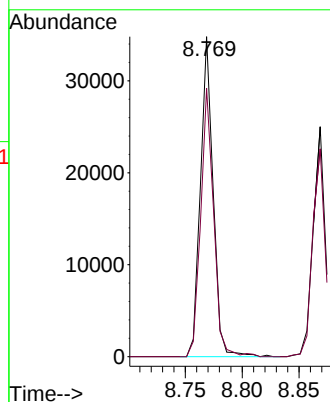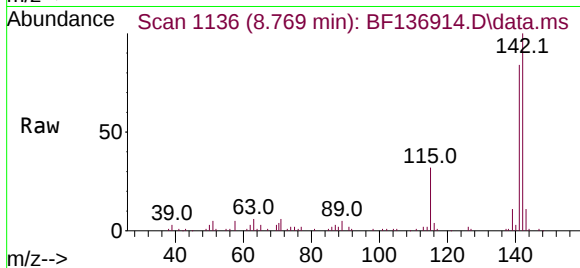

#38

1-Methylnaphthalene

Concen: 2.390 ng

RT: 8.869 min Scan# 1153

Delta R.T. -0.018 min

Lab File: BF136914.D




Acq: 03 Jan 2024 18:44


Tgt Ion:142 Resp: 19133

Ion Ratio Lower Upper

142 100

141 90.4 73.6 110.4

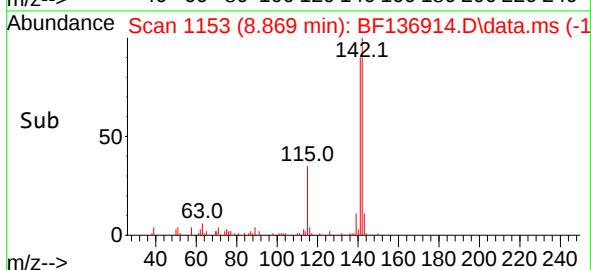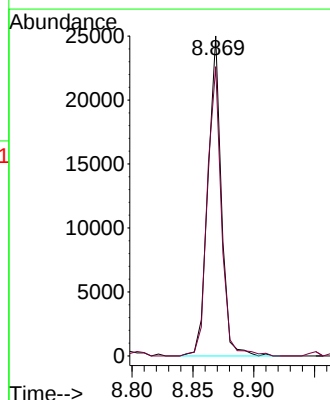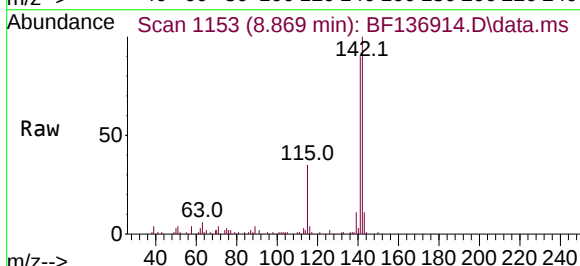



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.810 min Scan# 11

Delta R.T. -0.018 min


Lab File: BF136914.D

Acq: 03 Jan 2024 18:44

Instrument :

BNA_F

ClientSampleId :

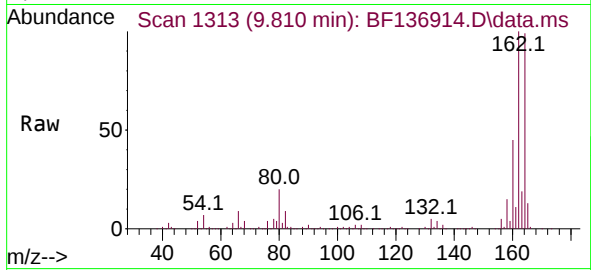




Tgt Ion:164 Resp: 118856

Ion Ratio Lower Upper

164 100

162 100.6 81.6 122.4

160 45.0 34.9 52.3

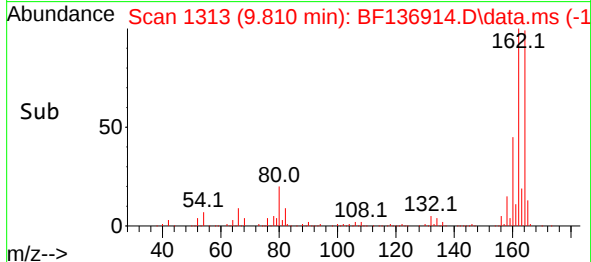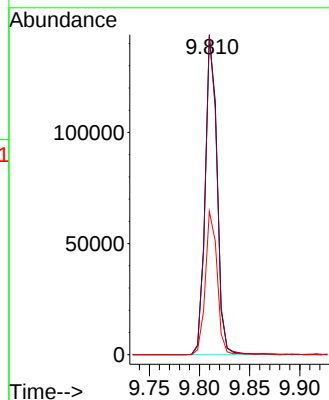

#42

2,4,6-Tribromophenol

Concen: 93.523 ng

RT: 10.610 min Scan# 1449

Delta R.T. -0.012 min

Lab File: BF136914.D

Acq: 03 Jan 2024 18:44




Tgt Ion:330 Resp: 130913


Ion Ratio Lower Upper

330 100

332 96.1 77.4 116.0

141 28.8 23.4 35.2

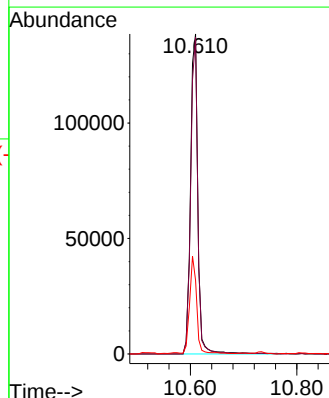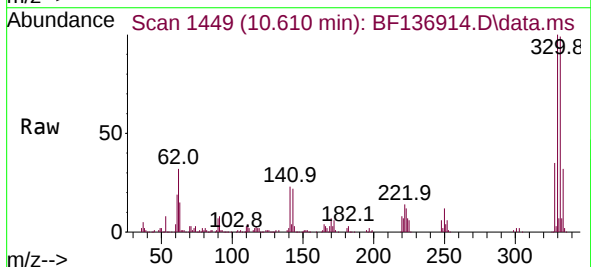

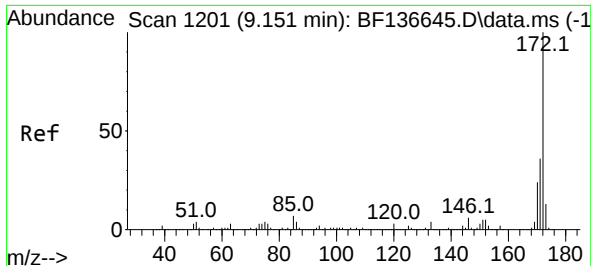

#45

2-Fluorobiphenyl

Concen: 69.783 ng

RT: 9.133 min Scan# 1198

Delta R.T. -0.018 min


Lab File: BF136914.D

Acq: 03 Jan 2024 18:44

Instrument :

BNA_F

ClientSampleId :






Tgt Ion:172 Resp: 616674

Ion Ratio Lower Upper

172 100

171 35.5 29.0 43.6

170 23.1 19.0 28.4

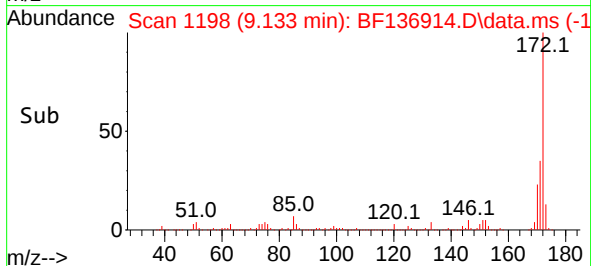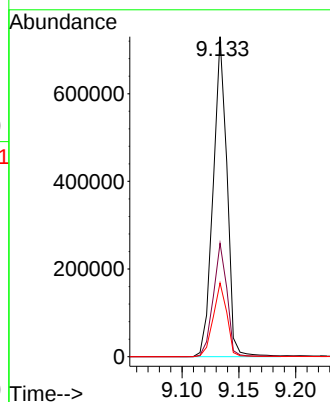

#50

Dimethylphthalate

Concen: 2.513 ng

RT: 9.810 min Scan# 1313

Delta R.T. 0.253 min

Lab File: BF136914.D

Acq: 03 Jan 2024 18:44




Tgt Ion:163 Resp: 21813


Ion Ratio Lower Upper

163 100

194 0.0 3.3 4.9#

164 519.9 7.8 11.6#

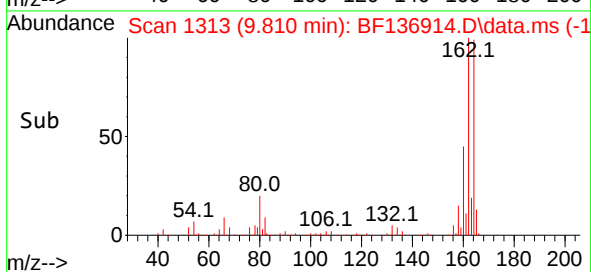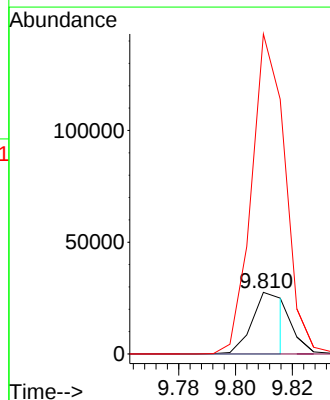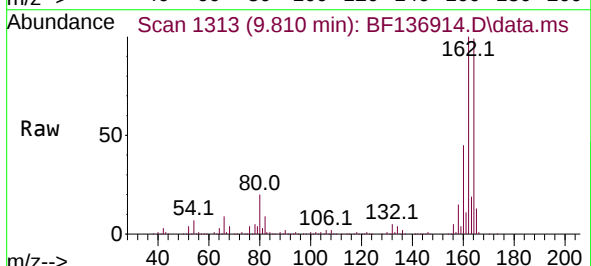



#51

2,6-Dinitrotoluene

Concen: 7.847 ng

RT: 9.810 min Scan# 11

Delta R.T. 0.188 min

Lab File: BF136914.D

Acq: 03 Jan 2024 18:44

Instrument :

BNA_F

ClientSampleId :





Tgt Ion:165 Resp: 15461

Ion Ratio Lower Upper

165 100

63 1.3 39.8 59.6#

89 1.4 38.8 58.2#

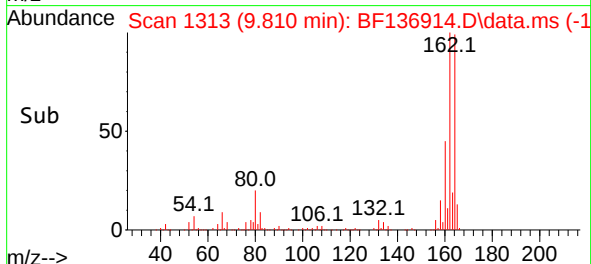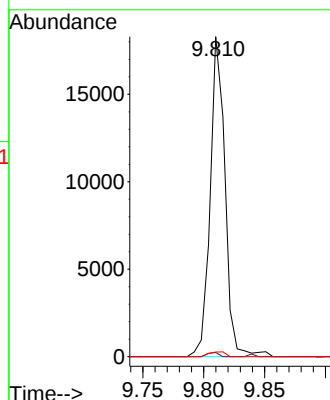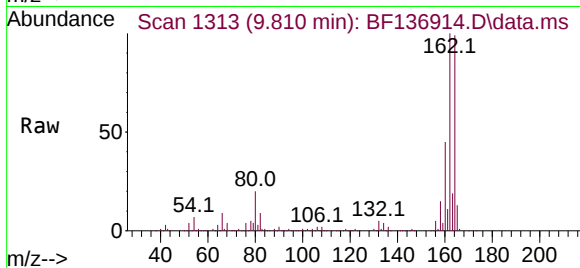

#57

2,4-Dinitrotoluene

Concen: 6.045 ng

RT: 9.810 min Scan# 1313

Delta R.T. -0.212 min

Lab File: BF136914.D

Acq: 03 Jan 2024 18:44

Tgt Ion:165 Resp: 15461




Ion Ratio Lower Upper


165 100

63 1.3 41.0 61.6#

89 1.4 59.9 89.9#

182 0.0 2.0 3.0#

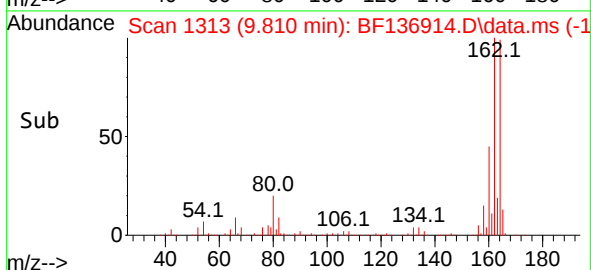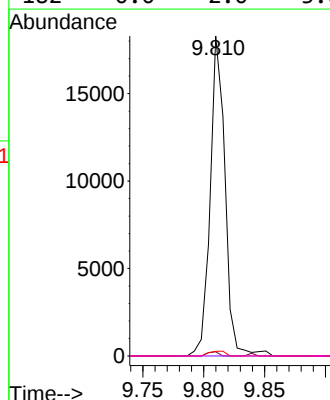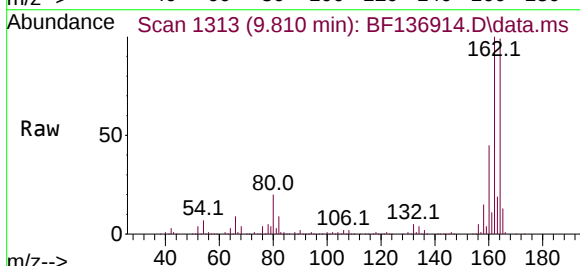



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.304 min Scan# 1

Delta R.T. -0.012 min

Lab File: BF136914.D

Acq: 03 Jan 2024 18:44

Instrument :

BNA_F

ClientSampleId :





Tgt Ion:188 Resp: 208246

Ion Ratio Lower Upper

188 100

94 8.8 7.5 11.3

80 9.2 8.1 12.1

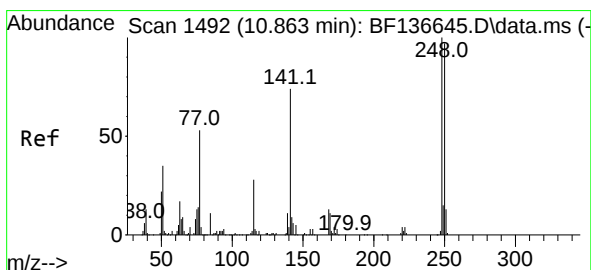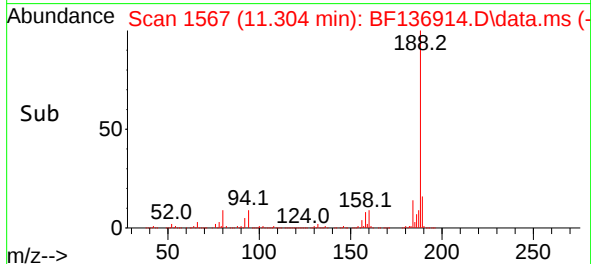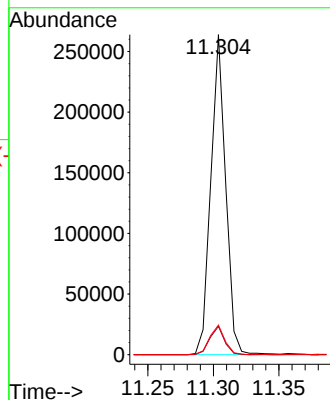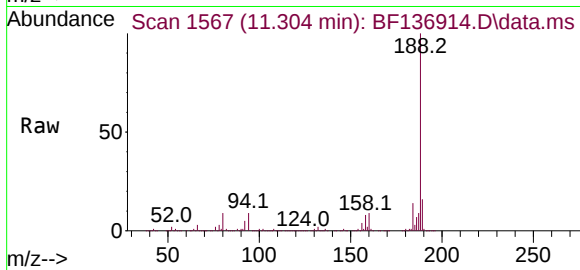

#67

4-Bromophenyl-phenylether

Concen: 3.399 ng

RT: 10.610 min Scan# 1449

Delta R.T. -0.253 min

Lab File: BF136914.D

Acq: 03 Jan 2024 18:44




Tgt Ion:248 Resp: 7862


Ion Ratio Lower Upper

248 100

250 202.6 77.8 116.6#

141 399.0 59.2 88.8#

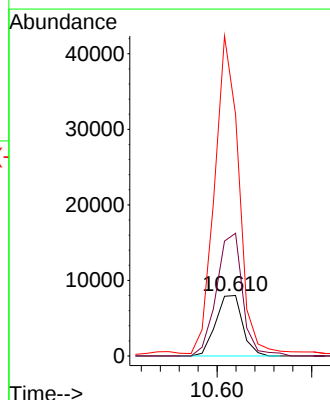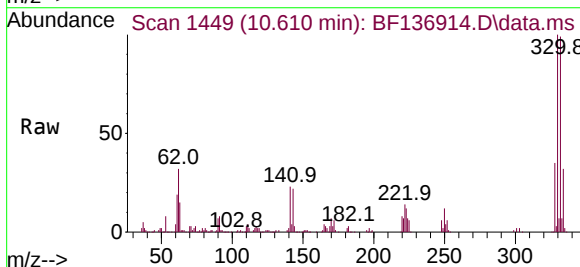



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.963 min Scan# 20

Delta R.T. -0.006 min


Lab File: BF136914.D

Acq: 03 Jan 2024 18:44

Instrument :

BNA_F

ClientSampleId :

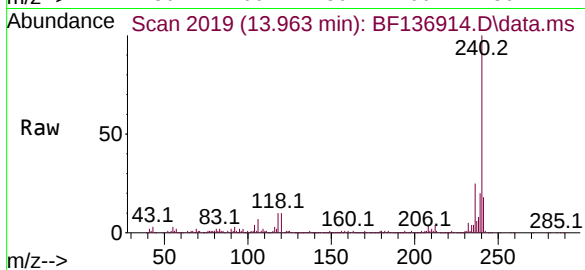




Tgt Ion:240 Resp: 121379

Ion Ratio Lower Upper

240 100

120 9.6 10.3 15.5#

236 25.1 19.4 29.2

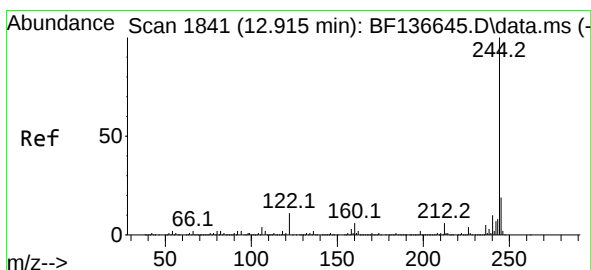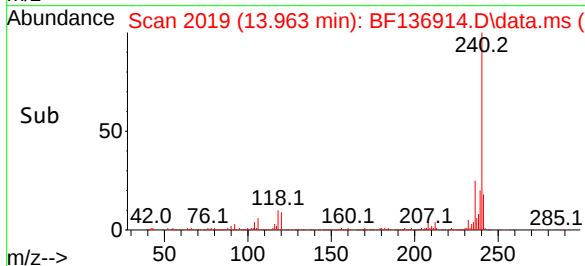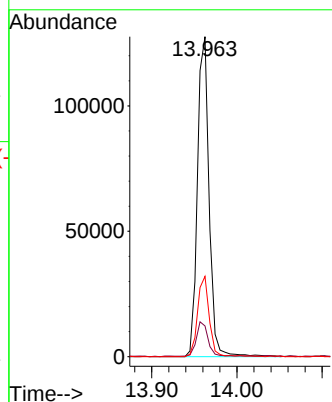

#79

Terphenyl-d14

Concen: 58.394 ng

RT: 12.898 min Scan# 1838

Delta R.T. -0.018 min

Lab File: BF136914.D

Acq: 03 Jan 2024 18:44




Tgt Ion:244 Resp: 507188


Ion Ratio Lower Upper

244 100

212 6.3 5.0 7.4


122 11.5 9.0 13.4

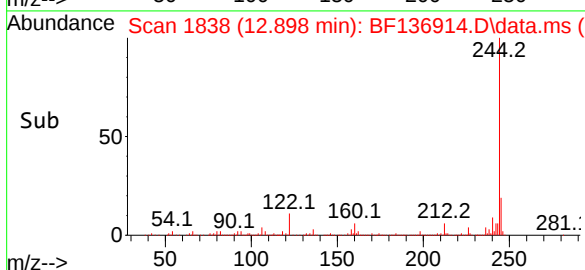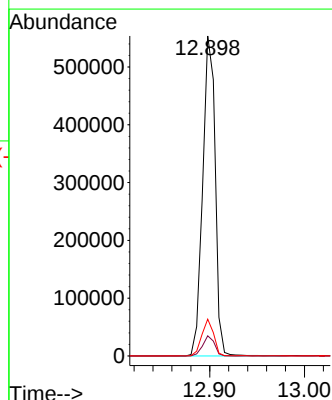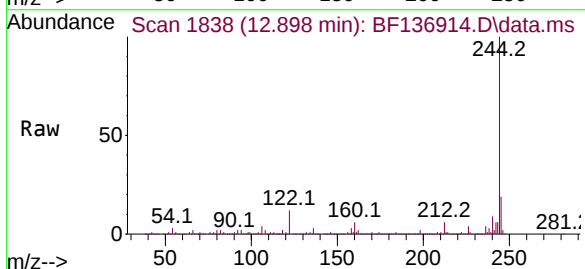



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.445 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BF136914.D
 Acq: 03 Jan 2024 18:44

Instrument :
 BNA_F
 ClientSampleId :

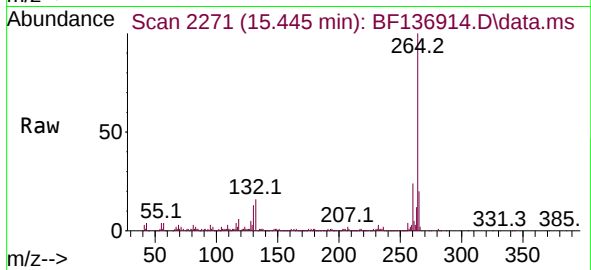

Tgt Ion:264 Resp: 140198

Ion	Ratio	Lower	Upper
264	100		
260	23.7	18.3	27.5
265	20.2	17.0	25.6

