
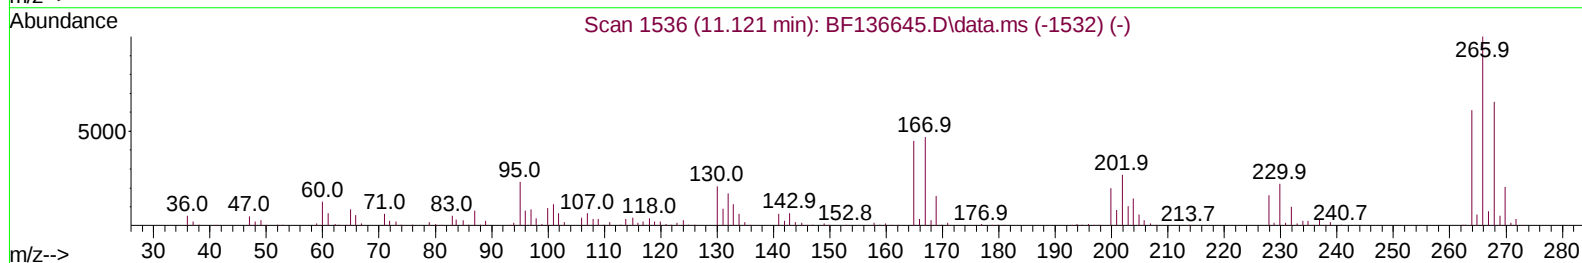
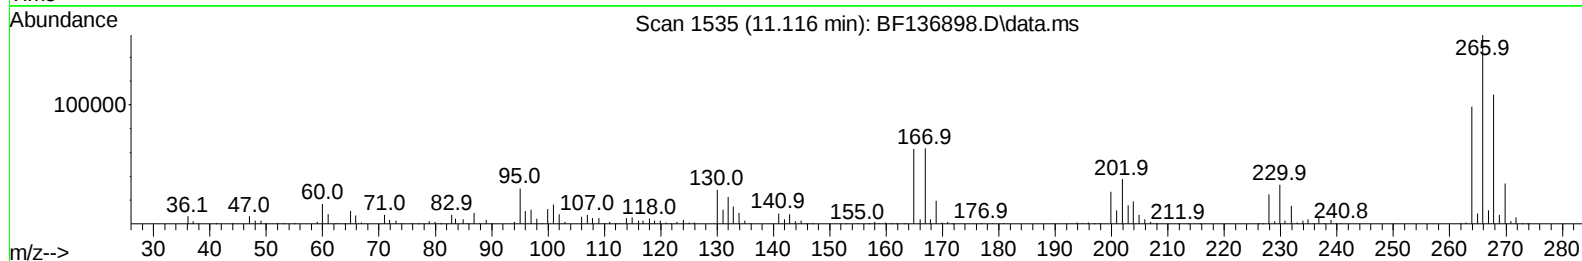


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136898.D
Acq On : 03 Jan 2024 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 01:43:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

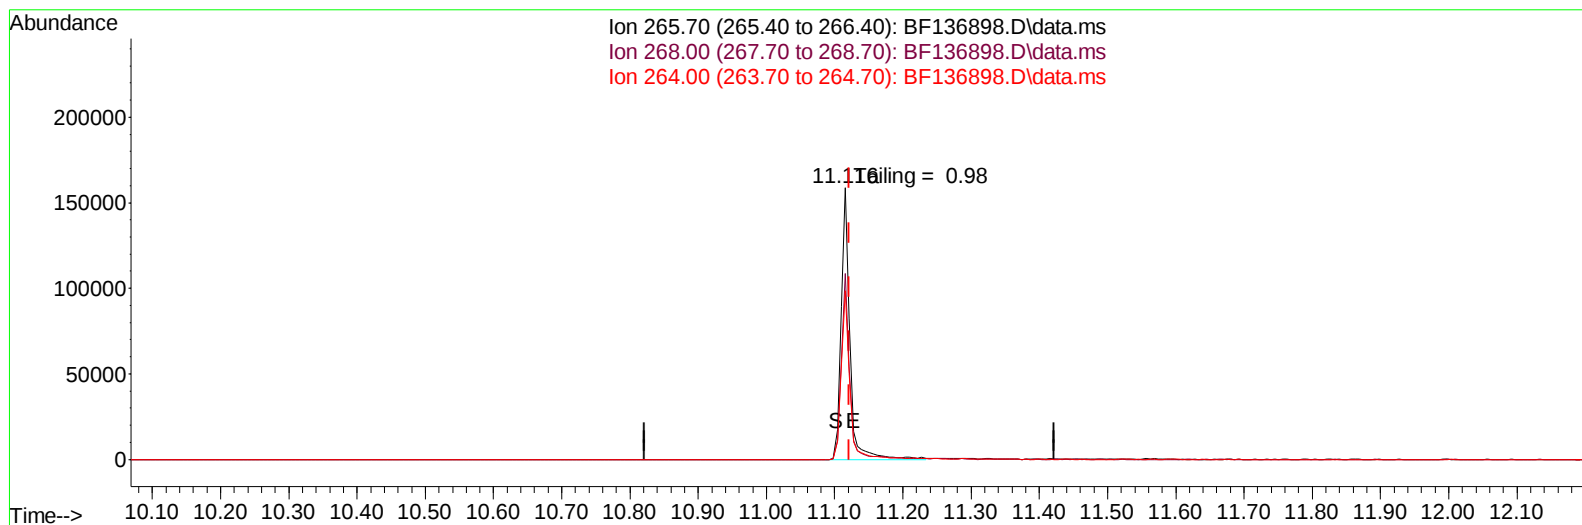




TIC: BF136898.D\data.ms

(70) Pentachlorophenol (C)**11.116min (-0.006) 45192.86 ng****response 141564**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	68.39
264.00	61.20	62.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136898.D
Acq On : 03 Jan 2024 09:43
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 01:43:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

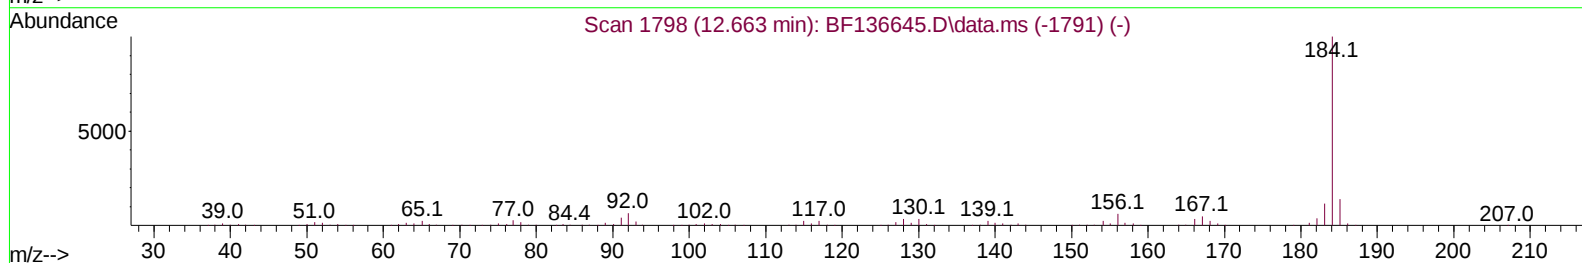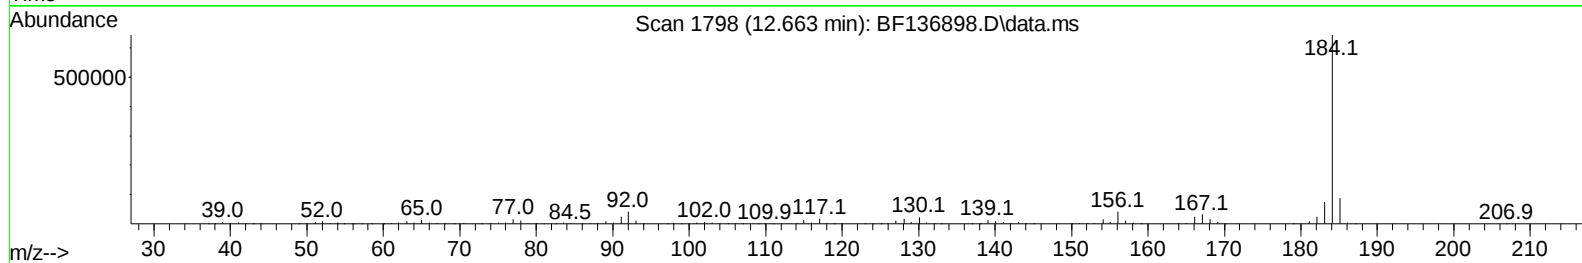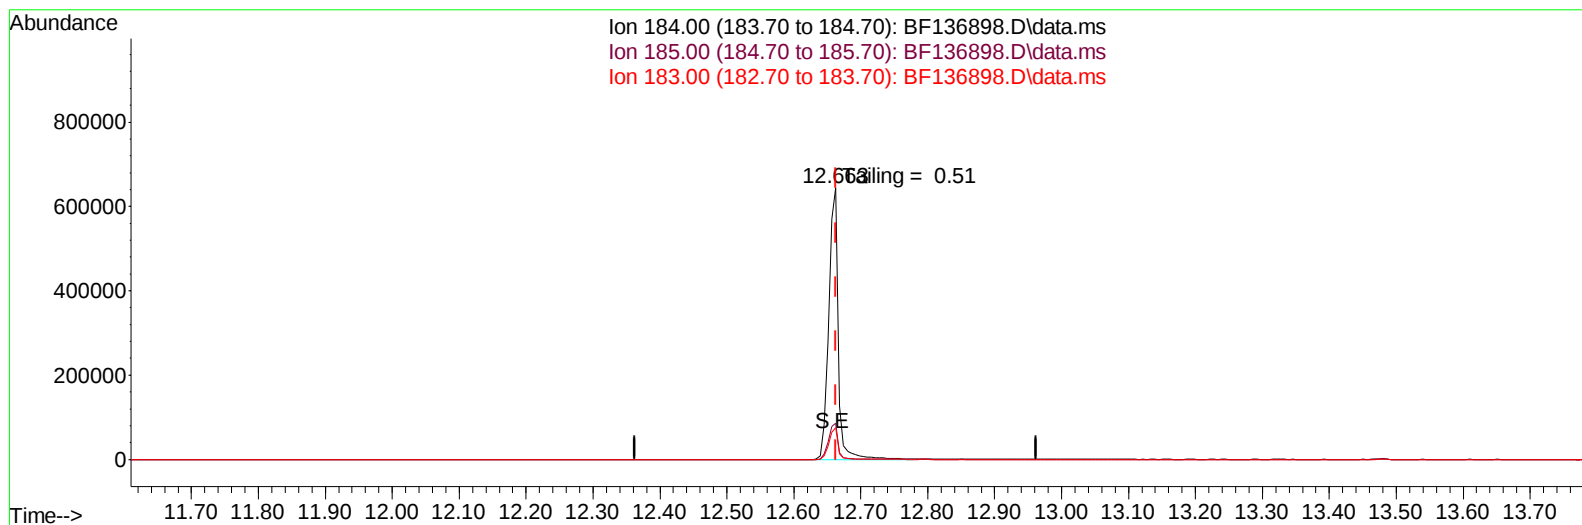

TIC: BF136898.D\data.ms

(77) Benzidine**12.663min (+ 0.000) 62203.34 ng****response 649275**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.45
183.00	11.60	11.60
0.00	0.00	0.00