

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
 Data File : BF136900.D
 Acq On : 03 Jan 2024 10:46
 Operator : CG\JU
 Sample : PB157973BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157973BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.063	501	506	517	rBV	50842	87493	2.09%	0.395%
2	5.440	564	570	573	rBV	2812145	2852456	67.98%	12.866%
3	6.434	733	739	742	rBV	2348105	2948705	70.27%	13.300%
4	6.781	794	798	801	rBV	671850	517149	12.32%	2.333%
5	7.345	888	894	897	rBV	1628929	1963036	46.78%	8.854%
6	8.057	1010	1015	1018	rBV	838761	695774	16.58%	3.138%
7	9.139	1192	1199	1202	rBV	3681833	3620695	86.28%	16.331%
8	9.810	1308	1313	1317	rBV	869807	813299	19.38%	3.668%
9	10.616	1444	1450	1453	rBV	2080036	2218463	52.87%	10.006%
10	11.304	1563	1567	1571	rBV	1005218	914325	21.79%	4.124%
11	12.910	1834	1840	1843	rBV	3557716	4196257	100.00%	18.927%
12	13.963	2015	2019	2030	rVB	838183	748849	17.85%	3.378%
13	15.445	2265	2271	2282	rBV	411868	594599	14.17%	2.682%




Sum of corrected areas: 22171100

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136900.D
Acq On : 03 Jan 2024 10:46
Operator : CG\JU
Sample : PB157973BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157973BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

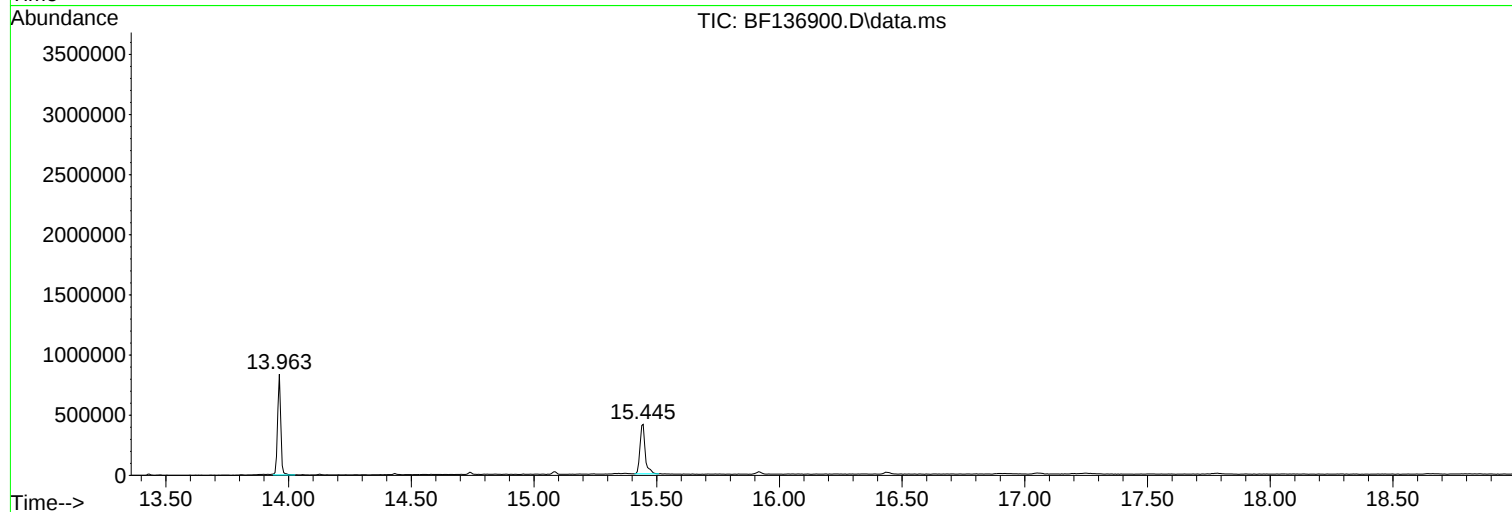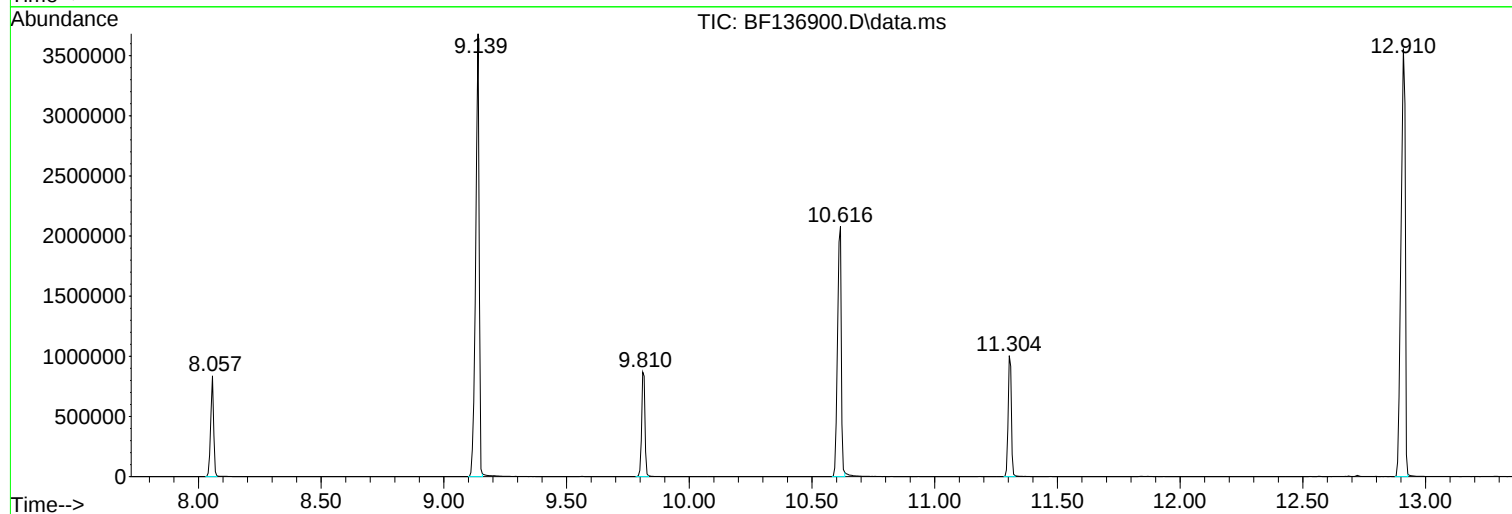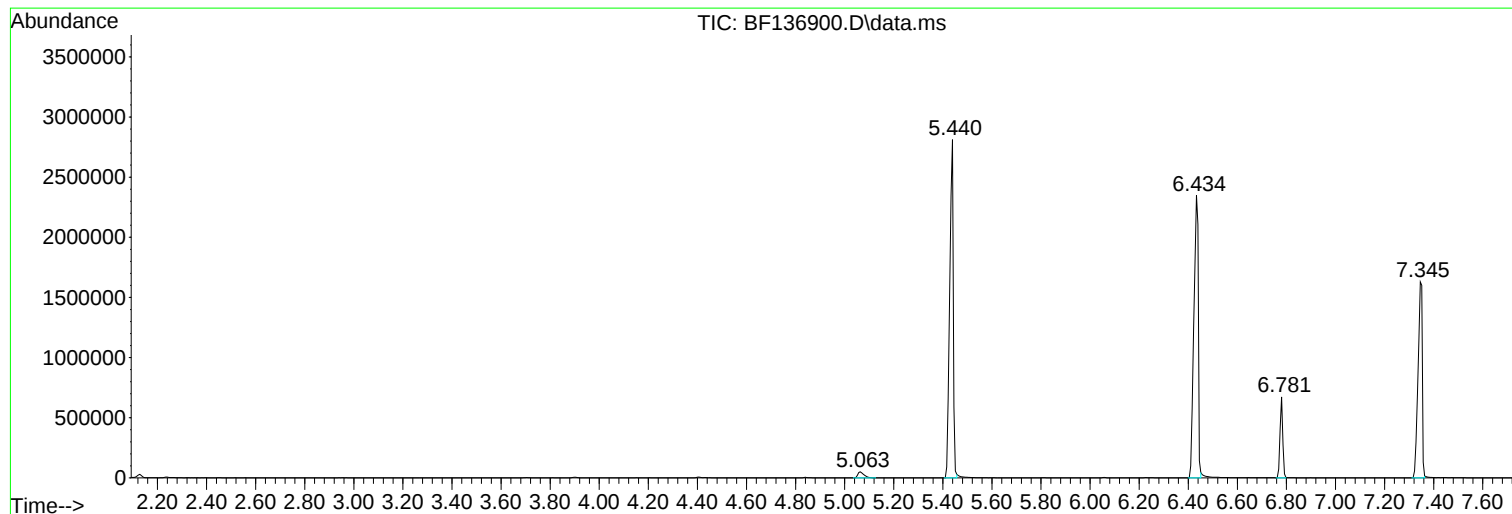

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136900.D
Acq On : 03 Jan 2024 10:46
Operator : CG\JU
Sample : PB157973BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157973BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Acetic acid, 1,1-dimethylet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.063	3.38 ng	87493	1,4-Dichlorobenzene-d4	6.781

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	56		
2	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	38		
4	3-Hexanol	102	C6H14O	000623-37-0	33		
5	3-Octanol	130	C8H18O	000589-98-0	33		

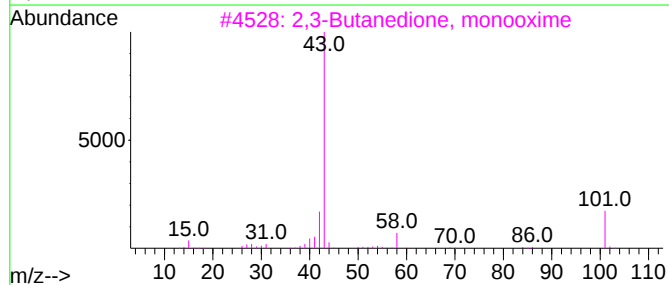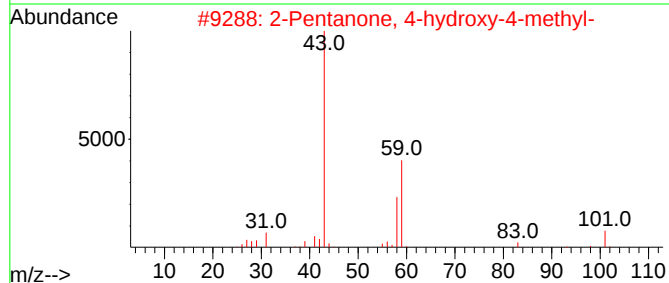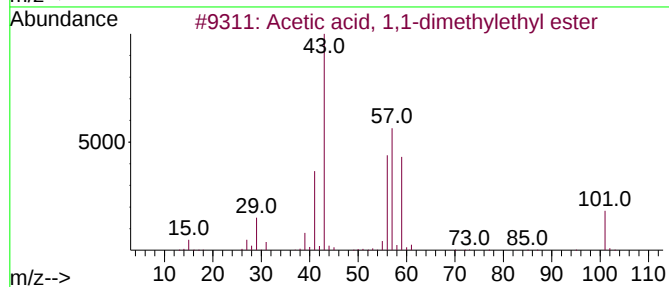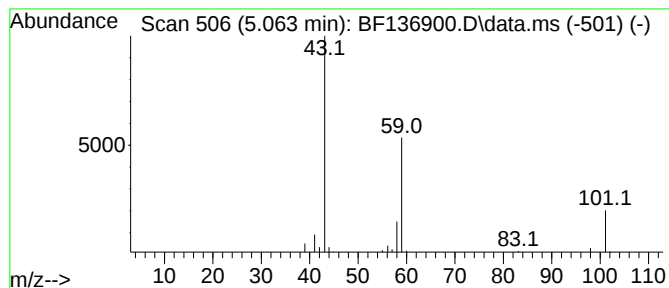

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136900.D
Acq On : 03 Jan 2024 10:46
Operator : CG\JU
Sample : PB157973BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157973BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Acetic acid, 1,...	5.063	3.4	ng	87493	1	6.781	517149	20.0