

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136902.D
Acq On : 03 Jan 2024 12:04
Operator : CG\JU
Sample : PB158099BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158099BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.063	500	506	517	rBV	48834	85785	2.12%	0.399%
2	5.440	564	570	573	rBV	2635200	2814278	69.59%	13.078%
3	6.434	733	739	742	rBV	2247288	2864066	70.82%	13.309%
4	6.781	794	798	801	rBV	654923	505497	12.50%	2.349%
5	7.351	888	895	897	rBV	1654435	1886196	46.64%	8.765%
6	8.057	1010	1015	1018	rBV	809779	677625	16.76%	3.149%
7	9.139	1192	1199	1202	rBV	3644178	3532630	87.35%	16.416%
8	9.816	1308	1314	1317	rBV	913410	788638	19.50%	3.665%
9	10.616	1444	1450	1453	rBV	1999861	2153143	53.24%	10.005%
10	11.304	1563	1567	1571	rBV	947481	886896	21.93%	4.121%
11	12.910	1834	1840	1843	rBV	3658332	4044049	100.00%	18.792%
12	13.963	2015	2019	2028	rVB	775585	707178	17.49%	3.286%
13	15.445	2266	2271	2281	rBV	387578	573983	14.19%	2.667%




Sum of corrected areas: 21519964

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136902.D
Acq On : 03 Jan 2024 12:04
Operator : CG\JU
Sample : PB158099BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158099BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

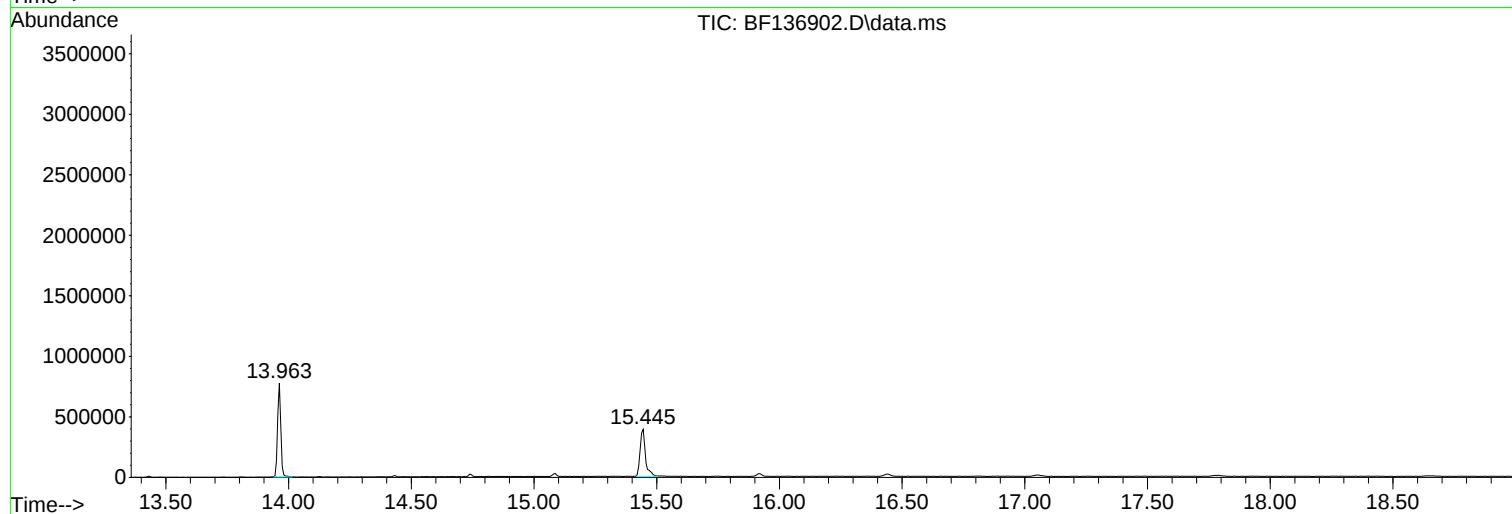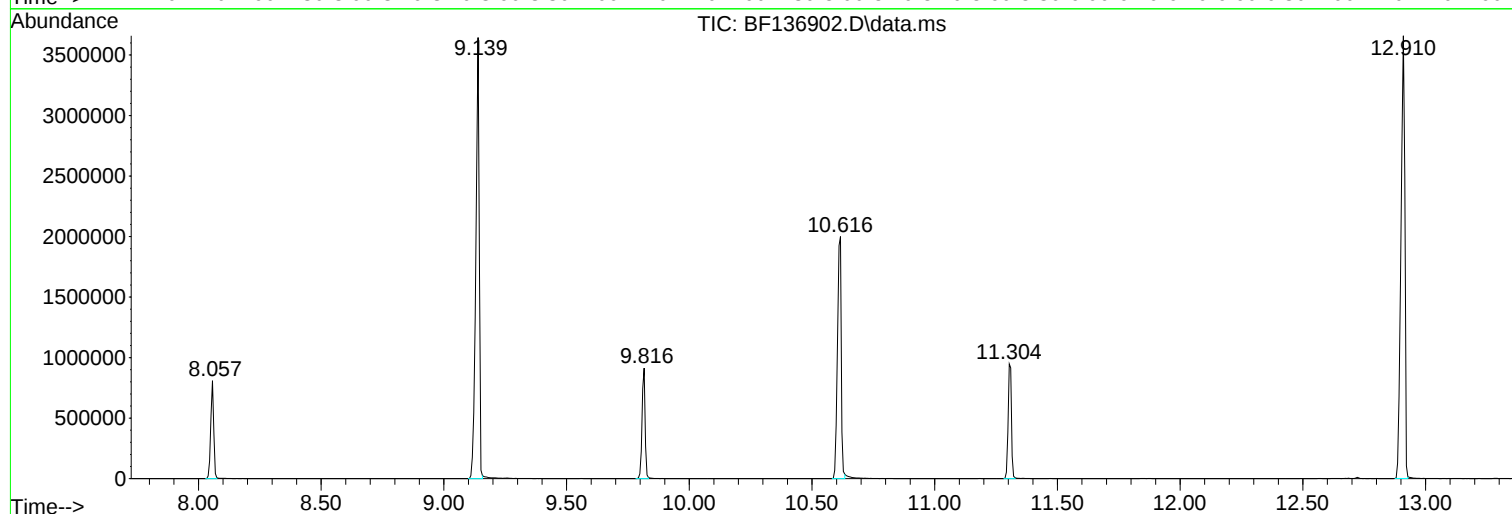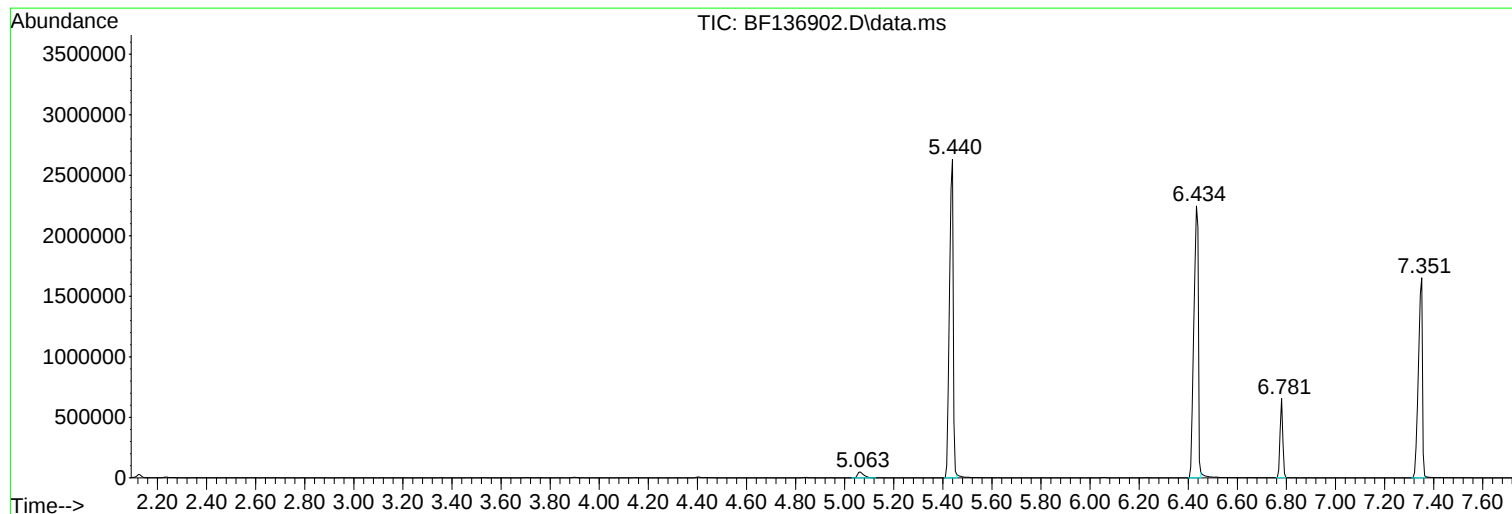

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136902.D
Acq On : 03 Jan 2024 12:04
Operator : CG\JU
Sample : PB158099BL
Misc :
ALS Vial : 5 Sample Multiplier: 1












Instrument :
BNA_F
ClientSampleId :
PB158099BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
5.063	3.39 ng	85785	1,4-Dichlorobenzene-d4		6.781	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	56
2	Acetic acid, 1,1-dimethylethyl e...		116	C6H12O2	000540-88-5	39
3	Propane, 2-methyl-2-(1-methyleth...		116	C7H16O	017348-59-3	33
4	2-Pentanol, 2,4-dimethyl-		116	C7H16O	000625-06-9	28
5	Acetic acid, cyano-, 1,1-dimethy...		141	C7H11NO2	001116-98-9	23

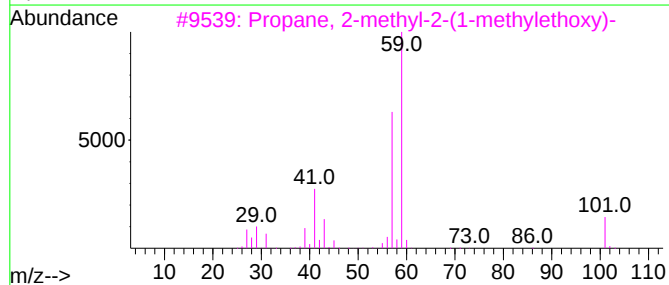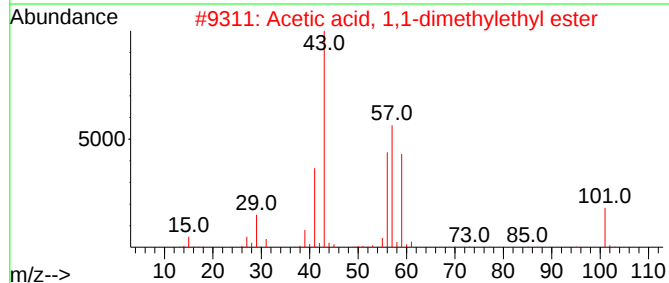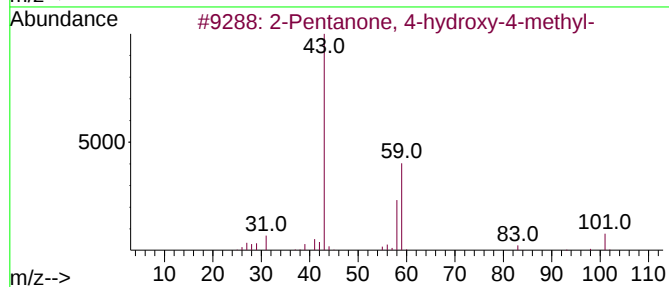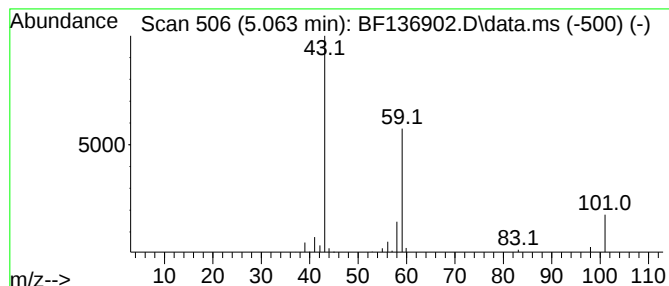

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136902.D
Acq On : 03 Jan 2024 12:04
Operator : CG\JU
Sample : PB158099BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158099BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.063	3.4	ng	85785	1	6.781	505497	20.0