

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
 Data File : BF136904.D
 Acq On : 03 Jan 2024 13:08
 Operator : CG\JU
 Sample : PB158147BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB158147BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.134	3	8	16	rVB	27463	36937	1.17%	0.213%
2	5.434	565	569	572	rBV	2217465	2256292	71.75%	13.013%
3	6.434	733	739	742	rBV	2056485	2241802	71.29%	12.930%
4	6.781	794	798	801	rBV	566007	437191	13.90%	2.522%
5	7.345	888	894	897	rBV	1366639	1454499	46.26%	8.389%
6	8.057	1010	1015	1018	rBV	702431	584271	18.58%	3.370%
7	9.139	1192	1199	1202	rBV	2920389	2800472	89.06%	16.152%
8	9.810	1308	1313	1317	rBV	706175	668364	21.26%	3.855%
9	10.610	1444	1449	1452	rBV	1864481	1712434	54.46%	9.877%
10	11.304	1563	1567	1571	rBV	912754	774011	24.62%	4.464%
11	12.910	1834	1840	1843	rBV	3089736	3144456	100.00%	18.136%
12	13.962	2015	2019	2029	rVB	632015	605049	19.24%	3.490%
13	15.080	2205	2209	2214	rBV2	29043	34702	1.10%	0.200%
14	15.445	2265	2271	2285	rBV	318180	494695	15.73%	2.853%
15	15.915	2345	2351	2357	rBV2	29541	45635	1.45%	0.263%
16	16.439	2435	2440	2449	rVB2	24542	47457	1.51%	0.274%




Sum of corrected areas: 17338267

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136904.D
Acq On : 03 Jan 2024 13:08
Operator : CG\JU
Sample : PB158147BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158147BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

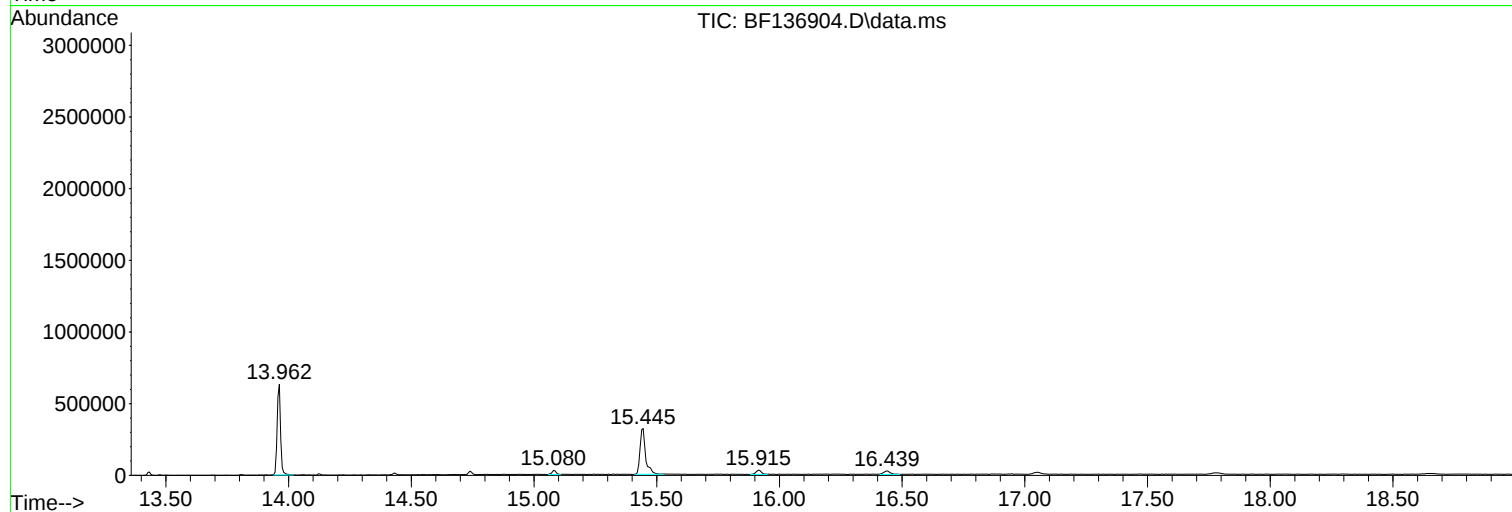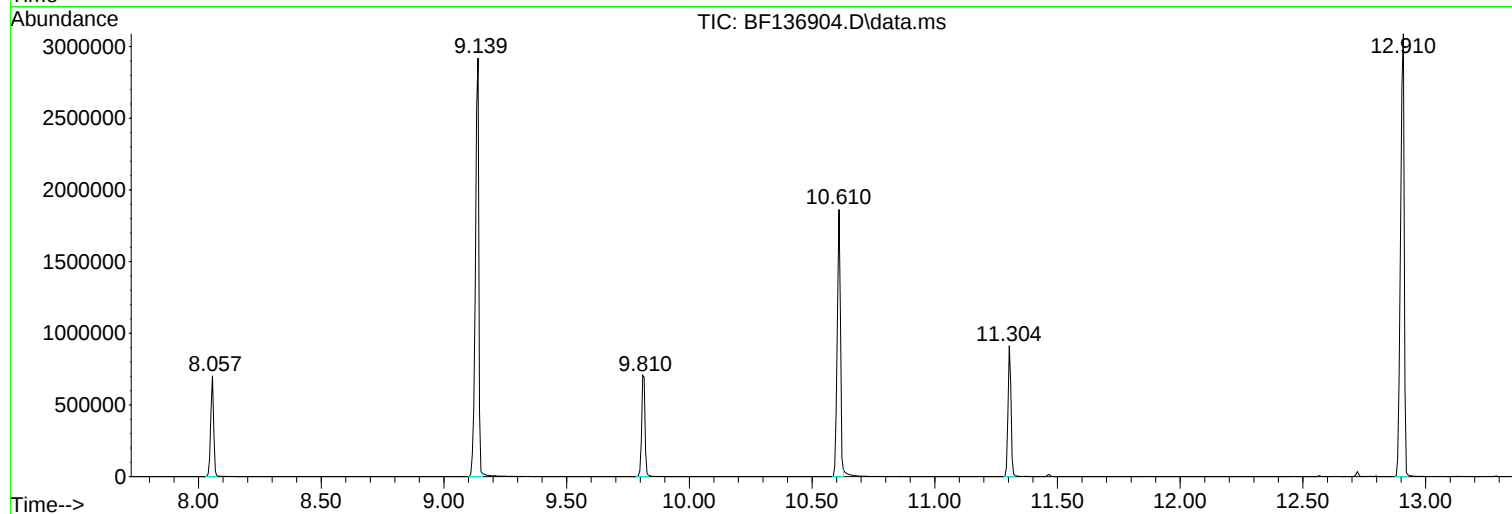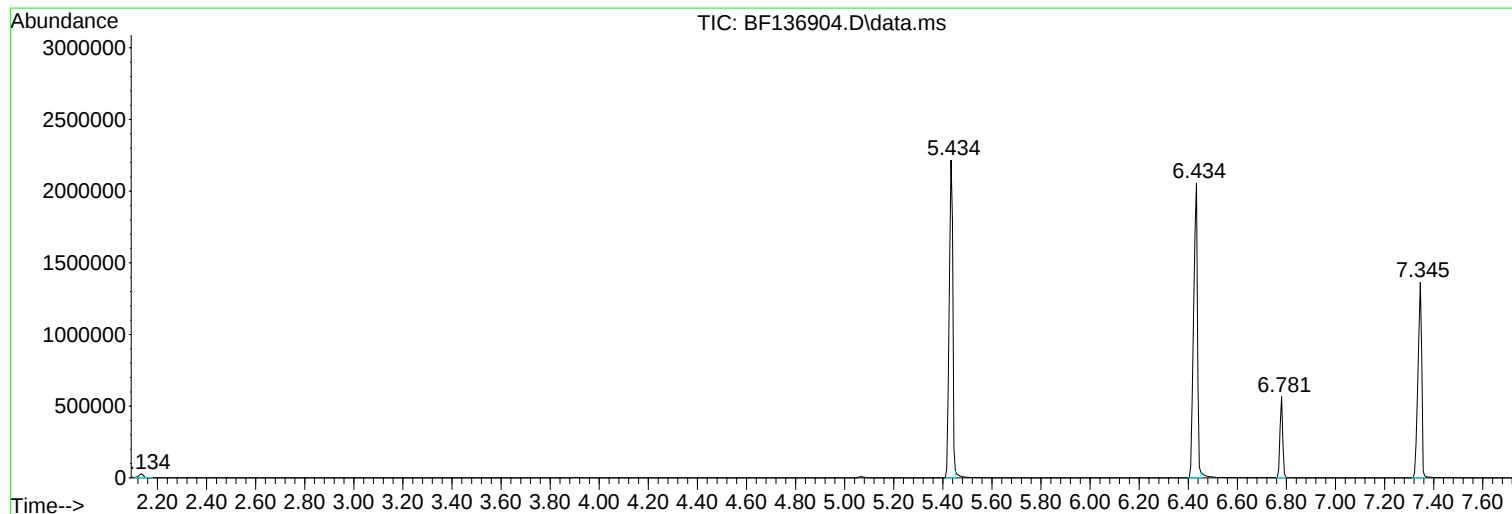

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136904.D
Acq On : 03 Jan 2024 13:08
Operator : CG\JU
Sample : PB158147BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158147BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136904.D
Acq On : 03 Jan 2024 13:08
Operator : CG\JU
Sample : PB158147BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158147BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------