


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136898.D
Acq On : 03 Jan 2024 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

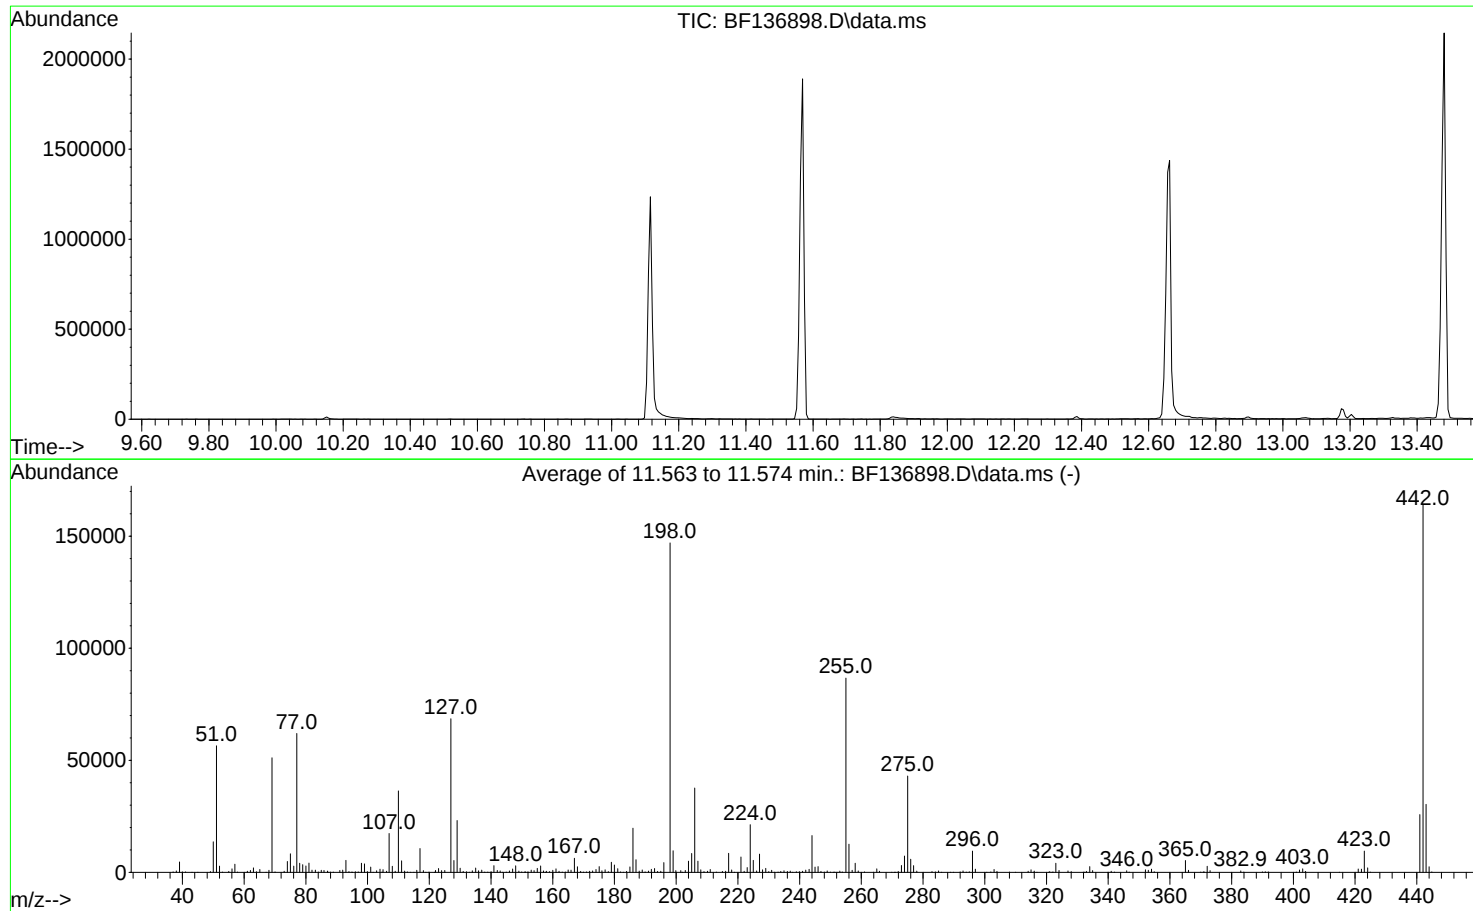

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	56457	PASS
68	69	0.00	2	1.9	958	PASS
69	198	0.00	100	34.8	51151	PASS
70	69	0.00	2	0.4	210	PASS
127	198	10	80	46.6	68549	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	147029	PASS
199	198	5	9	6.6	9662	PASS
275	198	10	60	29.2	42981	PASS
365	198	1	100	3.6	5278	PASS
441	198	0.01	100	17.5	25789	PASS
442	442	50	100	100.0	164157	PASS
443	442	15	24	18.5	30347	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/3/2024	BNA_F	<u>BF136898.D</u>
Compound Name	Response	Retention Time
DDT	379659	13.48
DDD	15101	13.174
DDE	279	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15380	395039	3.89

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
 Data File : BF136898.D
 Acq On : 03 Jan 2024 09:43
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 04 01:43:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

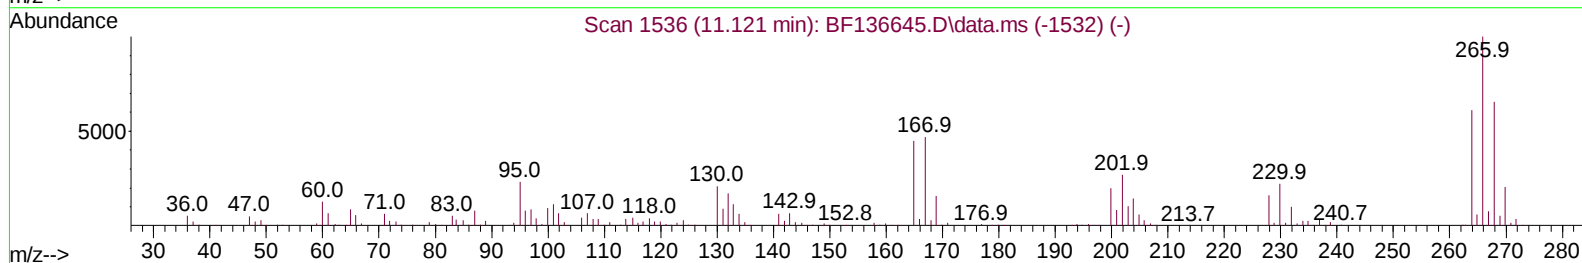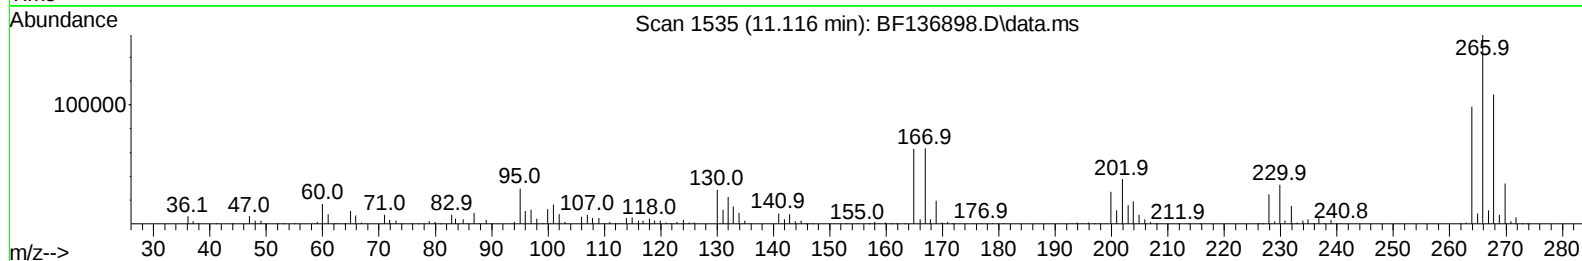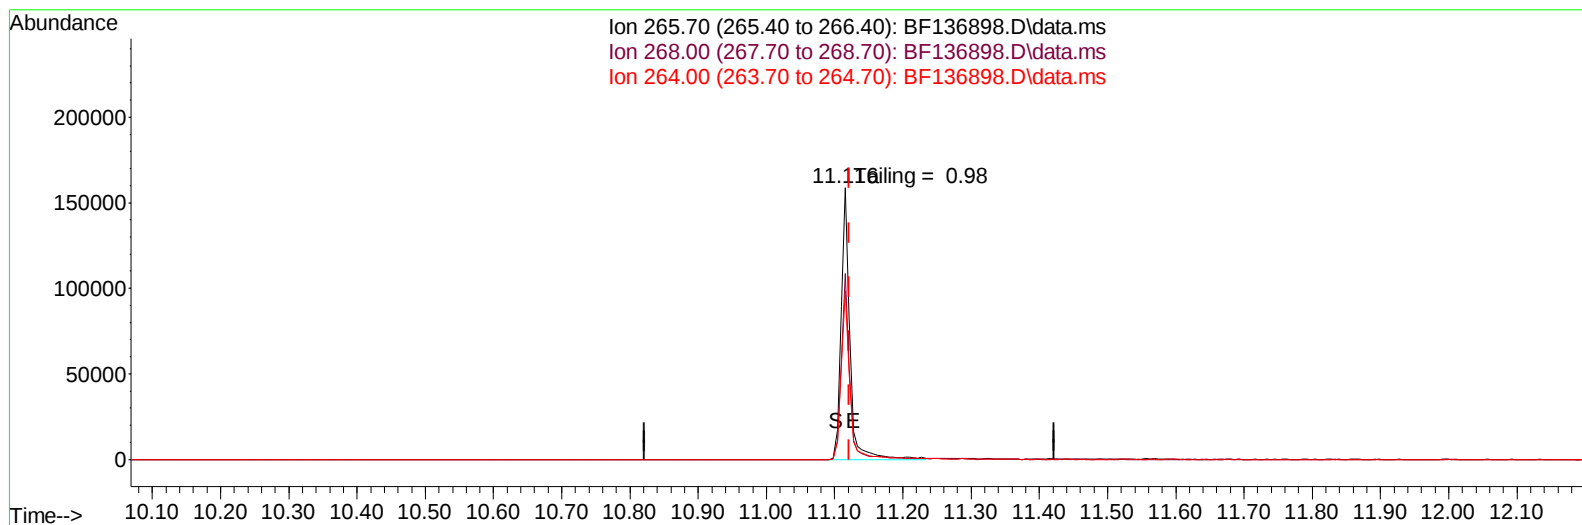

TIC: BF136898.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.006) 45192.86 ng




response 141564

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	68.39
264.00	61.20	62.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136898.D
Acq On : 03 Jan 2024 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 04 01:43:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

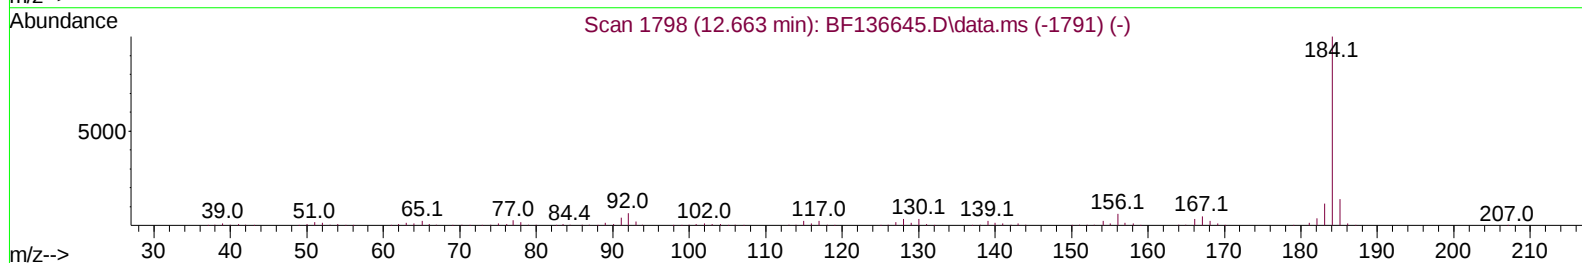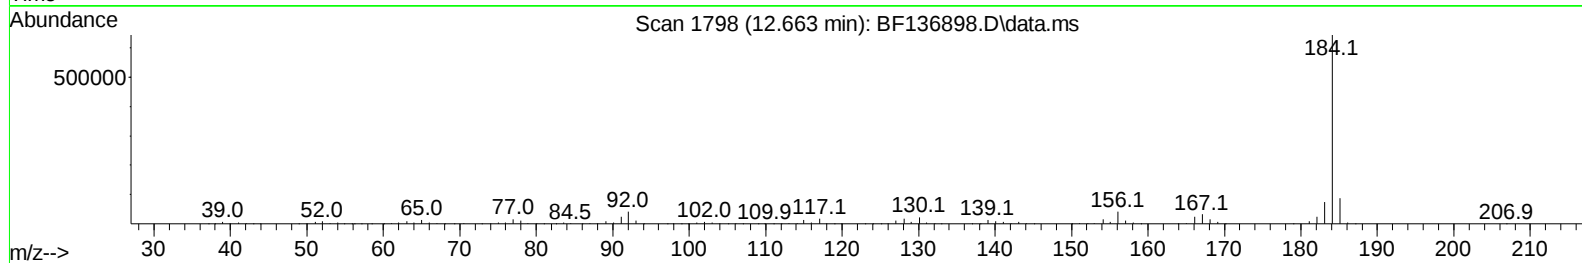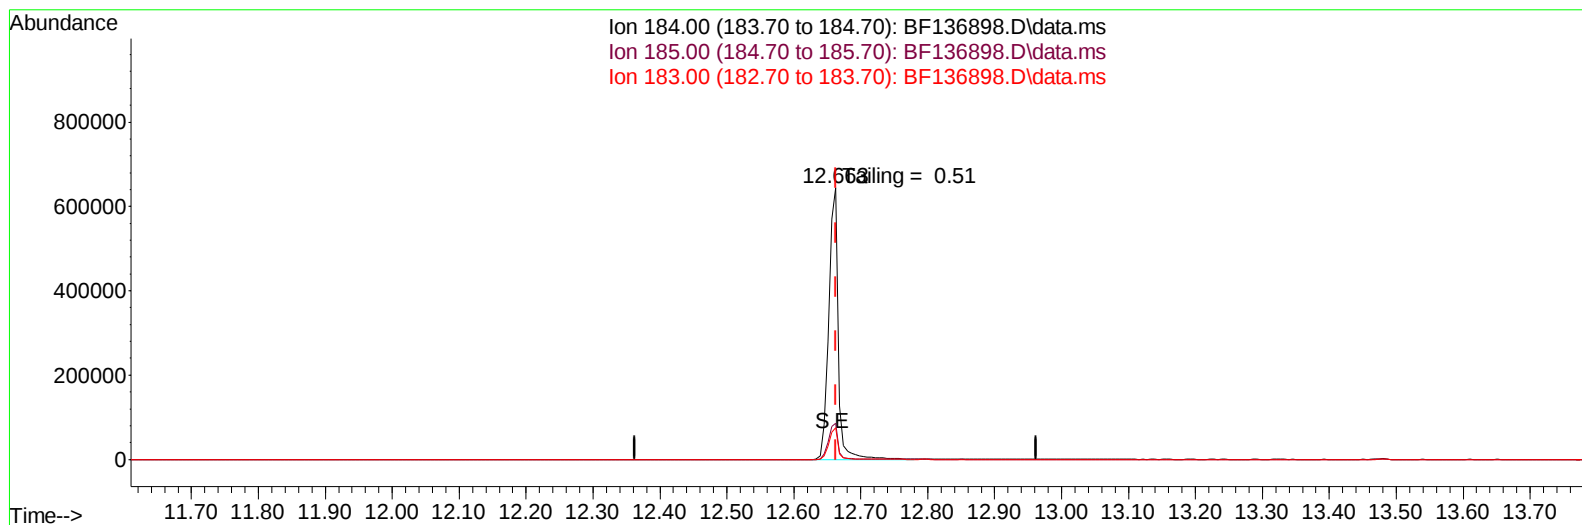

TIC: BF136898.D\data.ms

(77) Benzidine

12.663min (+ 0.000) 62203.34 ng

response 649275

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.45
183.00	11.60	11.60
0.00	0.00	0.00