
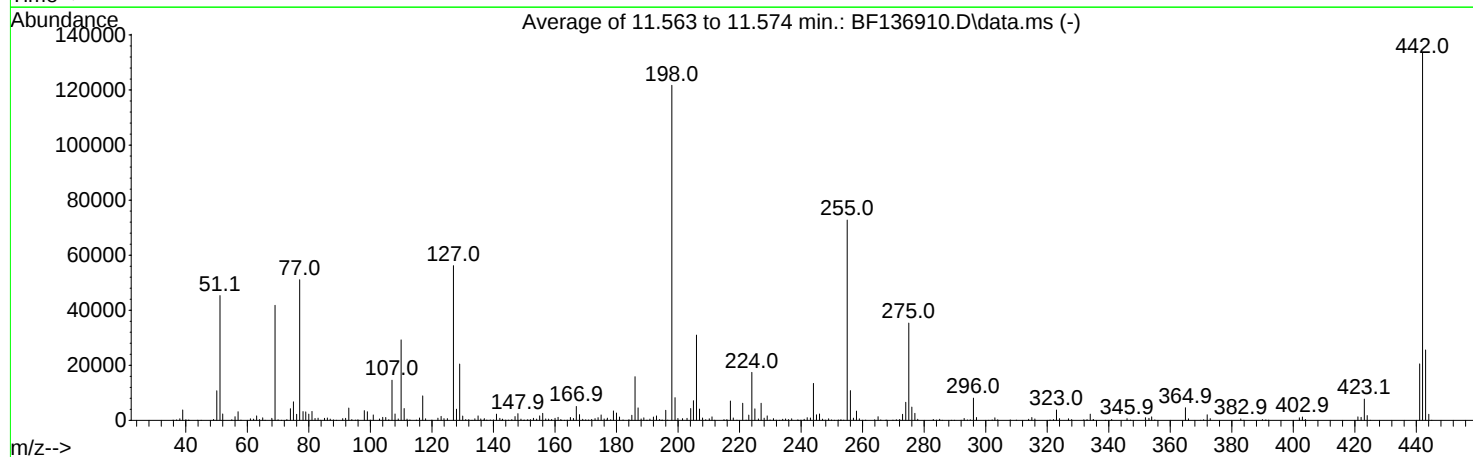


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136910.D
Acq On : 03 Jan 2024 16:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

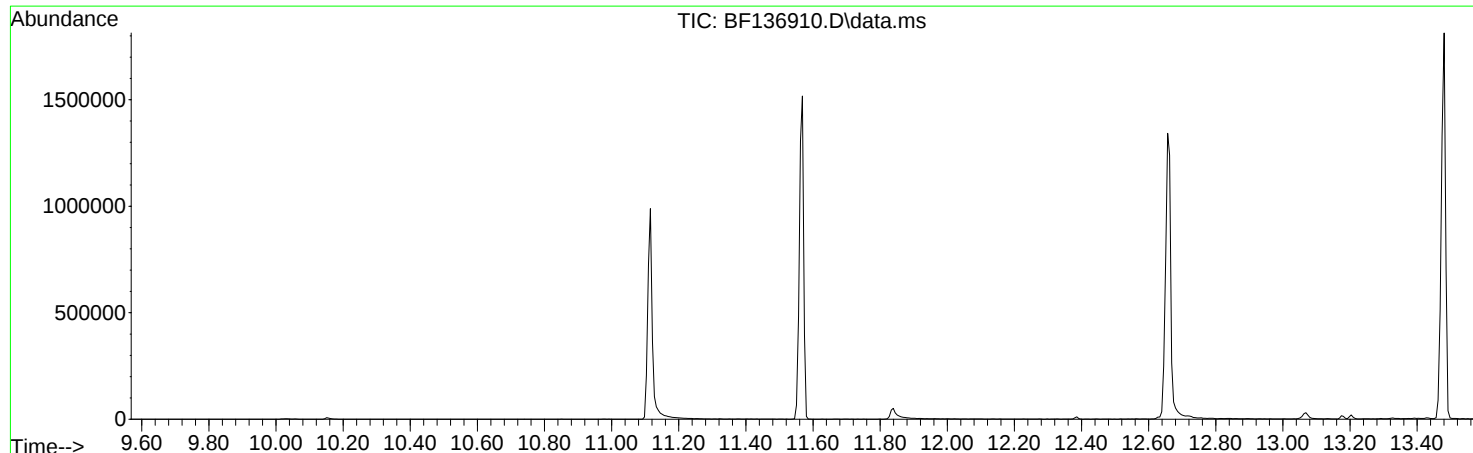

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	45349	PASS
68	69	0.00	2	1.8	761	PASS
69	198	0.00	100	34.3	41788	PASS
70	69	0.00	2	0.6	255	PASS
127	198	10	80	46.2	56222	PASS
197	198	0.00	2	0.1	121	PASS
198	198	100	100	100.0	121707	PASS
199	198	5	9	6.8	8237	PASS
275	198	10	60	29.1	35356	PASS
365	198	1	100	3.8	4571	PASS
441	198	0.01	100	16.9	20548	PASS
442	442	50	100	100.0	133637	PASS
443	442	15	24	19.1	25557	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/3/2024	BNA_F	<u>BF136910.D</u>
Compound Name	Response	Retention Time
DDT	332352	13.48
DDD	6303	13.204
DDE	460	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6763	339115	1.99

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136910.D
Acq On : 03 Jan 2024 16:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 04 01:45:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

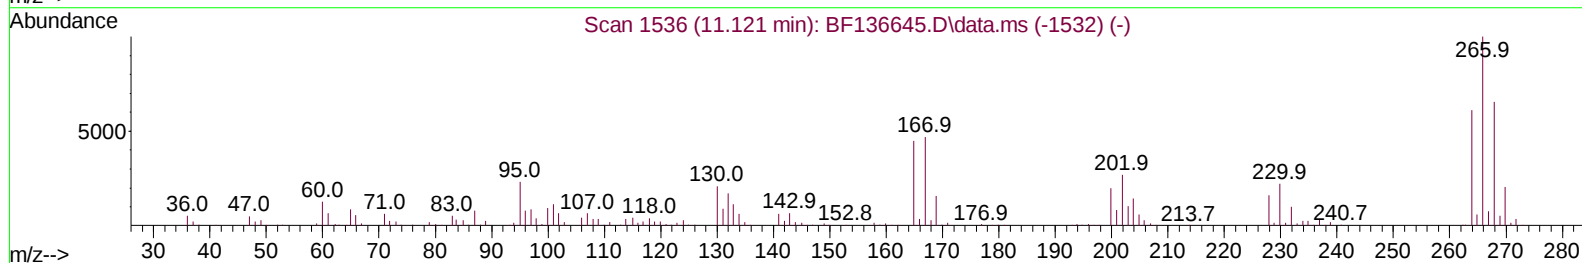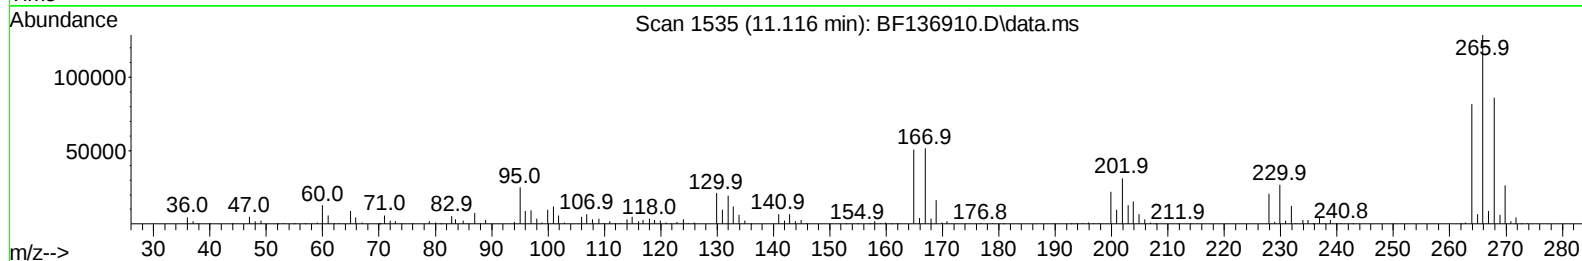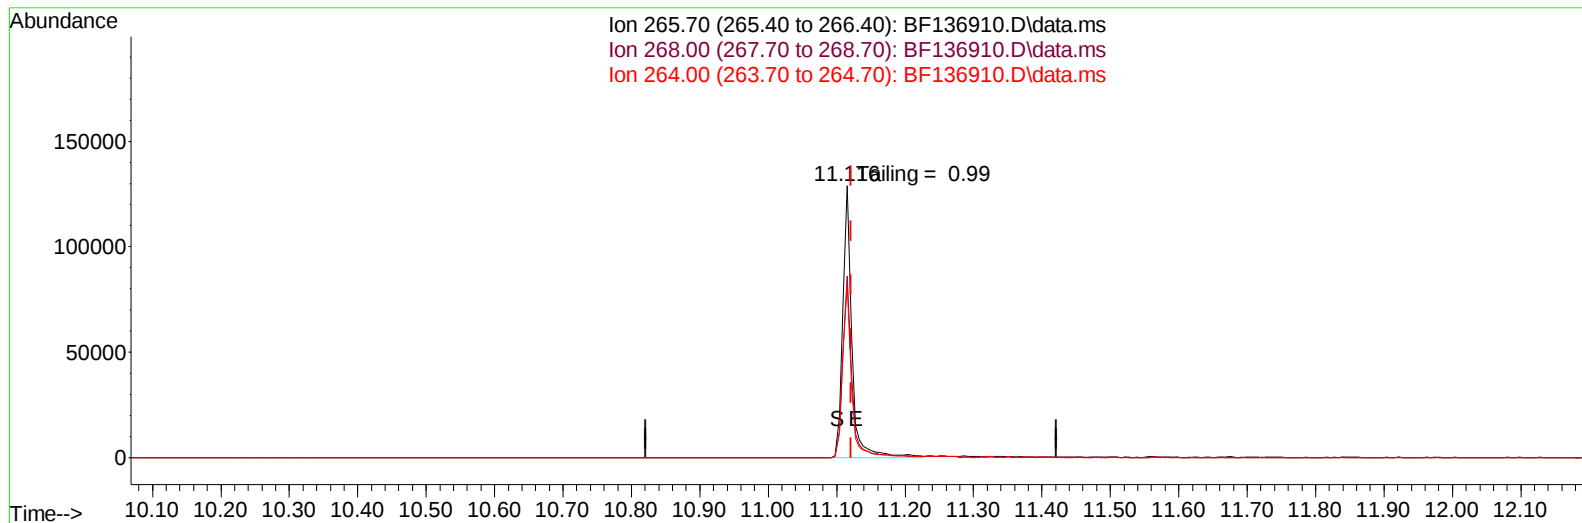

TIC: BF136910.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.006) 33758.15 ng




response 117430

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	66.92
264.00	61.20	63.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010324\
Data File : BF136910.D
Acq On : 03 Jan 2024 16:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 04 01:45:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

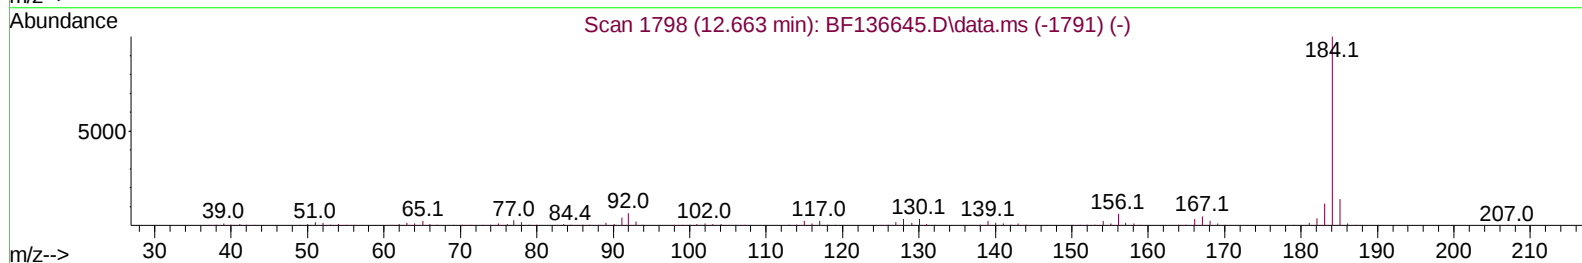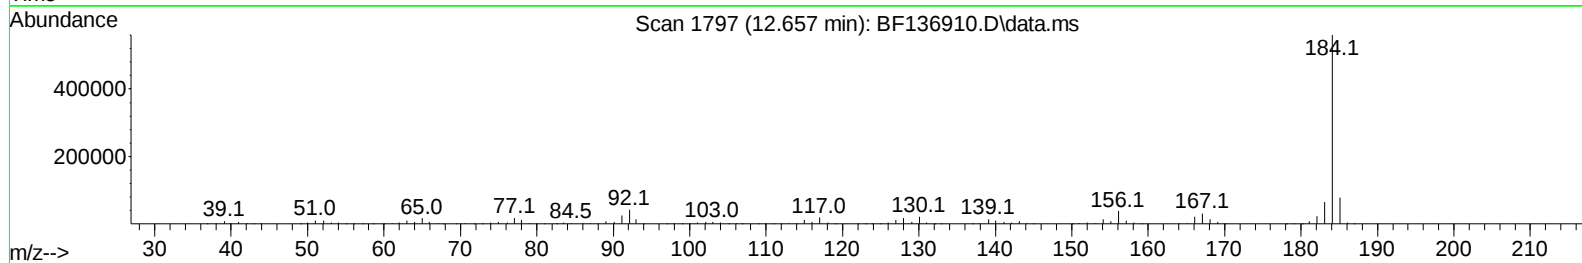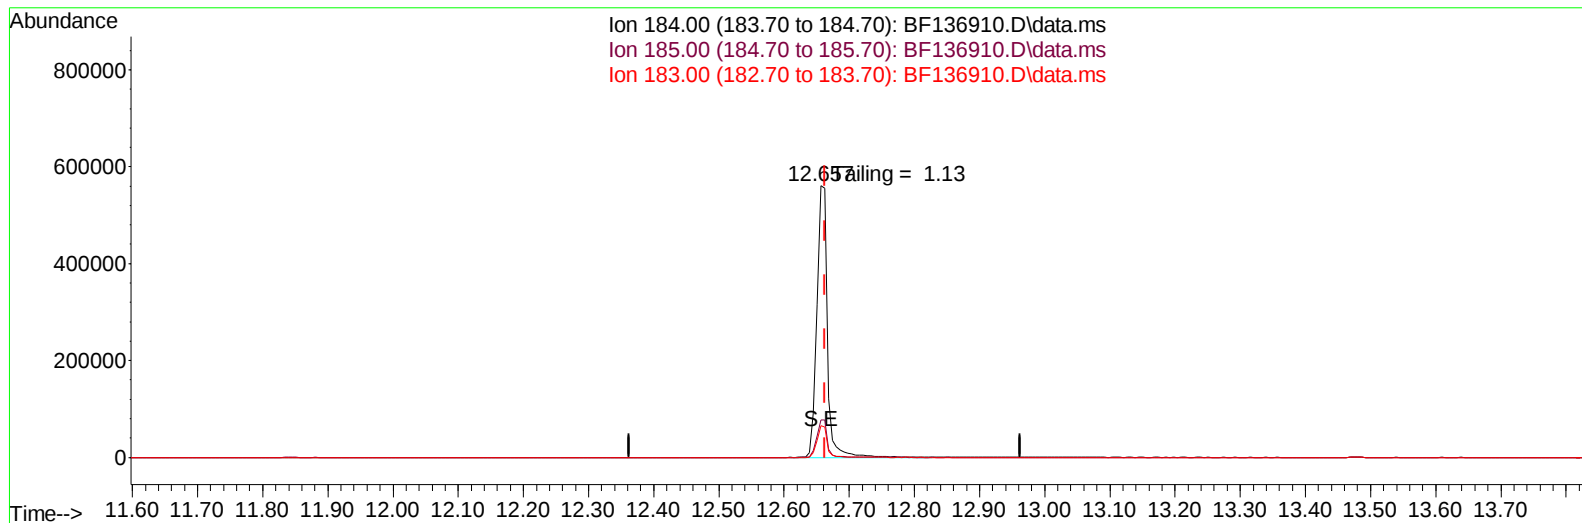

TIC: BF136910.D\data.ms

(77) Benzidine

12.657min (-0.006) 0.00 ng

response 634371

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.82
183.00	11.60	11.63
0.00	0.00	0.00