
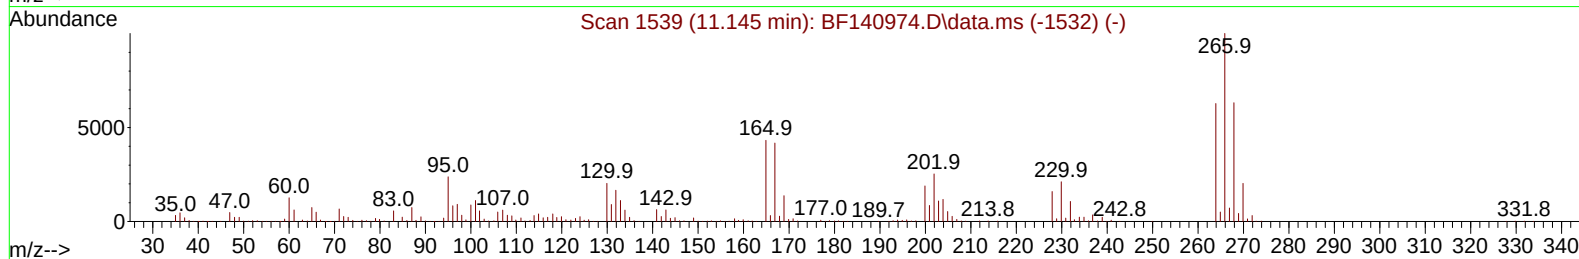
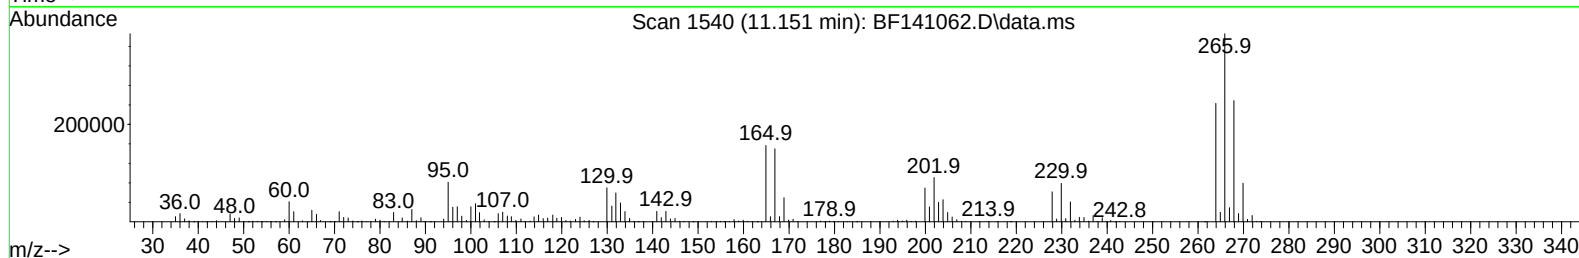


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010325\
Data File : BF141062.D
Acq On : 03 Jan 2025 10:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 12:00:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

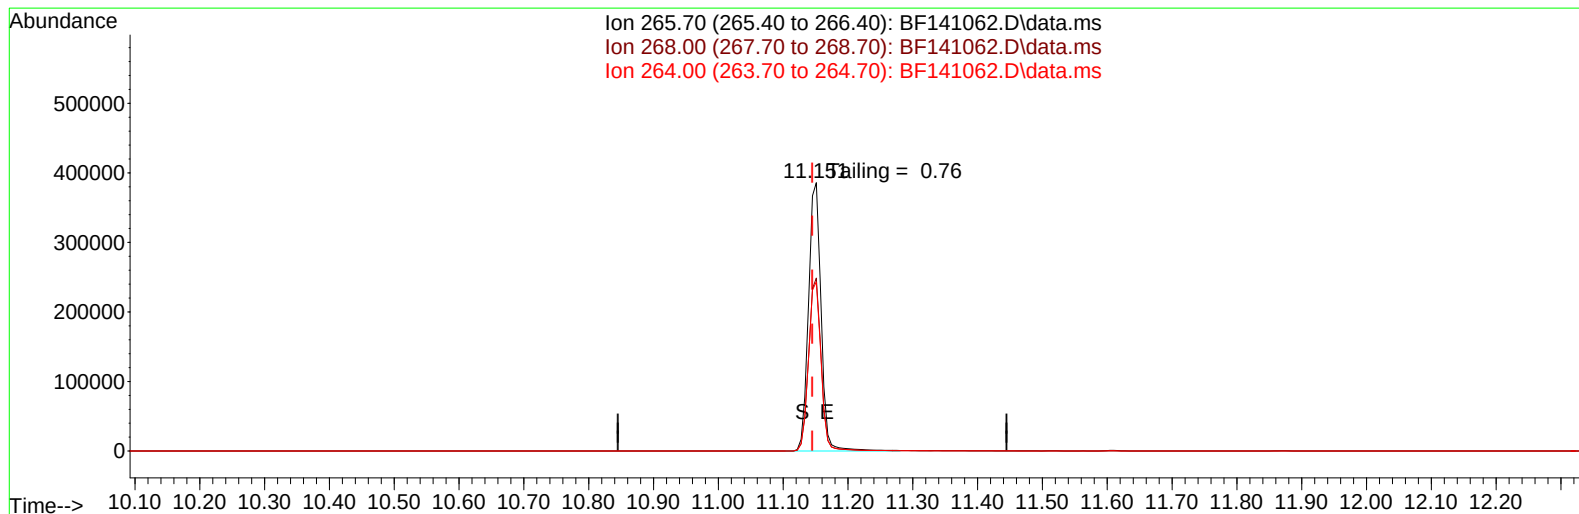

TIC: BF141062.D\data.ms

(70) Pentachlorophenol (C)




11.151min (+ 0.006) 98688.99 ng

response 522943

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.43
264.00	62.80	63.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010325\
Data File : BF141062.D
Acq On : 03 Jan 2025 10:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 12:00:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

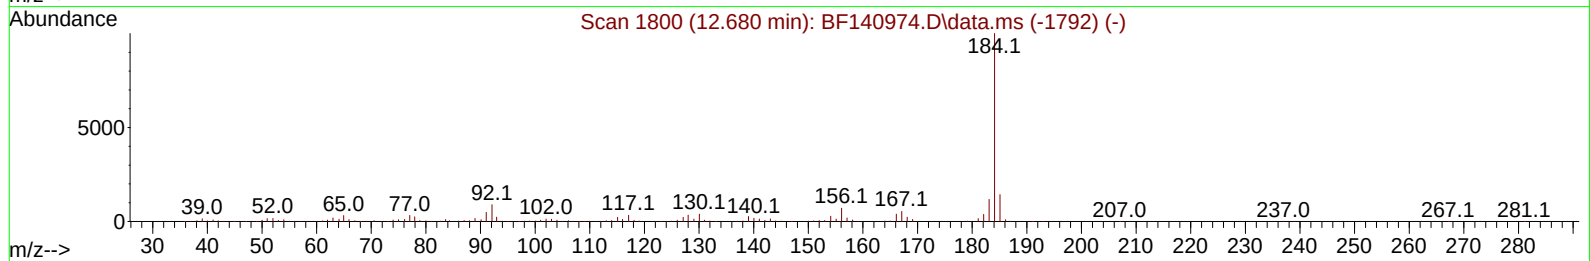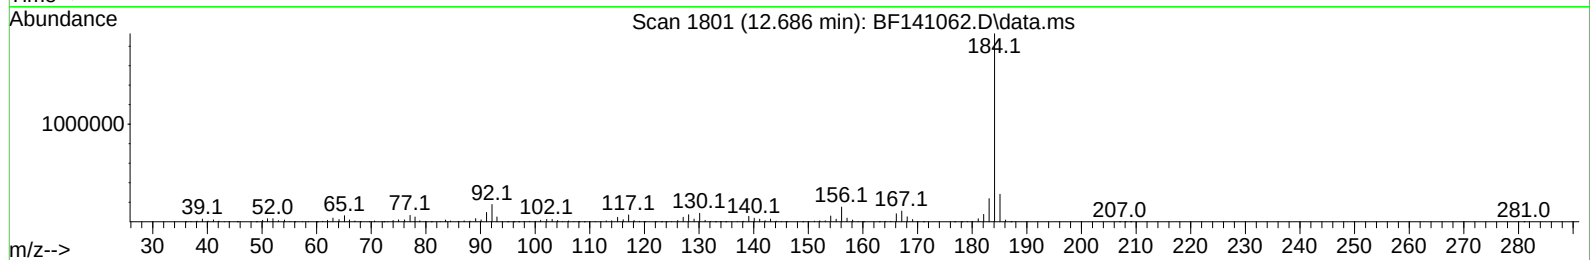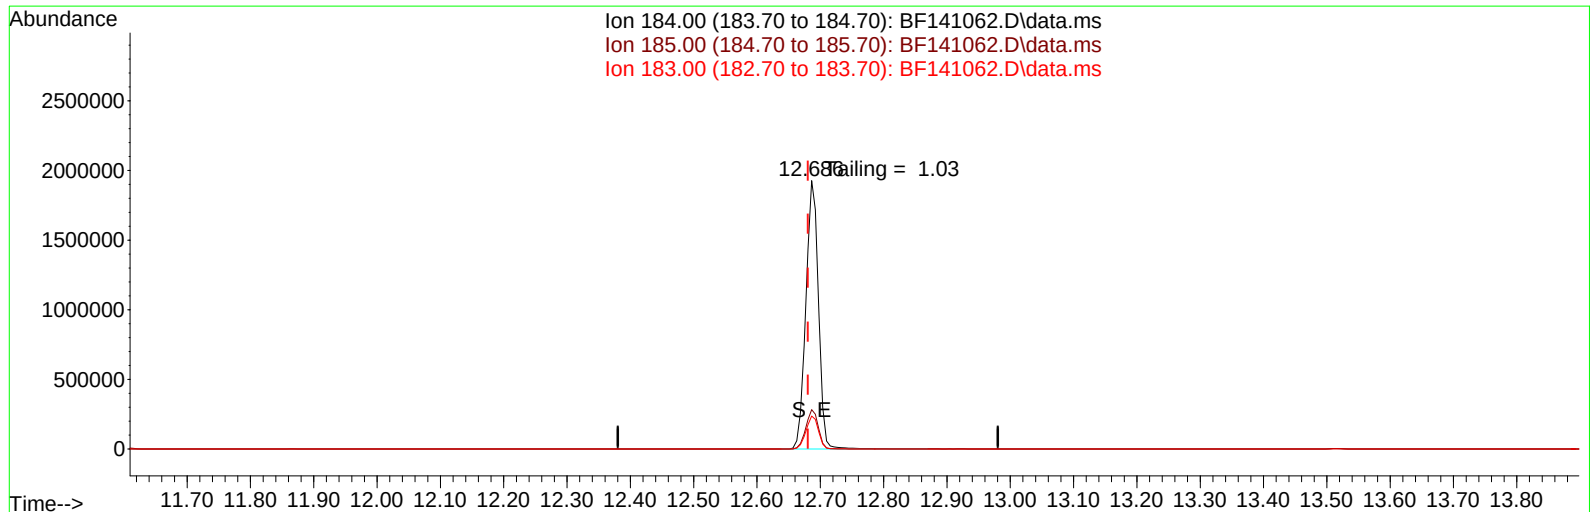

TIC: BF141062.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 65120.53 ng

response 2680950

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.68
183.00	11.70	12.33
0.00	0.00	0.00