


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010325\
Data File : BF141062.D
Acq On : 03 Jan 2025 10:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 27 00:31:16 2024

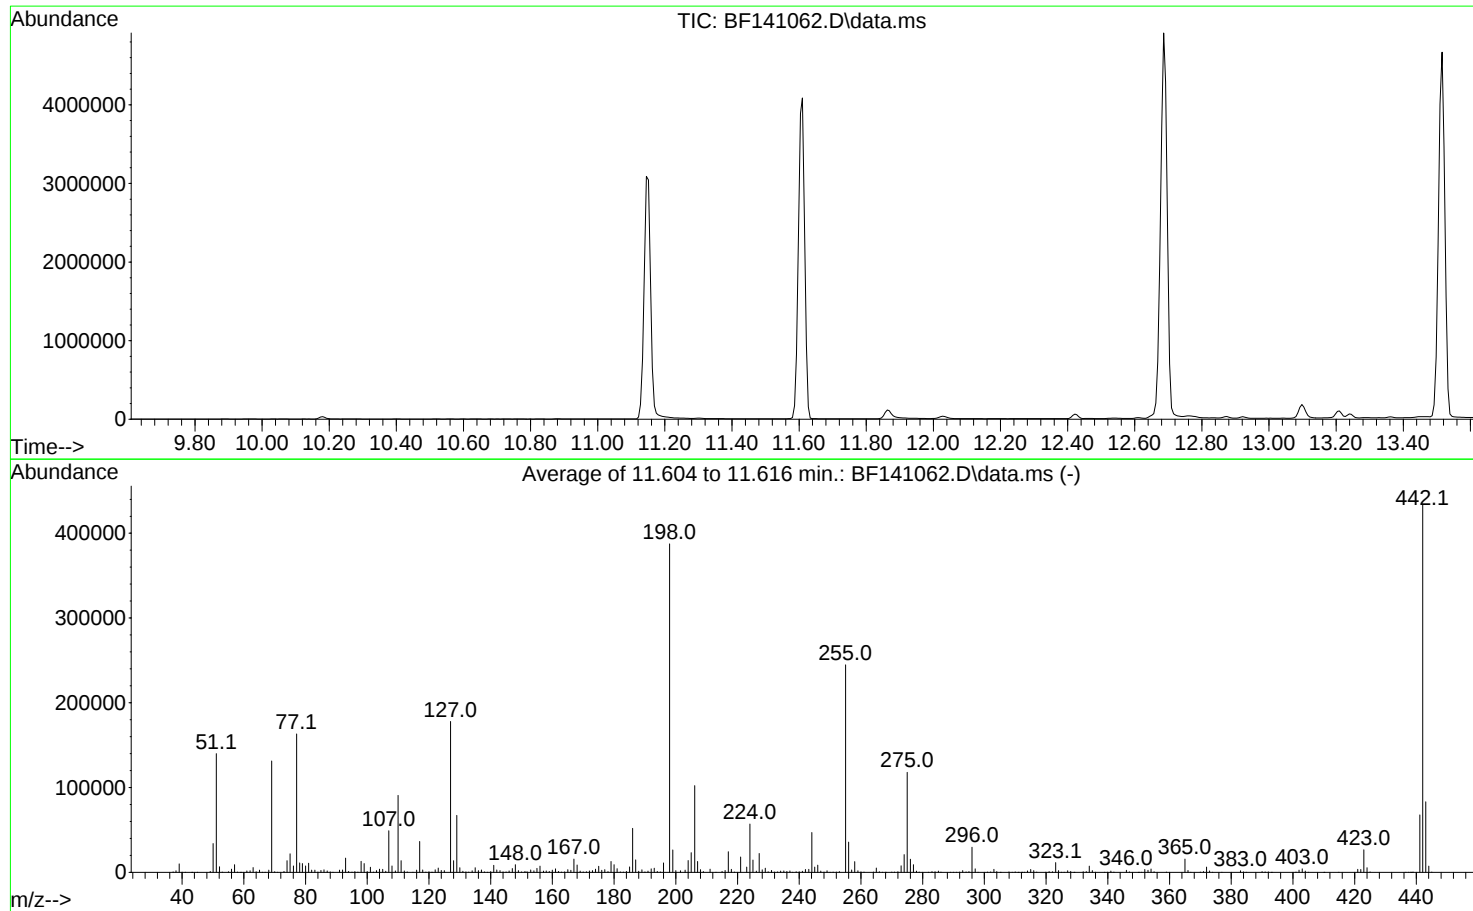

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	140083	PASS
68	69	0.00	2	2.0	2563	PASS
69	198	0.00	100	33.9	131296	PASS
70	69	0.00	2	0.6	778	PASS
127	198	10	80	45.9	177941	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	387499	PASS
199	198	5	9	6.8	26453	PASS
275	198	10	60	30.5	118032	PASS
365	198	1	100	4.0	15586	PASS
441	198	0.01	100	17.5	67832	PASS
442	442	50	100	100.0	433877	PASS
443	442	15	24	19.2	83237	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/3/2025	BNA_F	<u>BF141062.D</u>
Compound Name	Response	Retention Time
DDT	1171841	13.516
DDD	34253	13.21
DDE	3566	12.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37819	1209660	3.13

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010325\
Data File : BF141062.D
Acq On : 03 Jan 2025 10:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 03 12:00:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

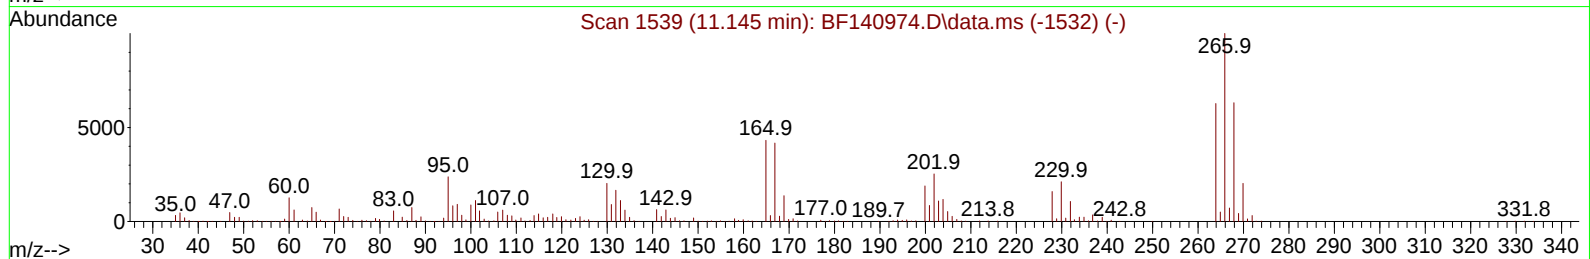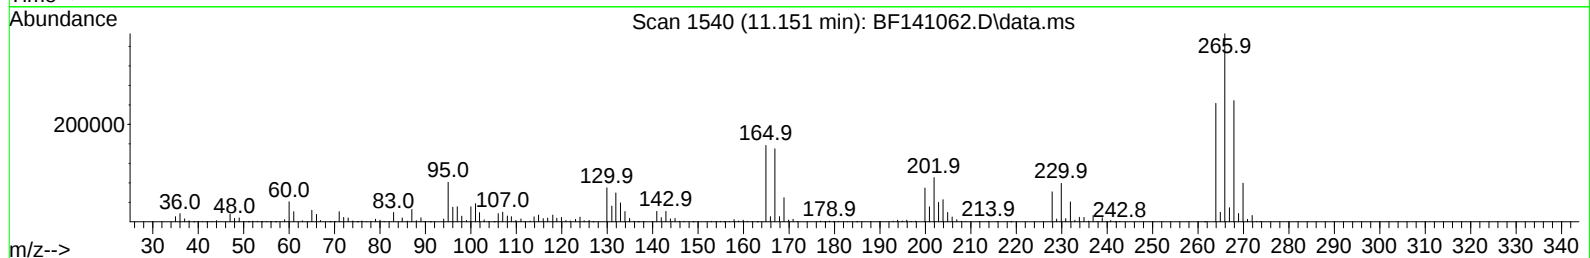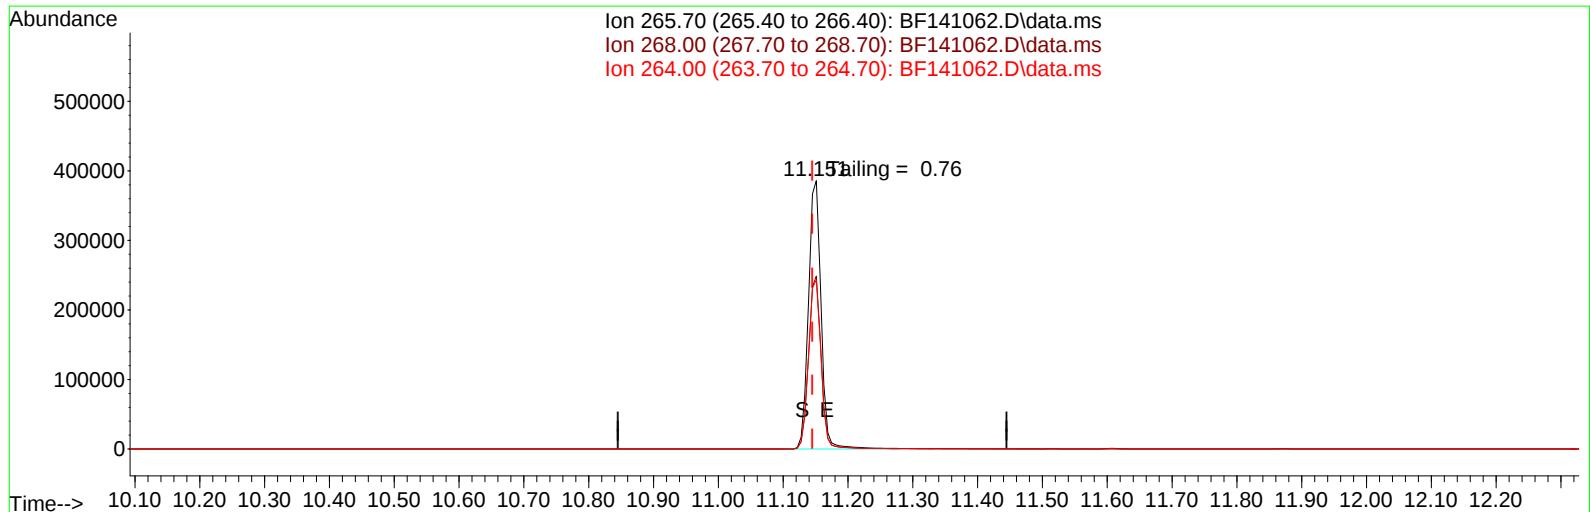

TIC: BF141062.D\data.ms

(70) Pentachlorophenol (C)

11.151min (+ 0.006) 98688.99 ng




response 522943

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.43
264.00	62.80	63.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010325\
Data File : BF141062.D
Acq On : 03 Jan 2025 10:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 03 12:00:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

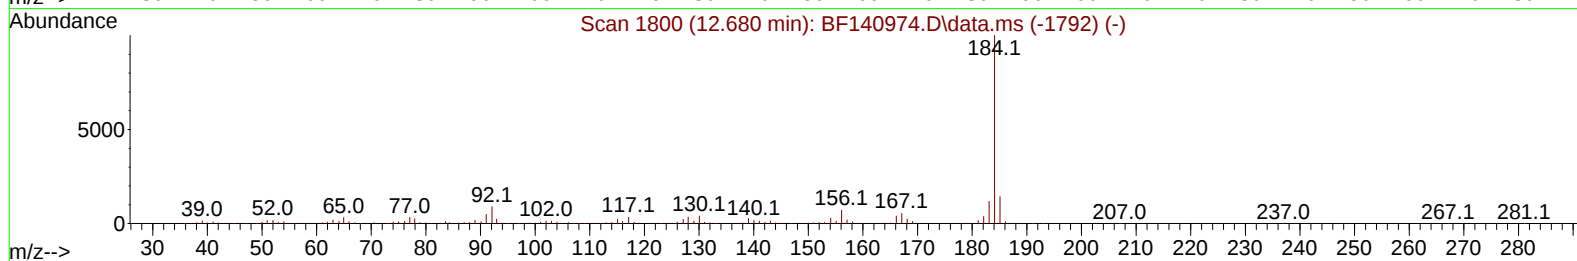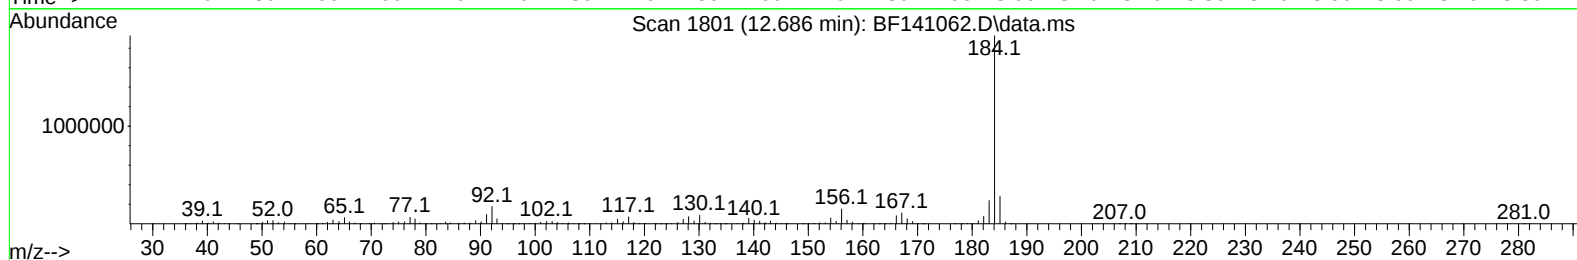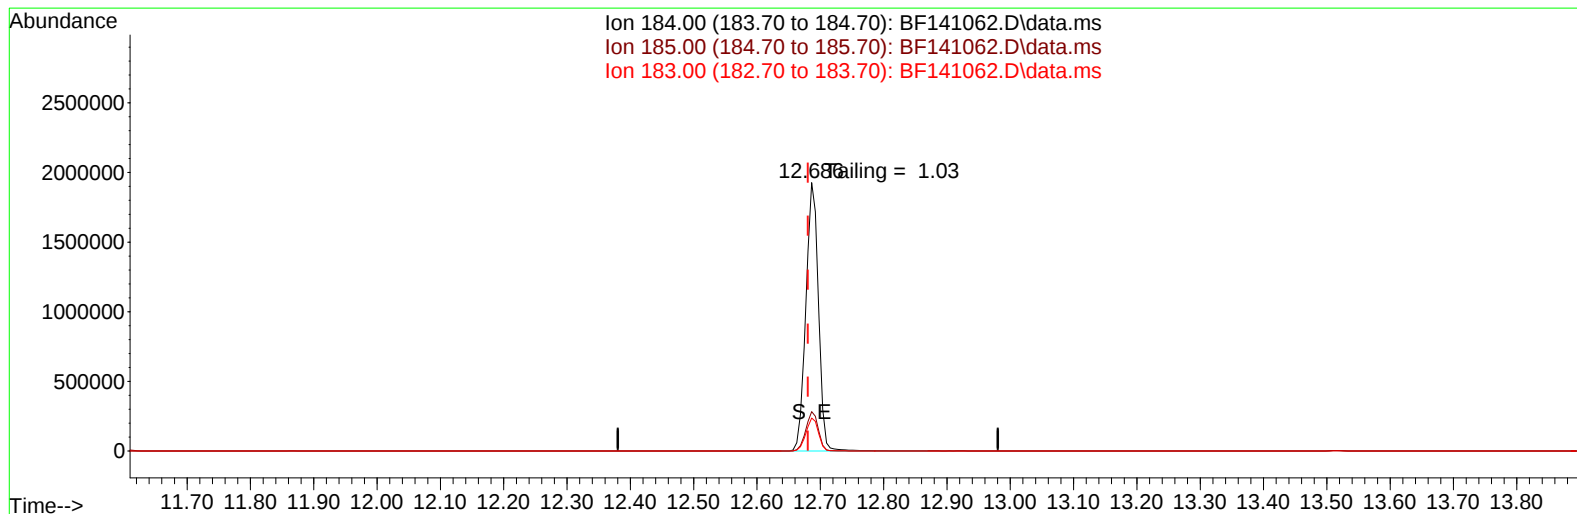

TIC: BF141062.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 65120.53 ng

response 2680950

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.68
183.00	11.70	12.33
0.00	0.00	0.00