
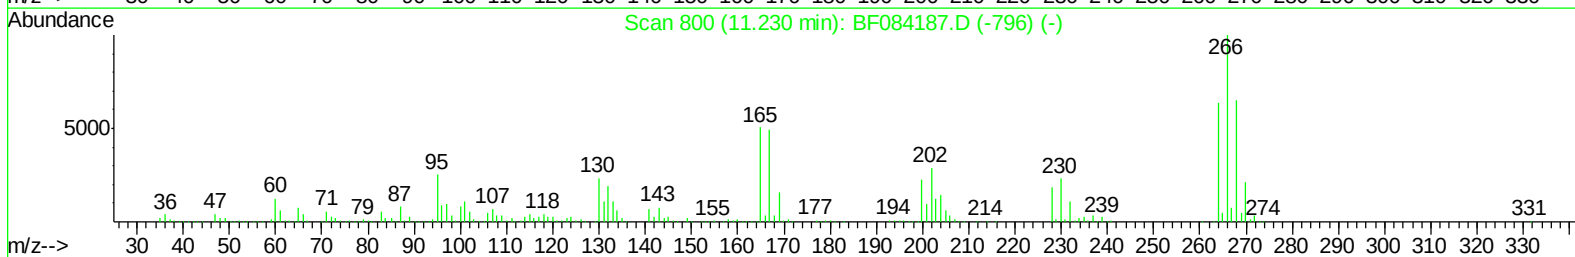
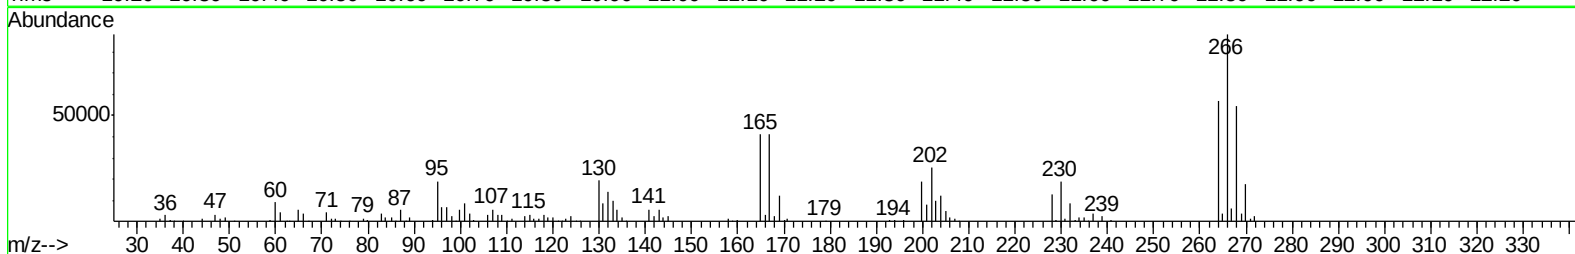


Data Path : Z:\HPCHEM1\BNA F\Data\BF010416\
Data File : BF084253.D
Acq On : 4 Jan 2016 23:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 06:09:08 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 12:22:40 2016
Response via : Initial Calibration

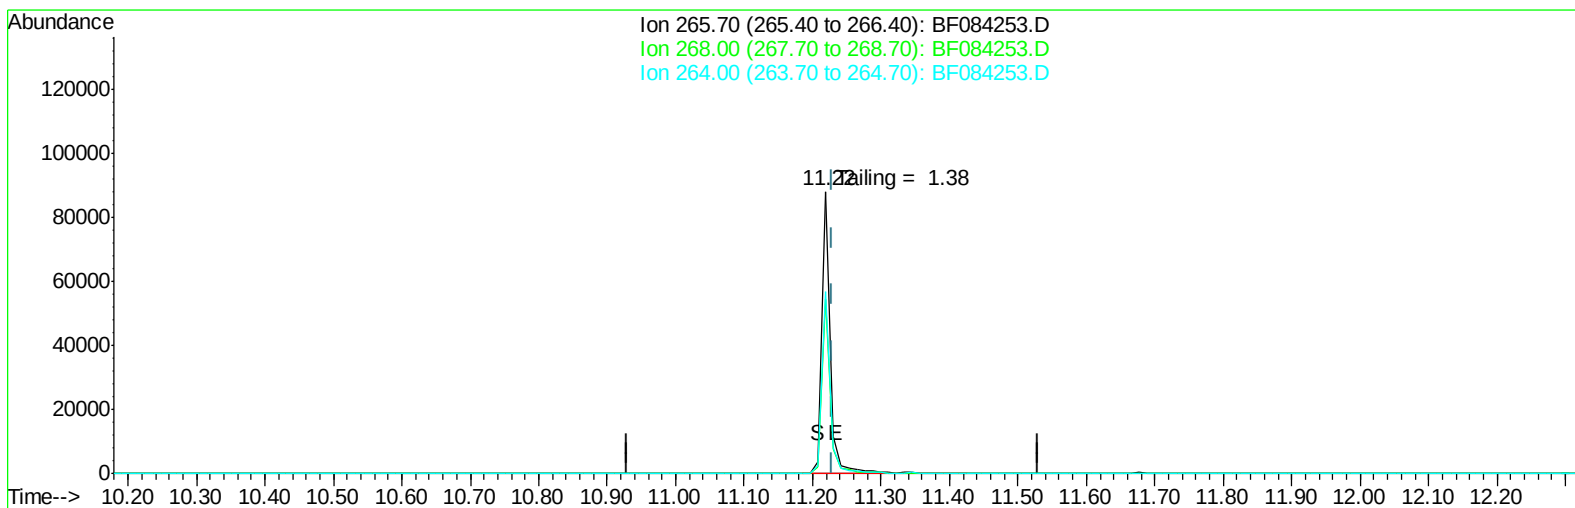

TIC: BF084253.D

(69) Pentachlorophenol (C)




11.219min (-0.011) 0.00ng

response 76129

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	61.74
264.00	62.70	64.55
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF010416\
Data File : BF084253.D
Acq On : 4 Jan 2016 23:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 06:09:08 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 12:22:40 2016
Response via : Initial Calibration

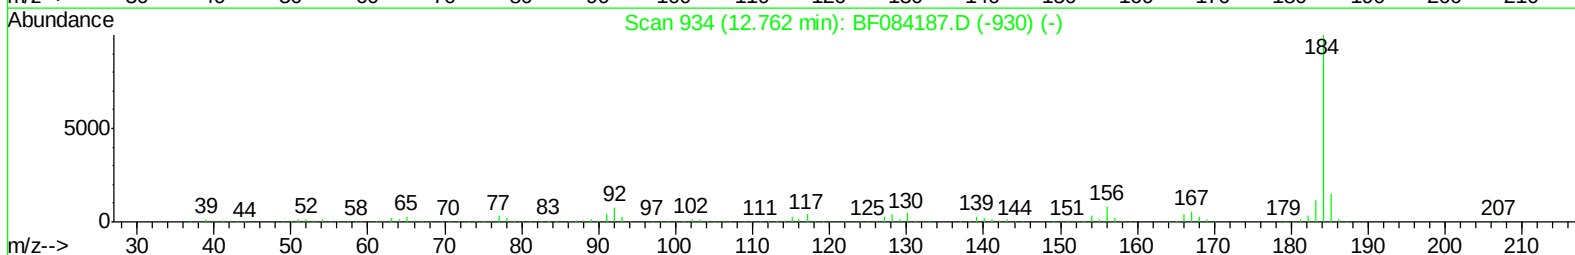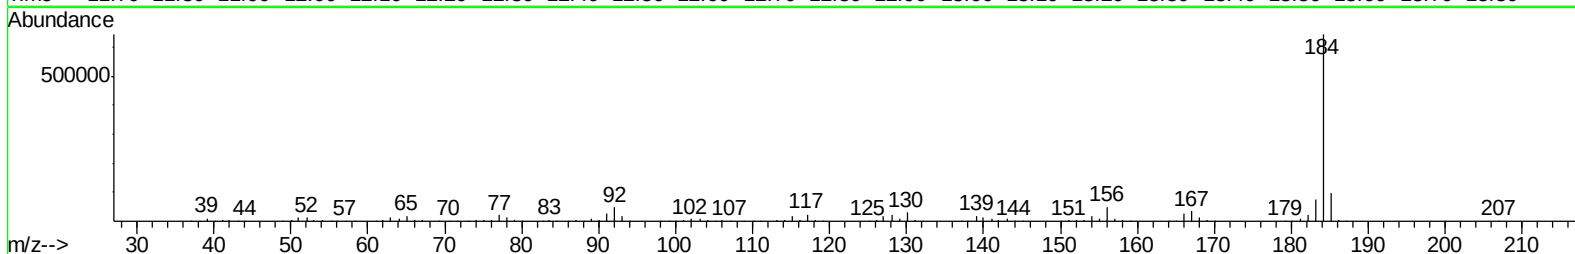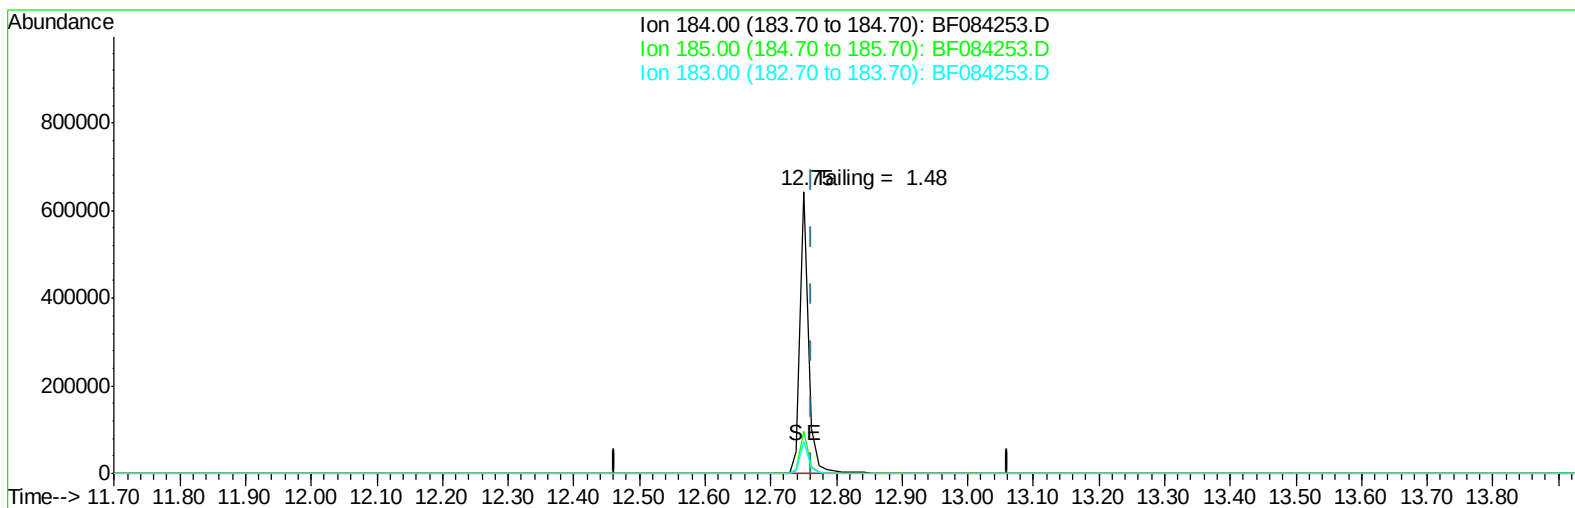

TIC: BF084253.D

(76) Benzidine

12.751min (-0.011) 0.00ng

response 579385

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.86
183.00	12.30	11.59
0.00	0.00	0.00