

Data Path : Z:\HPCHEM1\BNA F\DATA\BF010416\
 Data File : BF084249.D
 Acq On : 4 Jan 2016 19:57
 Operator : UM/SJ
 Sample : G4986-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PJ-SB-4-1.5-2.0

Quant Time: Jan 05 02:55:05 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 04 12:22:40 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	263846	20.00	ng	-0.01
21) Naphthalene-d8	8.18	136	1136378	20.00	ng	-0.01
38) Acenaphthene-d10	9.93	164	485746	20.00	ng	-0.02
63) Phenanthrene-d10	11.41	188	818244	20.00	ng	-0.01
75) Chrysene-d12	14.05	240	575692	20.00	ng	-0.01
86) Perylene-d12	15.49	264	544993	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	1427629	87.52	ng	0.01
7) Phenol-d6	6.53	99	1717017	83.81	ng	0.00
23) Nitrobenzene-d5	7.46	82	1338131	65.54	ng	-0.01
41) 2,4,6-Tribromophenol	10.73	330	477066	97.28	ng	-0.01
44) 2-Fluorobiphenyl	9.25	172	1724656	60.65	ng	-0.01
78) Terphenyl-d14	13.00	244	1358408	52.67	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.65	163	538652	15.51	ng	Qvalue # 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF010416\
Data File : BF084249.D
Acq On : 4 Jan 2016 19:57
Operator : UM/SJ
Sample : G4986-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PJ-SB-4-1.5-2.0

Quant Time: Jan 05 02:55:05 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 12:22:40 2016
Response via : Initial Calibration

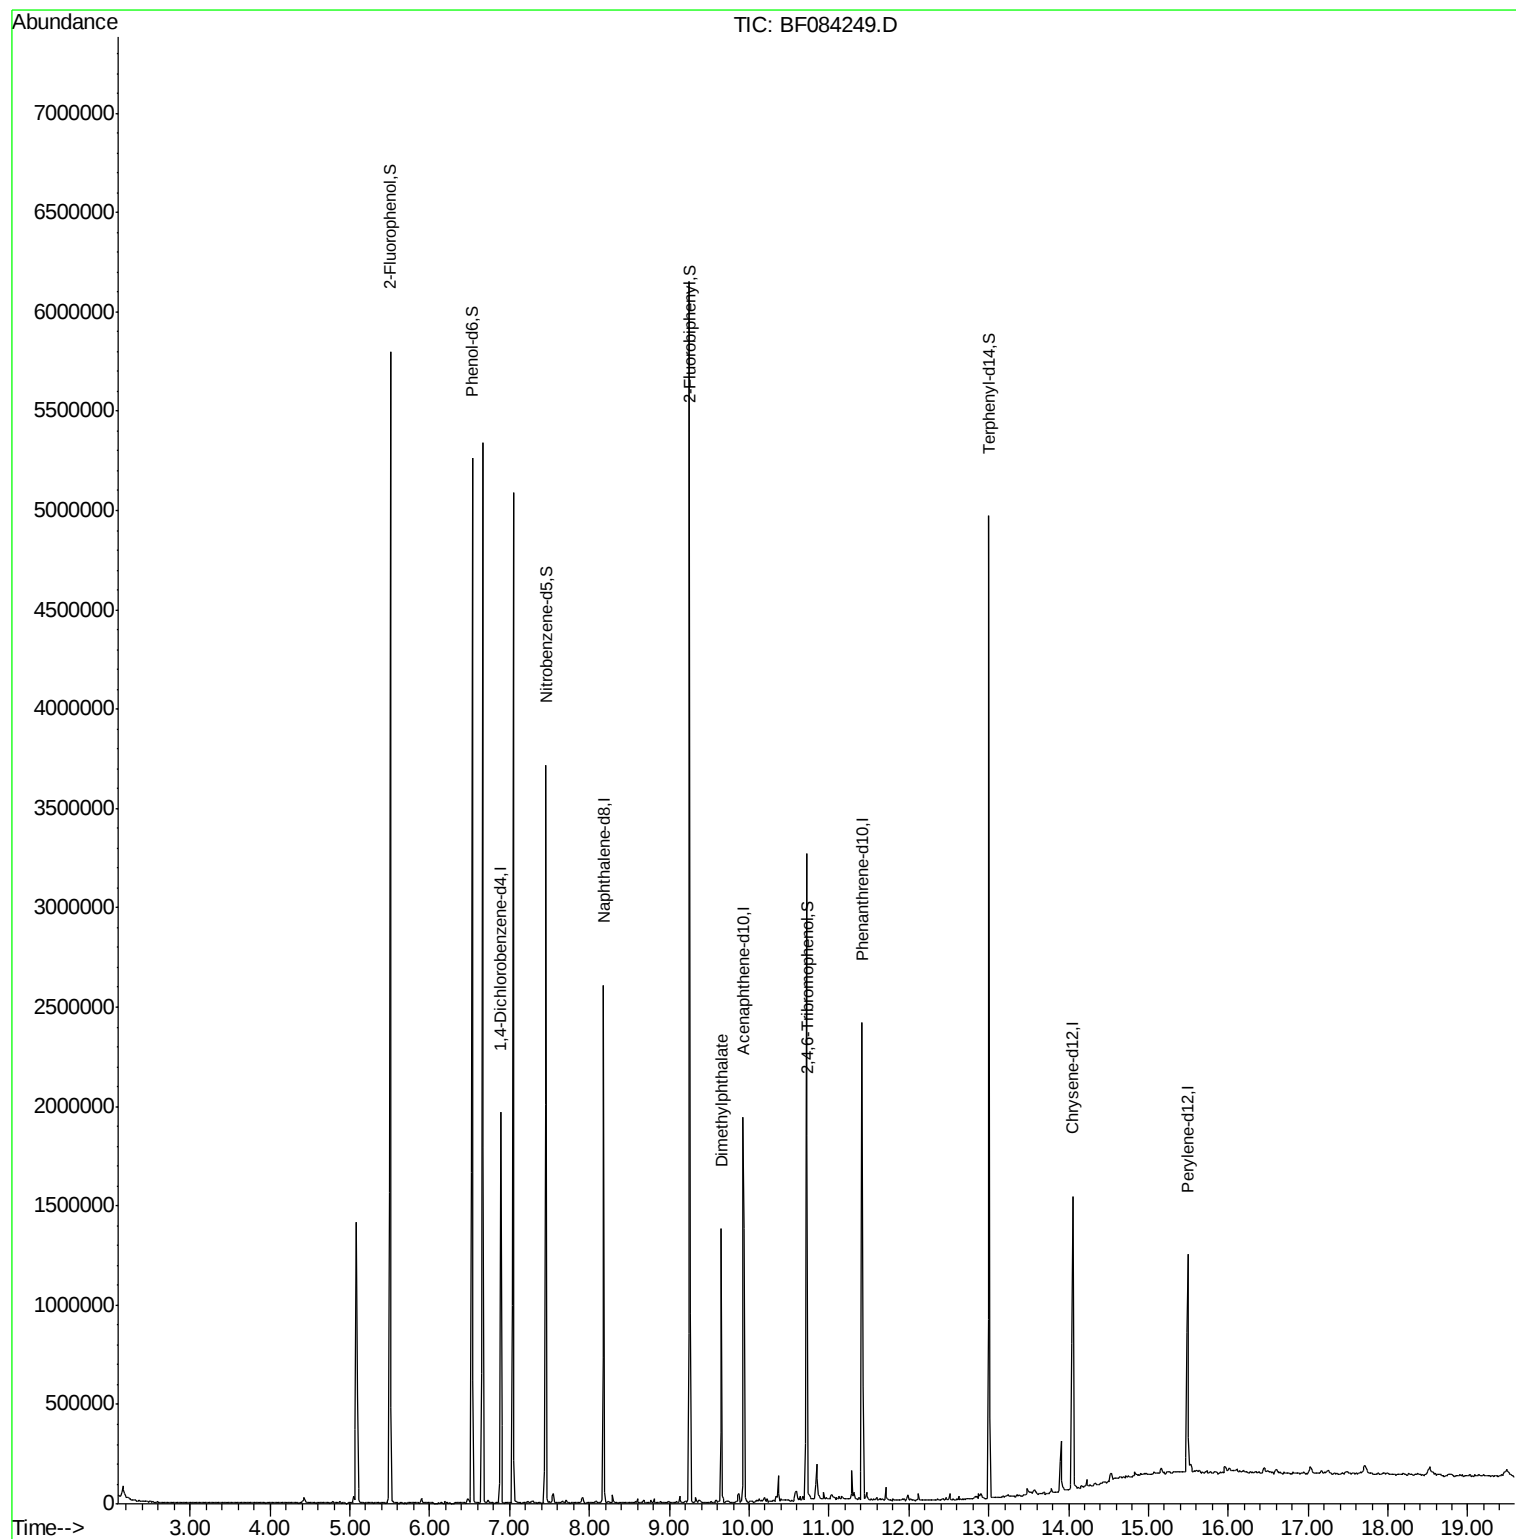



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.89 min Scan# 420

Delta R.T. -0.01 min

Lab File: BF084249.D

Acq: 4 Jan 2016 19:57

Instrument :

BNA_F

ClientSampleId :

PJ-SB-4-1.5-2.0


Tot Ion:152 Resp: 263846

Ion Ratio Lower Upper

152 100

150 156.7 123.0 184.4




115 71.1 51.4 77.2

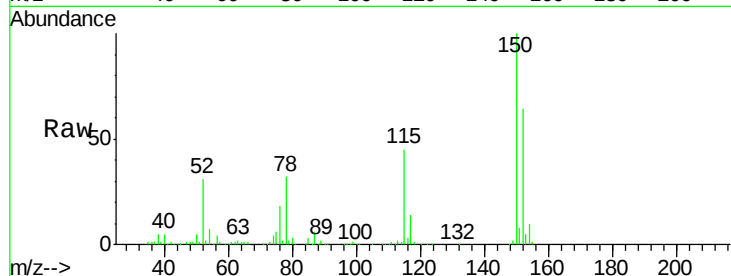

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

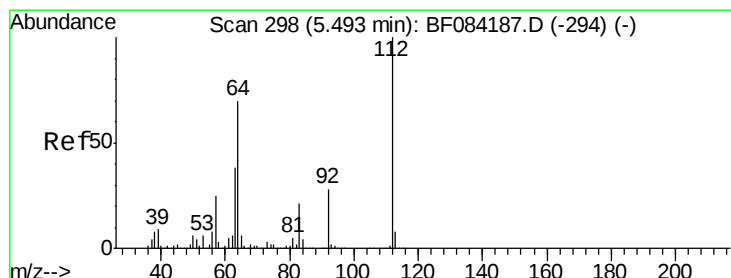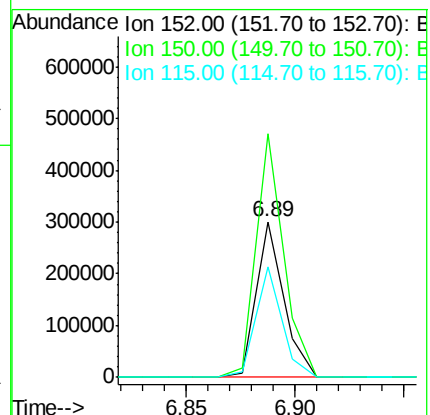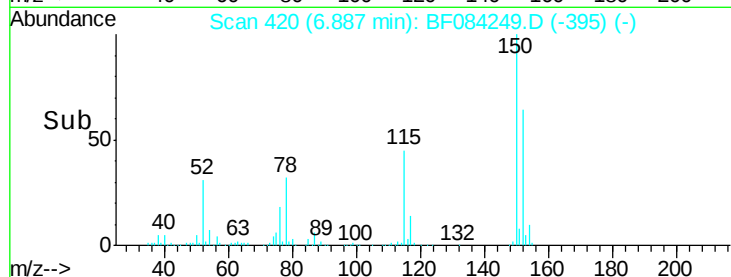

#5

2-Fluorophenol

Concen: 87.52 ng

RT: 5.50 min Scan# 299

Delta R.T. 0.01 min

Lab File: BF084249.D

Acq: 4 Jan 2016 19:57


Tgt Ion:112 Resp: 1427629

Ion Ratio Lower Upper

112 100

64 66.9 36.6 55.0#



63 36.0 19.4 29.0#

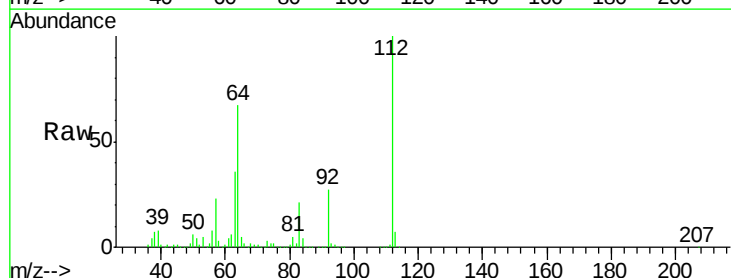

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

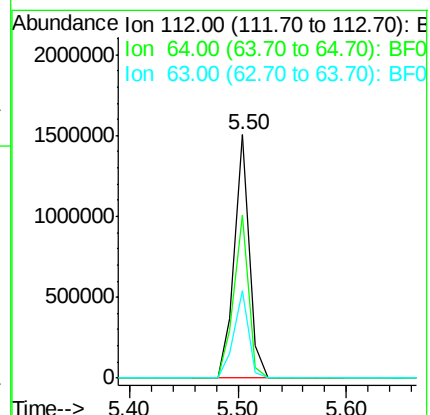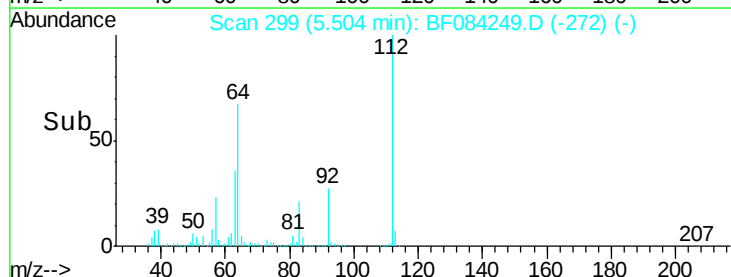



#7

Phenol-d6

Concen: 83.81 ng

RT: 6.53 min Scan# 389

Delta R.T. 0.00 min

Lab File: BF084249.D

Acq: 4 Jan 2016 19:57

Instrument :





BNA_F

ClientSampleId :

PJ-SB-4-1.5-2.0

Tot Ion: 99 Resp: 1717017

Ion	Ratio	Lower	Upper
99	100		
42	23.5	12.8	19.2#
71	39.4	30.9	46.3

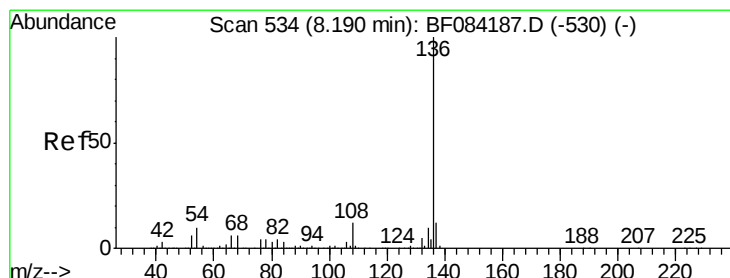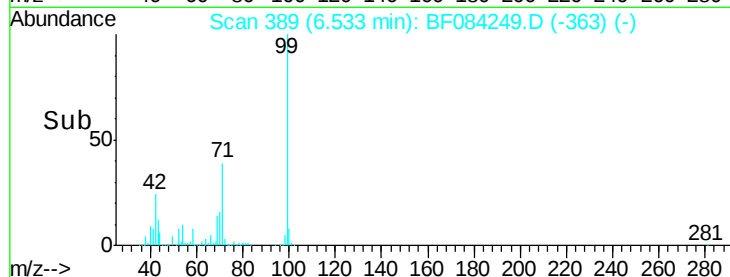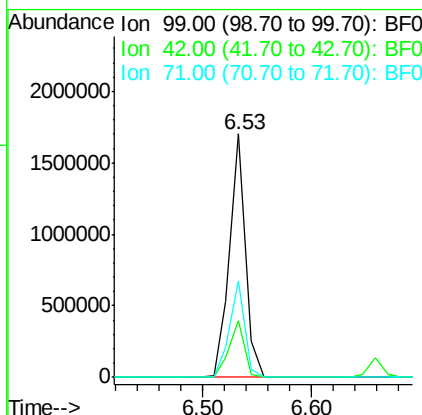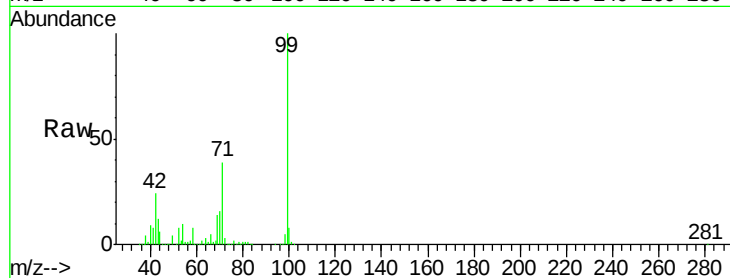

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.18 min Scan# 533




Delta R.T. -0.01 min

Lab File: BF084249.D

Acq: 4 Jan 2016 19:57

Tgt Ion: 136 Resp: 1136378

Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.7	13.1
54	8.1	5.8	8.8
68	4.6	4.2	6.2

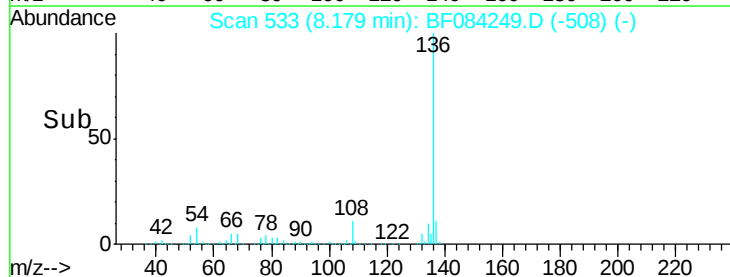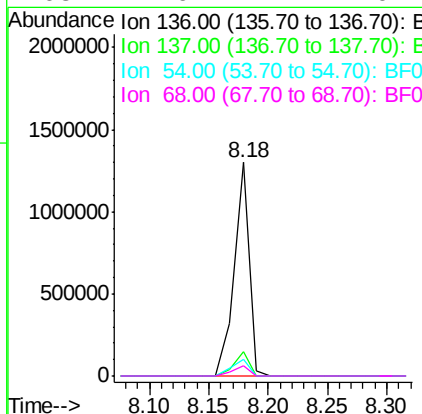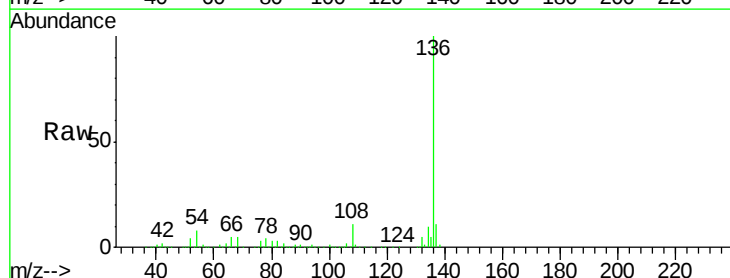







#23
 Nitrobenzene-d5
 Concen: 65.54 ng
 RT: 7.46 min Scan# 470
 Delta R.T. -0.01 min
 Lab File: BF084249.D
 Acq: 4 Jan 2016 19:57

Instrument :
 BNA_F
 ClientSampleId :
 PJ-SB-4-1.5-2.0

Tot Ion: 82 Resp: 1338131
 Ion Ratio Lower Upper
 82 100
 128 47.2 34.6 51.8
 54 55.9 38.4 57.6

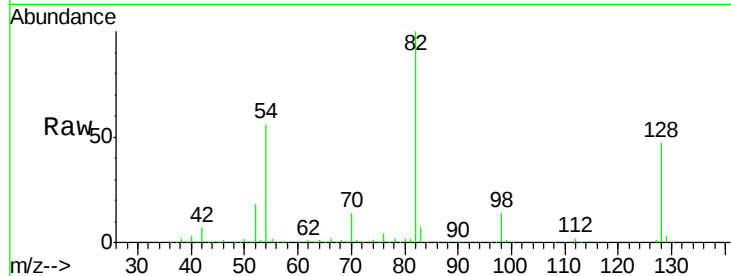


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

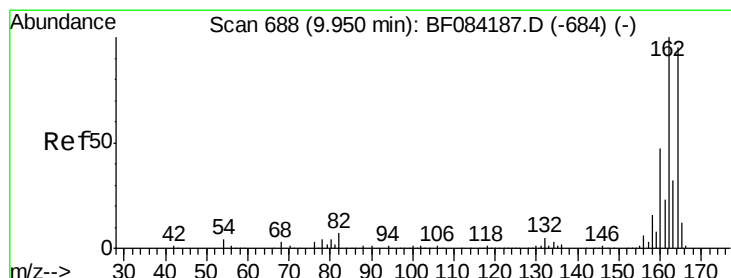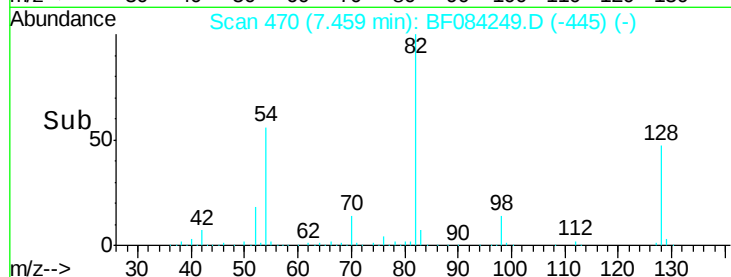
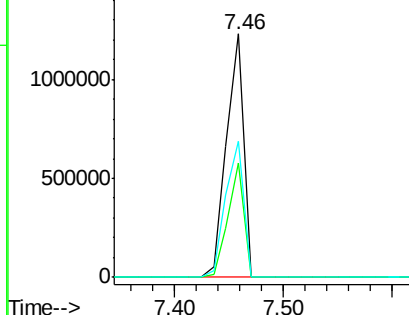



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.93 min Scan# 686
 Delta R.T. -0.02 min
 Lab File: BF084249.D
 Acq: 4 Jan 2016 19:57

Tgt Ion:164 Resp: 485746
 Ion Ratio Lower Upper
 164 100
 162 102.6 85.1 127.7
 160 46.0 37.5 56.3

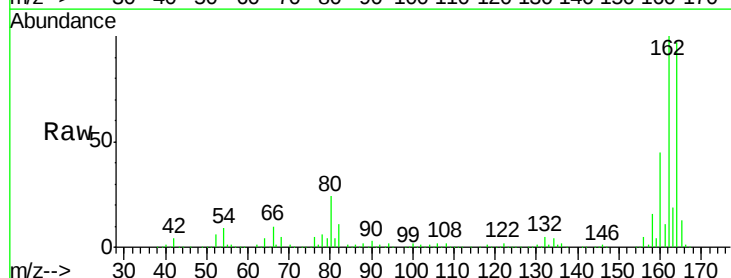

Abundance Ion 164.00 (163.70 to 164.70): B
 Ion 162.00 (161.70 to 162.70): B
 Ion 160.00 (159.70 to 160.70): B

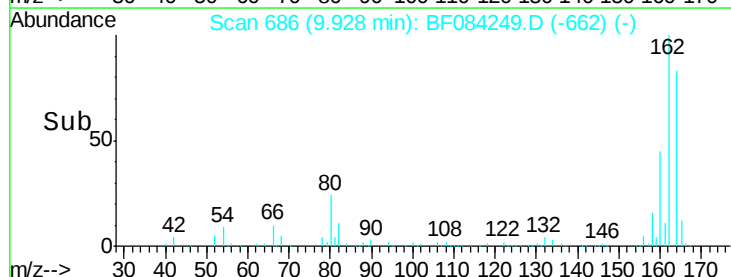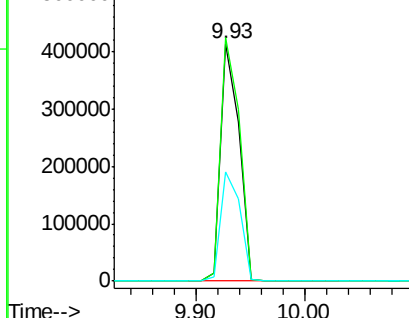

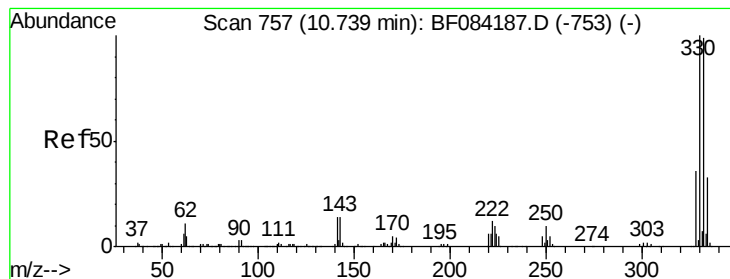

#41

2,4,6-Tribromophenol

Concen: 97.28 ng

RT: 10.73 min Scan# 756

Delta R.T. -0.01 min

Lab File: BF084249.D

Acq: 4 Jan 2016 19:57

Instrument :

BNA_F

ClientSampleId :

PJ-SB-4-1.5-2.0


Tot Ion:330 Resp: 477066

Ion Ratio Lower Upper

330 100

332 94.3 76.6 114.8




141 34.4 27.8 41.6

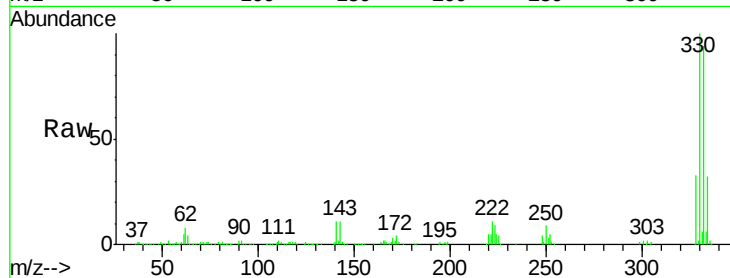

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

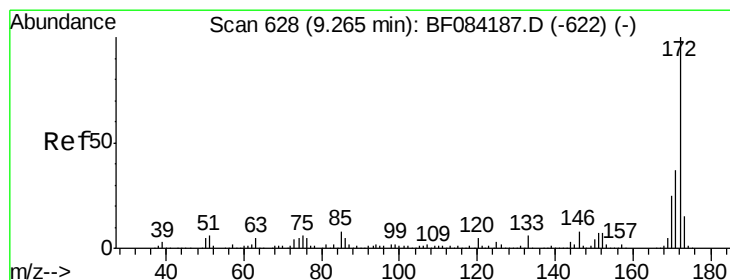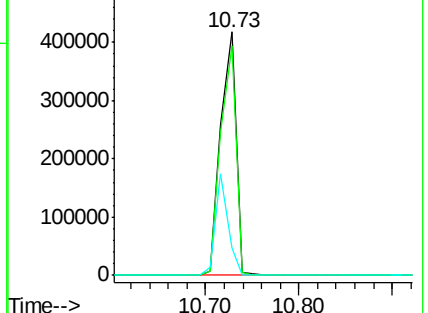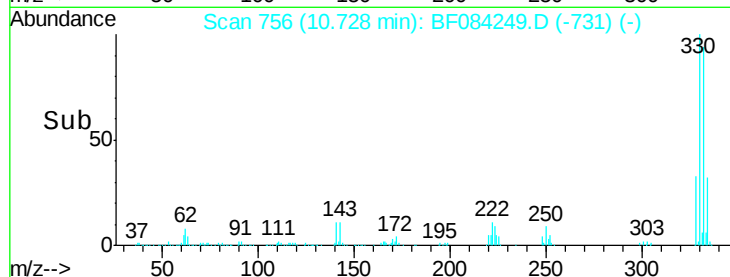

#44

2-Fluorobiphenyl

Concen: 60.65 ng

RT: 9.25 min Scan# 627

Delta R.T. -0.01 min

Lab File: BF084249.D

Acq: 4 Jan 2016 19:57


Tgt Ion:172 Resp: 1724656

Ion Ratio Lower Upper

172 100

171 36.6 28.9 43.3



170 25.2 18.6 27.8

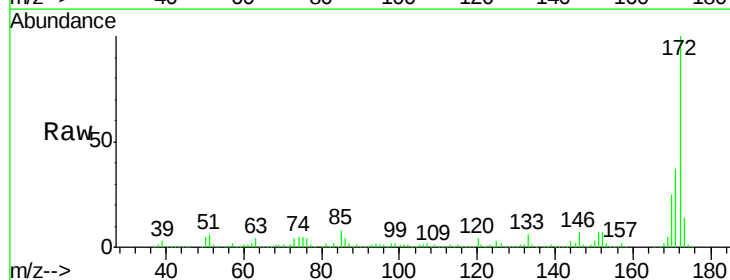


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

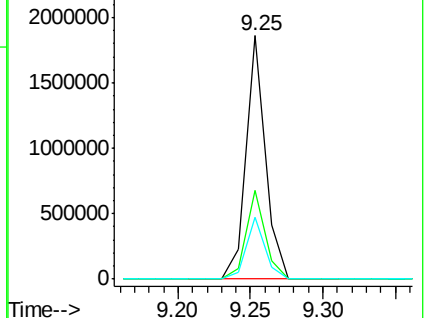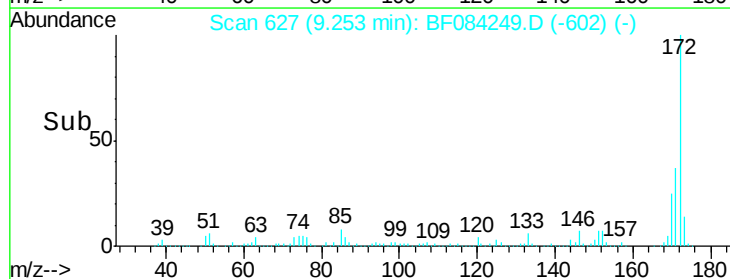

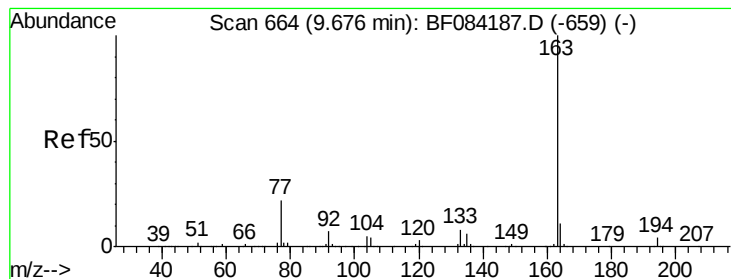

#49

Dimethylphthalate

Concen: 15.51 ng

RT: 9.65 min Scan# 662

Delta R.T. -0.02 min

Lab File: BF084249.D

Acq: 4 Jan 2016 19:57

Instrument :

BNA_F

ClientSampleId :

PJ-SB-4-1.5-2.0


Tot Ion:163 Resp: 538652

Ion Ratio Lower Upper

163 100

194 3.2 8.0 12.0#




164 10.0 8.0 12.0

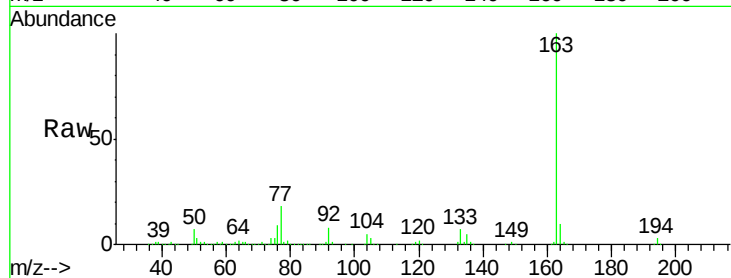

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

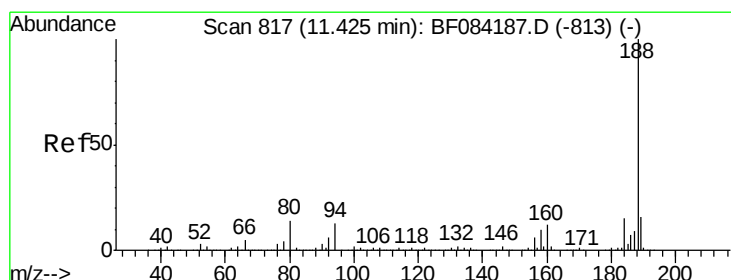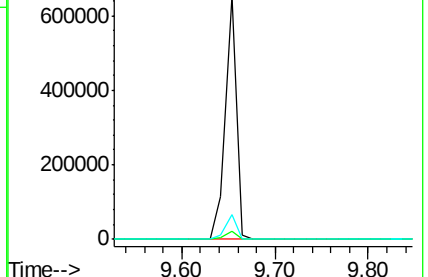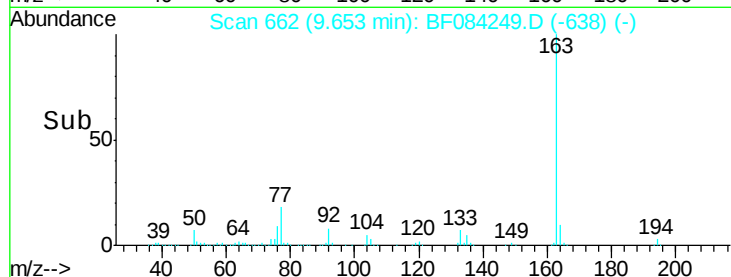

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.41 min Scan# 816

Delta R.T. -0.01 min

Lab File: BF084249.D

Acq: 4 Jan 2016 19:57


Tgt Ion:188 Resp: 818244

Ion Ratio Lower Upper

188 100

94 11.8 9.0 13.4



80 12.5 9.6 14.4

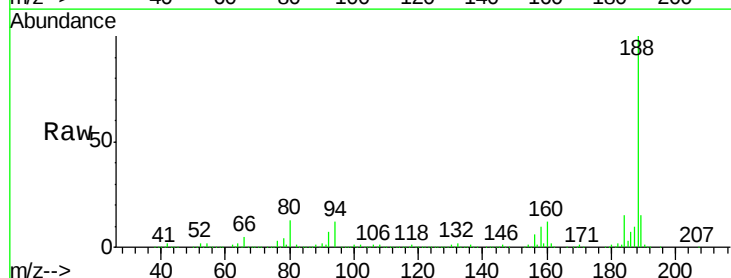


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

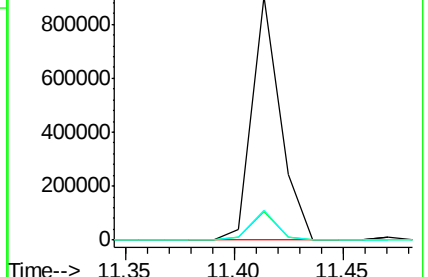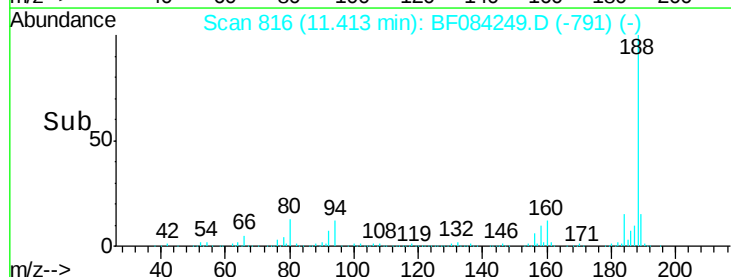

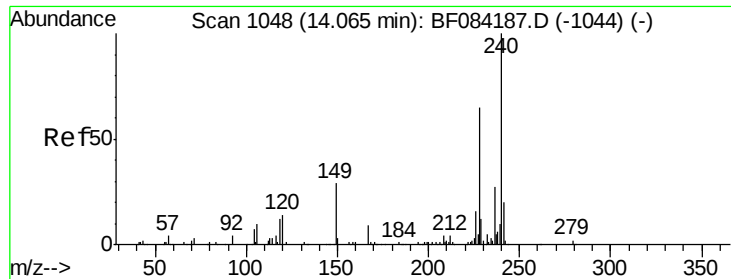

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.05 min Scan# 1047

Delta R.T. -0.01 min

Lab File: BF084249.D

Acq: 4 Jan 2016 19:57

Instrument :

BNA_F

ClientSampleId :

PJ-SB-4-1.5-2.0


Tot Ion:240 Resp: 575692

Ion Ratio Lower Upper

240 100

120 7.9 9.5 14.3#




236 26.1 20.6 31.0

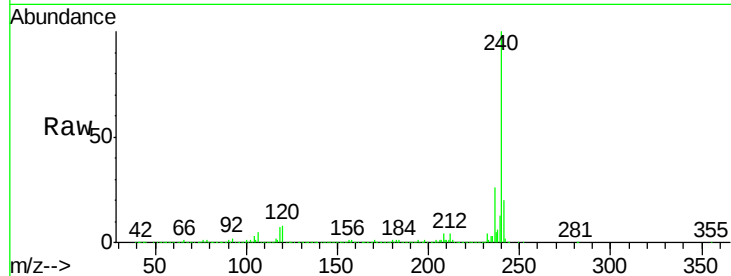

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

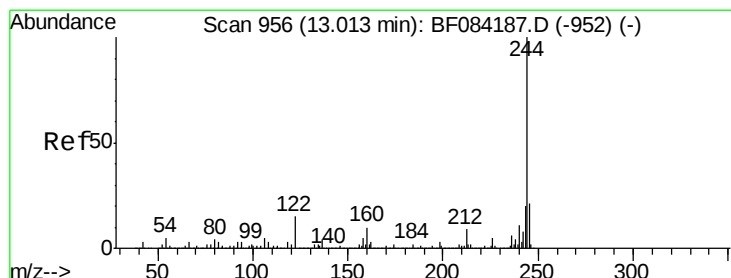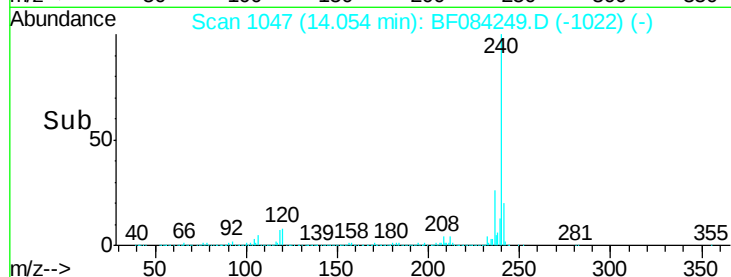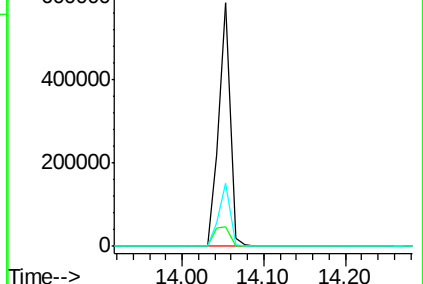

#78

Terphenyl-d14

Concen: 52.67 ng

RT: 13.00 min Scan# 955

Delta R.T. -0.01 min

Lab File: BF084249.D

Acq: 4 Jan 2016 19:57


Tgt Ion:244 Resp: 1358408

Ion Ratio Lower Upper

244 100

212 7.7 5.7 8.5



122 12.3 7.4 11.0#



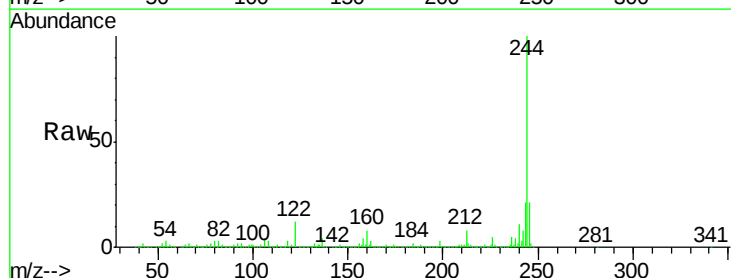


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

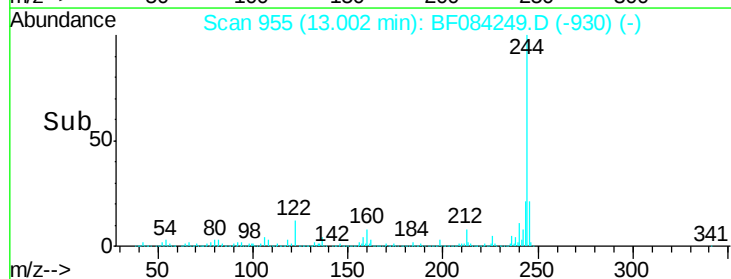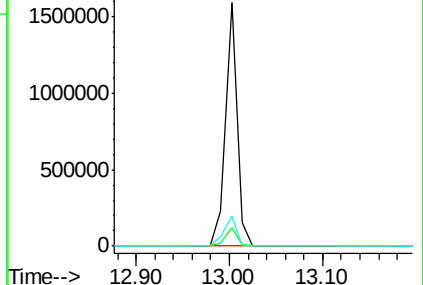

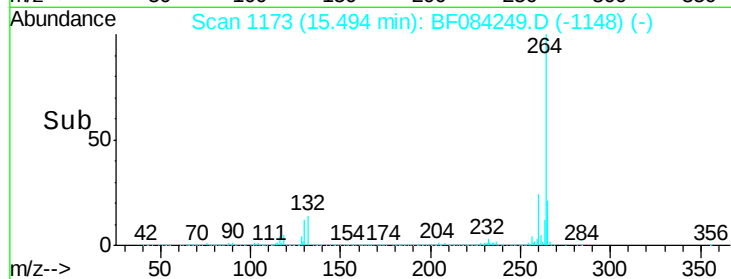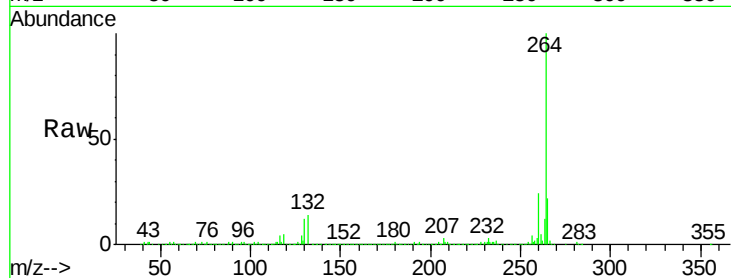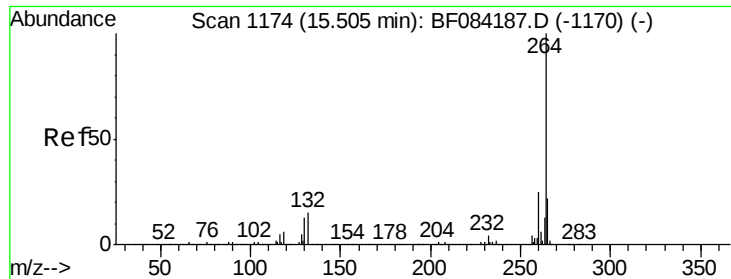

#86

Pervlene-d12

Concen: 20.00 ng

RT: 15.49 min Scan# 1173

Delta R.T. -0.01 min

Lab File: BF084249.D

Acq: 4 Jan 2016 19:57

Instrument :

BNA_F

ClientSampleId :

PJ-SB-4-1.5-2.0

Tot Ion:264 Resp: 544993

Ion Ratio Lower Upper

264 100

260 23.5 19.4 29.2

265 21.6 17.8 26.6

