


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010416\
 Data File : BF084231.D
 Acq On : 4 Jan 2016 9:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 04 12:22:40 2016

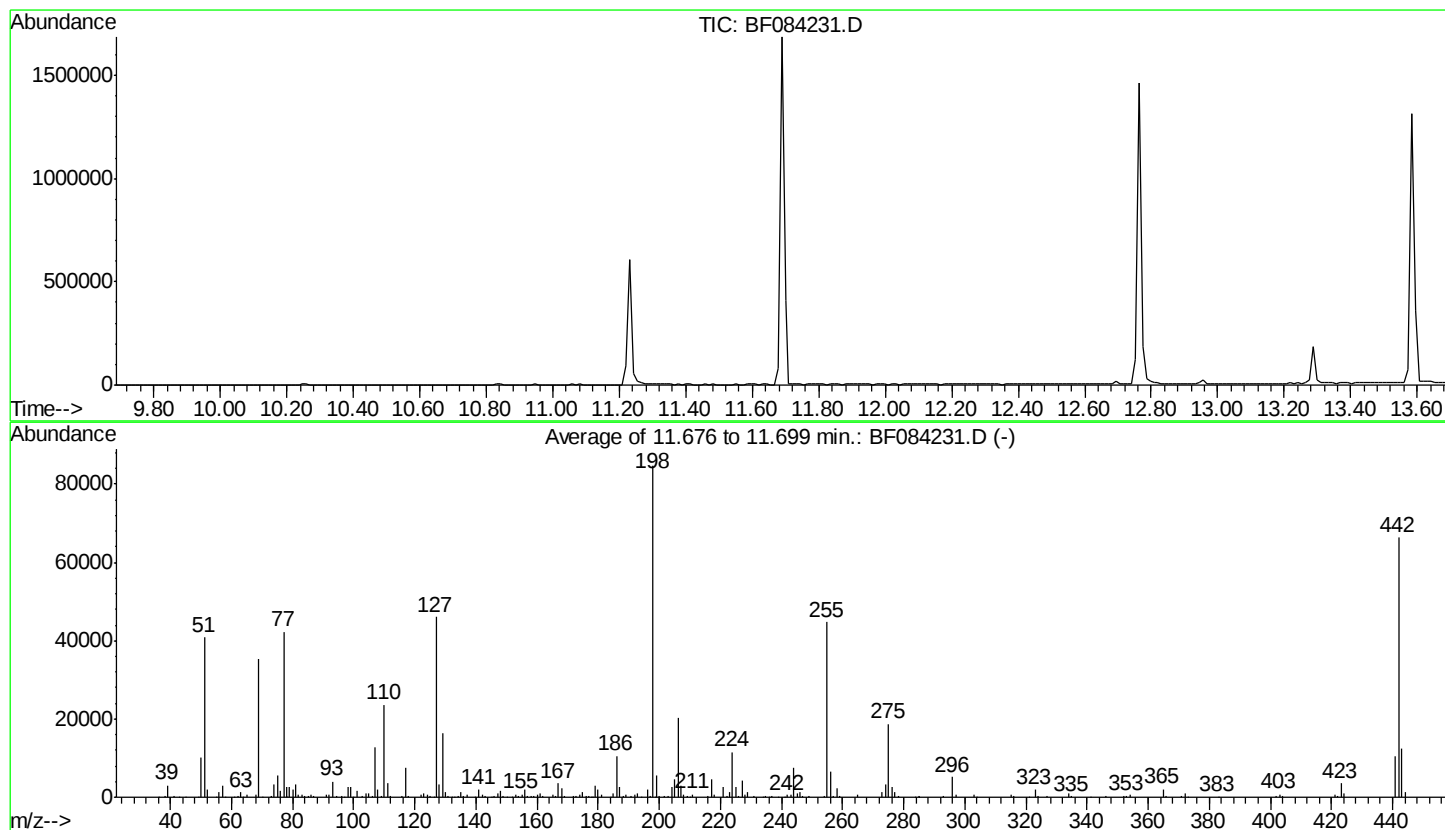

AutoFind: Scans 839, 840, 841; Background Corrected with Scan 836

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	40823	PASS
68	69	0.00	2	1.6	552	PASS
69	198	0.00	100	41.8	35452	PASS
70	69	0.00	2	0.4	130	PASS
127	198	10	80	54.3	46007	PASS
197	198	0.00	2	0.4	381	PASS
198	198	100	100	100.0	84733	PASS
199	198	5	9	6.6	5593	PASS
275	198	10	60	22.0	18658	PASS
365	198	1	100	2.5	2102	PASS
441	442	0.01	24	15.7	10439	PASS
442	198	50	100	78.3	66339	PASS
443	442	15	24	18.9	12531	PASS