


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010416\
 Data File : BF084253.D
 Acq On : 4 Jan 2016 23:29
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 04 12:22:40 2016

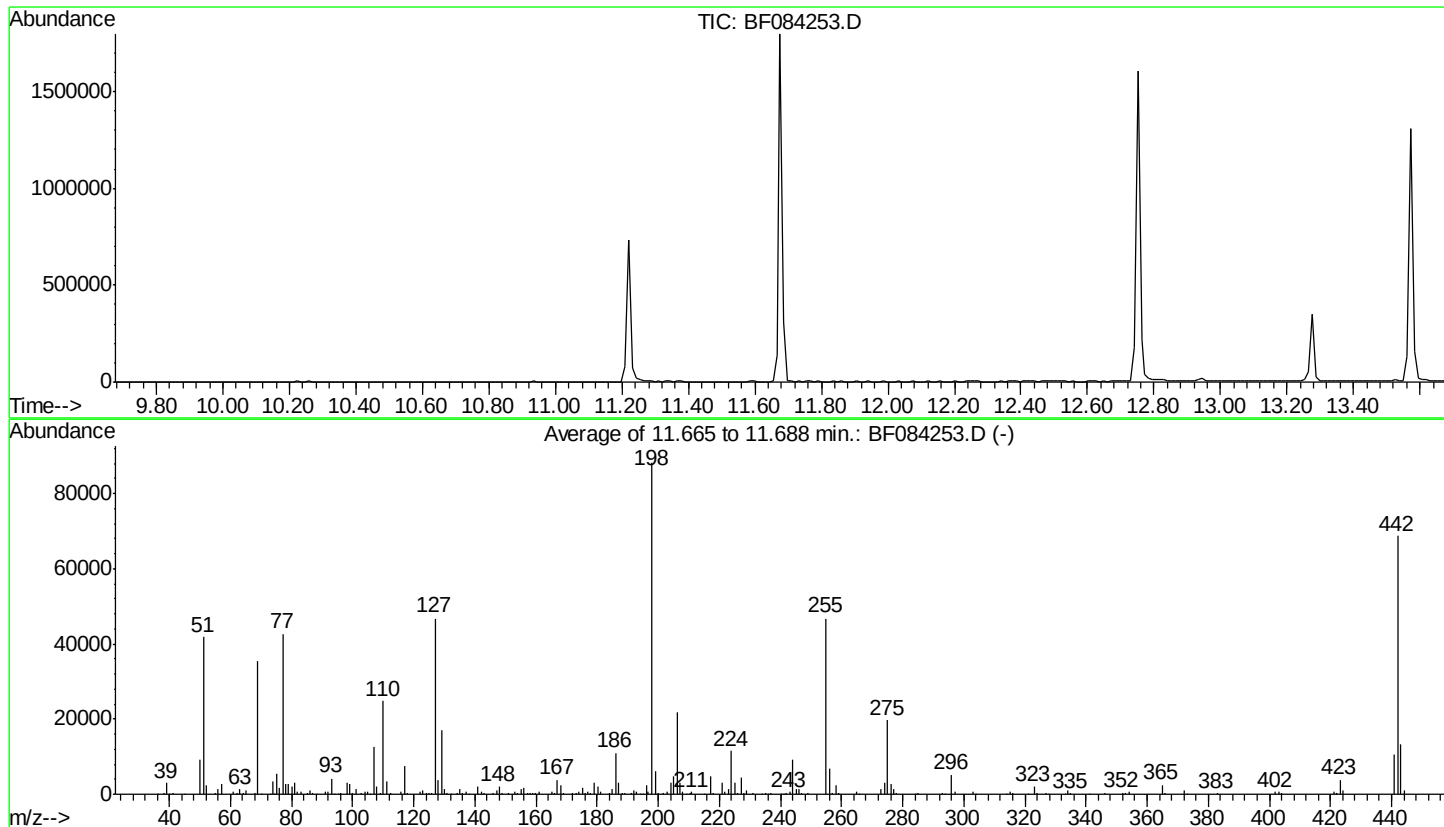

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	41854	PASS
68	69	0.00	2	1.3	447	PASS
69	198	0.00	100	40.0	35324	PASS
70	69	0.00	2	0.4	149	PASS
127	198	10	80	52.9	46668	PASS
197	198	0.00	2	0.6	569	PASS
198	198	100	100	100.0	88207	PASS
199	198	5	9	6.9	6043	PASS
275	198	10	60	22.3	19710	PASS
365	198	1	100	2.9	2523	PASS
441	442	0.01	24	15.5	10669	PASS
442	198	50	100	77.9	68678	PASS
443	442	15	24	19.1	13120	PASS