


Data Path : Z:\HPCHEM1\BNA F\DATA\BF010417\
 Data File : BF092072.D
 Acq On : 4 Jan 2017 16:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 28 17:32:10 2016

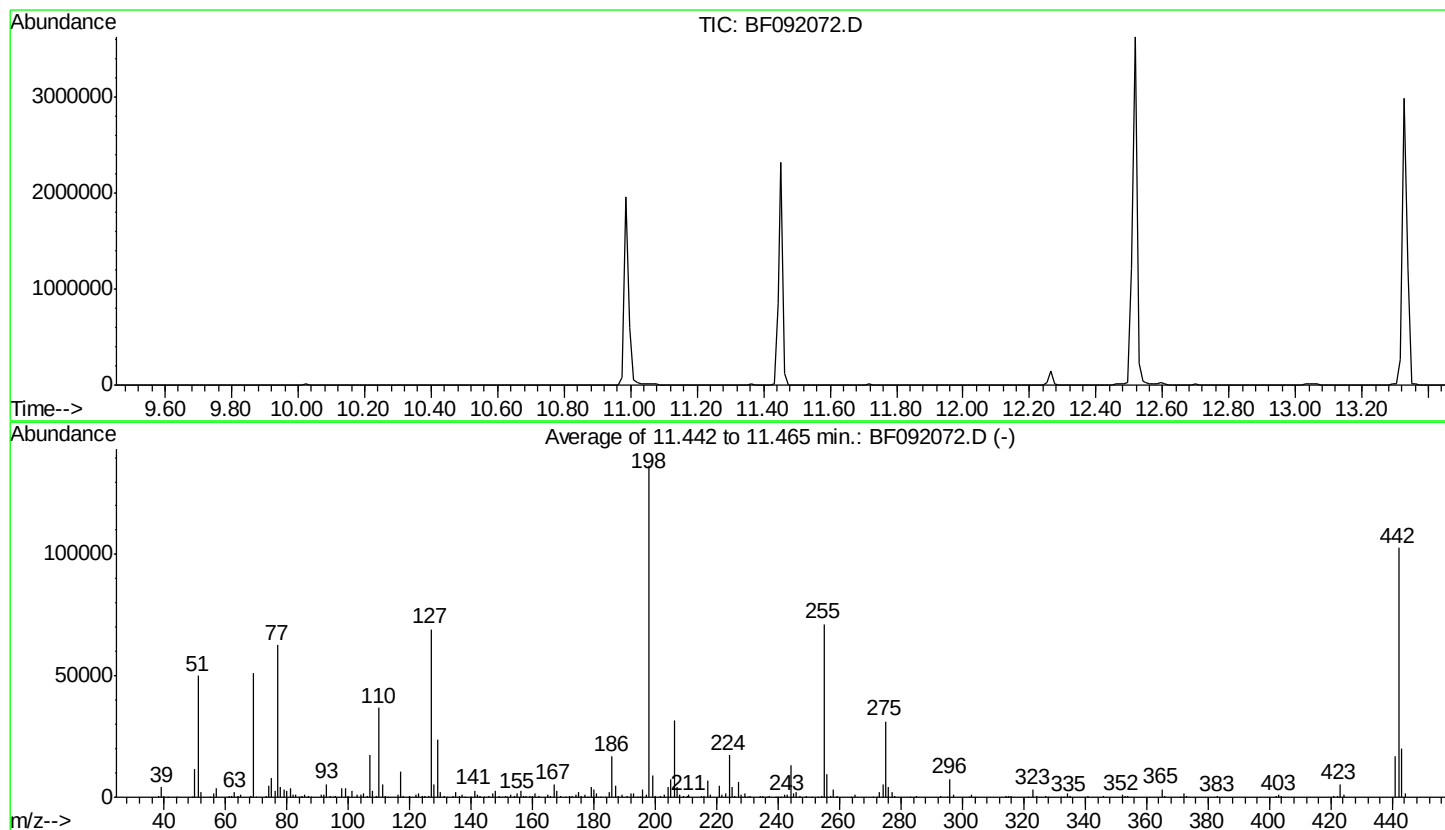

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	49925	PASS
68	69	0.00	2	1.4	706	PASS
69	198	0.00	100	37.6	51327	PASS
70	69	0.00	2	0.4	224	PASS
127	198	10	80	50.7	69218	PASS
197	198	0.00	2	0.6	887	PASS
198	198	100	100	100.0	136620	PASS
199	198	5	9	6.6	9068	PASS
275	198	10	60	23.0	31395	PASS
365	198	1	100	2.4	3338	PASS
441	442	0.01	24	16.4	16836	PASS
442	198	50	100	75.3	102810	PASS
443	442	15	24	19.7	20247	PASS