

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010424\
 Data File : BF136955.D
 Acq On : 04 Jan 2024 22:52
 Operator : CG\JU
 Sample : 05899-22DL 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GHL-SS-18-2-4DL

Quant Time: Jan 05 00:45:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.781	152	41978	20.000	ng	-0.01
21) Naphthalene-d8	8.057	136	160960	20.000	ng	-0.01
39) Acenaphthene-d10	9.816	164	81999	20.000	ng	-0.01
64) Phenanthrene-d10	11.310	188	152088	20.000	ng	0.00
76) Chrysene-d12	13.969	240	105935	20.000	ng	# 0.00
86) Perylene-d12	15.451	264	119762	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.422	112	23965	8.908	ng	0.00
7) Phenol-d6	6.434	99	30346	8.705	ng	0.00
23) Nitrobenzene-d5	7.340	82	17491	5.561	ng	-0.02
42) 2,4,6-Tribromophenol	10.610	330	8078	8.365	ng	-0.01
45) 2-Fluorobiphenyl	9.134	172	42334	6.944	ng	-0.02
79) Terphenyl-d14	12.898	244	46465	6.130	ng	-0.02
Target Compounds						Qvalue
25) Isophorone	7.340	82	17494	3.056	ng	# 65
31) Naphthalene	8.081	128	310493	35.113	ng	100
33) 4-Chloroaniline	8.081	127	40491	12.402	ng	# 34
35) Caprolactam	8.769	113	3199	4.104	ng	# 1
37) 2-Methylnaphthalene	8.769	142	162392	28.535	ng	98
46) 1,1'-Biphenyl	9.234	154	34447	5.006	ng	98
51) 2,6-Dinitrotoluene	9.816	165	11440	8.416	ng	# 30
52) Acenaphthene	9.845	154	58141	11.731	ng	97
53) 3-Nitroaniline	10.022	138	3840	2.667	ng	# 7
55) Dibenzofuran	10.022	168	264294	35.178	ng	97
56) 4-Nitrophenol	10.022	139	90376	92.976	ng	# 9
58) Fluorene	10.369	166	560193	93.971	ng	99
62) 4-Nitroaniline	10.369	138	5843	4.209	ng	# 21
71) Phenanthrene	11.345	178	1266161	162.250	ng	99
72) Anthracene	11.427	178	5371686	679.694	ng	98
73) Carbazole	11.575	167	2487855	333.887	ng	99
75) Fluoranthene	12.533	202	566986	67.924	ng	98
78) Pyrene	12.763	202	383650	36.892	ng	99
81) Benzo(a)anthracene	13.957	228	135533	18.425	ng	98
83) Chrysene	13.992	228	237922	33.075	ng	98
84) Bis(2-ethylhexyl)phtha...	13.945	149	29547	6.206	ng	# 98
87) Indeno(1,2,3-cd)pyrene	16.962	276	22607	2.614	ng	98
88) Benzo(b)fluoranthene	15.015	252	119986	15.000	ng	99
89) Benzo(k)fluoranthene	15.015	252	119986	15.875	ng	98
90) Benzo(a)pyrene	15.386	252	47382	7.017	ng	99
92) Benzo(g,h,i)perylene	17.427	276	18520	2.549	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010424\
Data File : BF136955.D
Acq On : 04 Jan 2024 22:52
Operator : CG\JU
Sample : 05899-22DL 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GHL-SS-18-2-4DL

Quant Time: Jan 05 00:45:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration



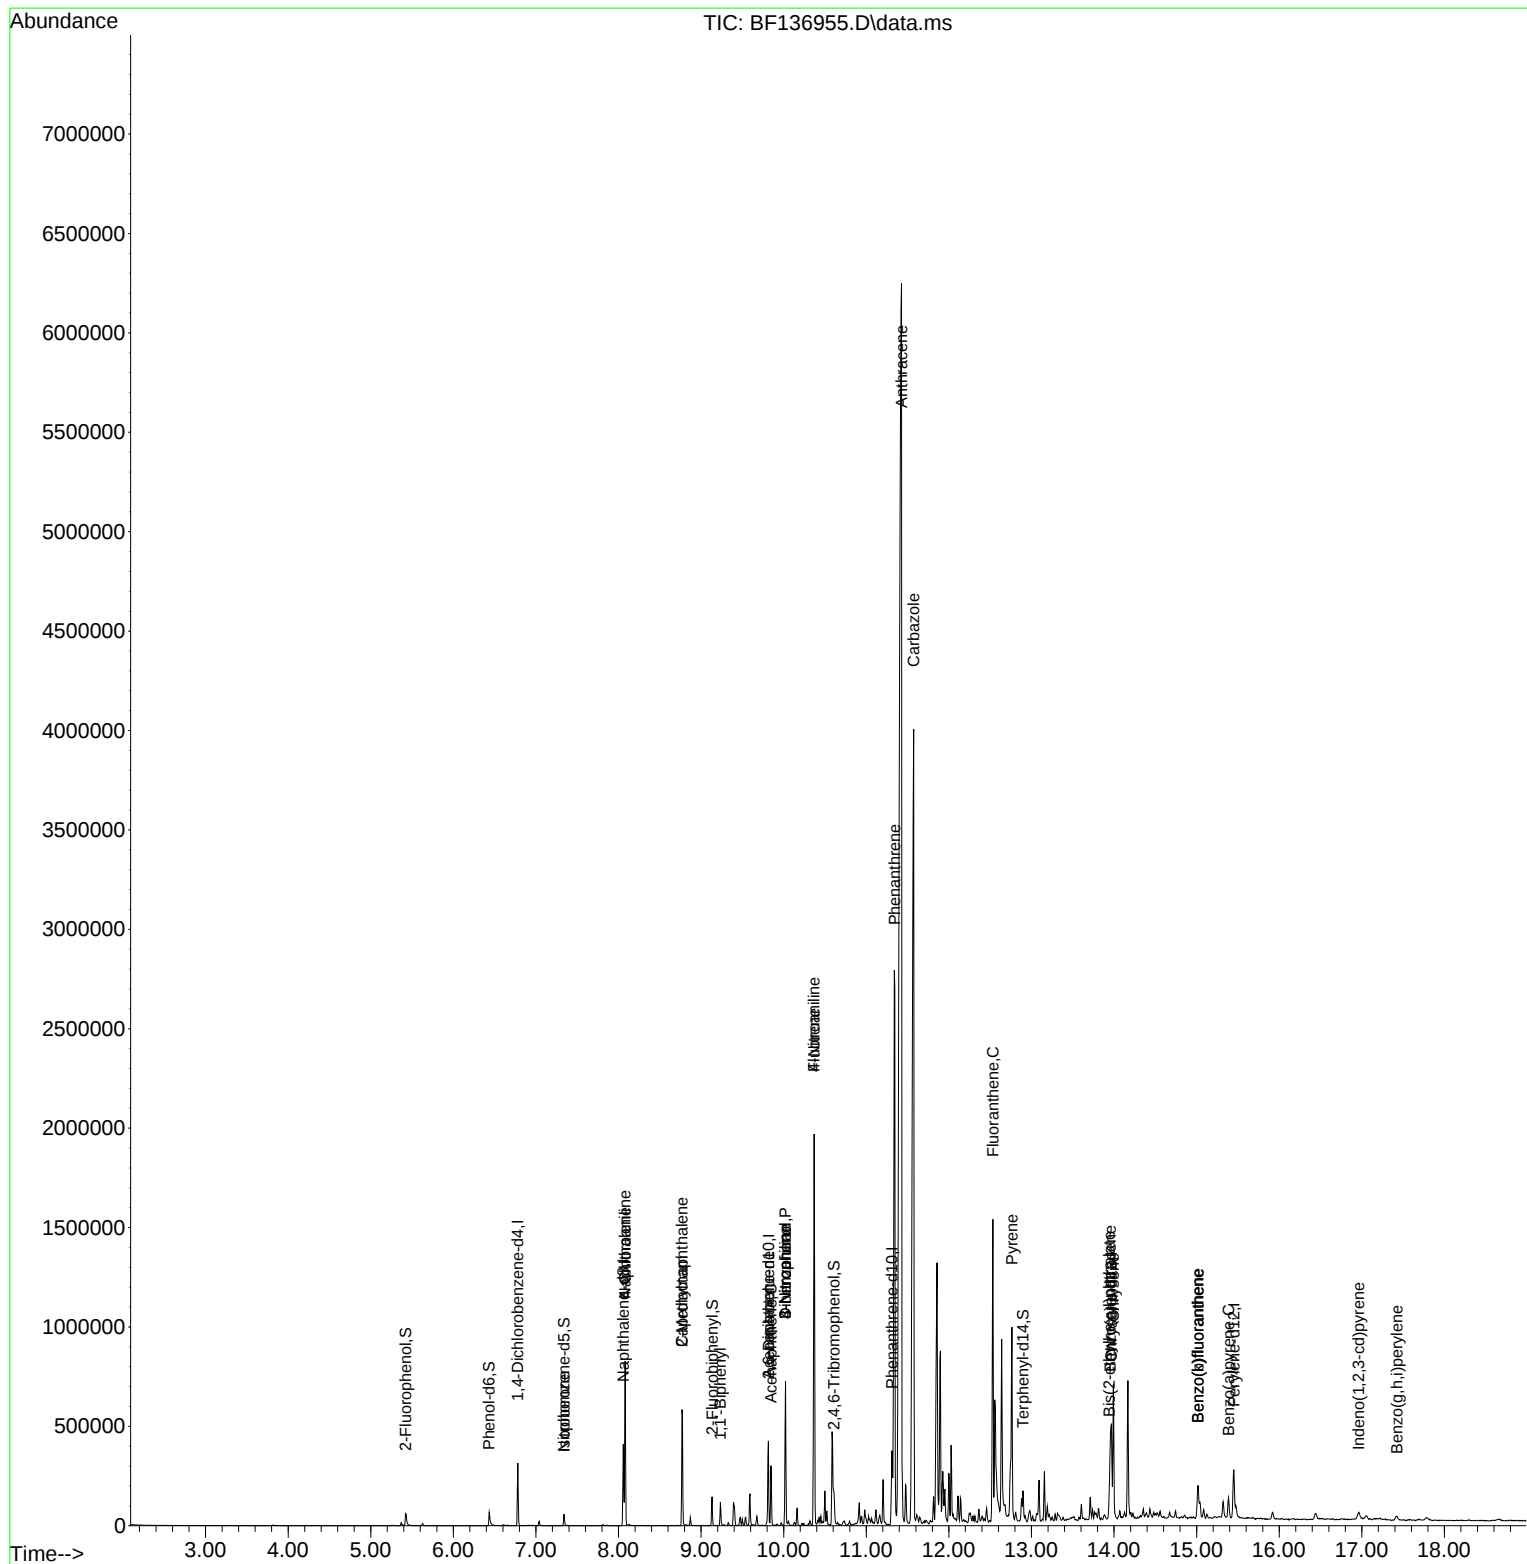




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.781 min Scan# 79
Delta R.T. -0.011 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52




Instrument :
BNA_F
ClientSampleId :
GHL-SS-18-2-4DL


Tgt Ion:152 Resp: 41978
Ion Ratio Lower Upper
152 100
150 160.9 127.0 190.6
115 61.4 49.0 73.4

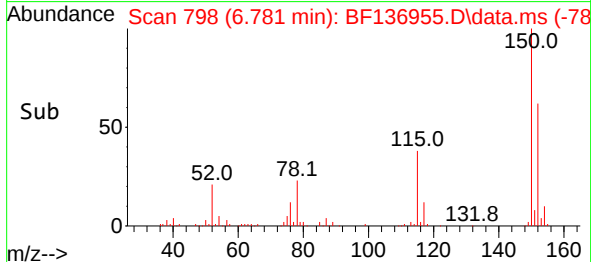

#5
2-Fluorophenol
Concen: 8.908 ng
RT: 5.422 min Scan# 567
Delta R.T. -0.006 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52

Tgt Ion:112 Resp: 23965
Ion Ratio Lower Upper
112 100
64 61.8 51.1 76.7
63 33.5 26.1 39.1









#7
Phenol-d6
Concen: 8.705 ng
RT: 6.434 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52




Instrument :
BNA_F
ClientSampleId :
GHL-SS-18-2-4DL

Tgt Ion: 99 Resp: 30346
Ion Ratio Lower Upper
99 100
42 18.9 16.1 24.1
71 32.9 27.4 41.2

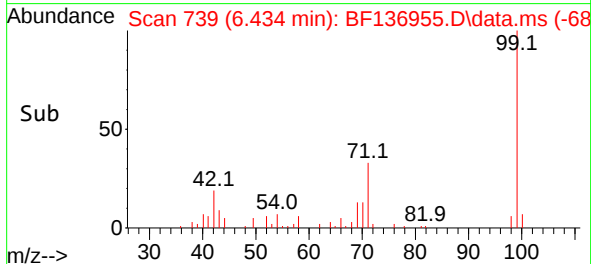

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.057 min Scan# 1015
Delta R.T. -0.012 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52

Tgt Ion:136 Resp: 160960
Ion Ratio Lower Upper
136 100
137 10.7 9.0 13.4
54 9.2 7.2 10.8
68 5.4 4.9 7.3





#23

Nitrobenzene-d5

Concen: 5.561 ng

RT: 7.340 min Scan# 893

Delta R.T. -0.017 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52

Instrument :

BNA_F

ClientSampleId :

GHL-SS-18-2-4DL





Tgt Ion: 82 Resp: 17491

Ion Ratio Lower Upper

82 100

128 40.5 35.3 52.9

54 58.3 44.5 66.7

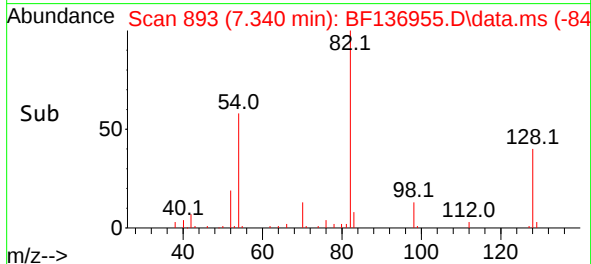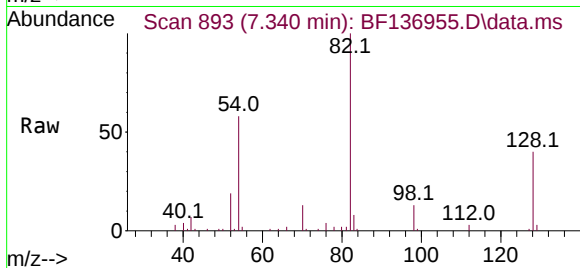

#25

Isophorone

Concen: 3.056 ng

RT: 7.340 min Scan# 893

Delta R.T. -0.276 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52




Tgt Ion: 82 Resp: 17494


Ion Ratio Lower Upper

82 100

95 0.0 5.5 8.3#

138 0.0 14.5 21.7#


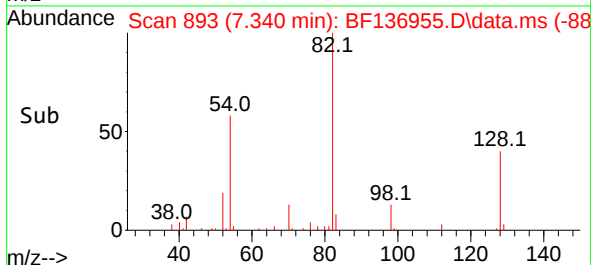
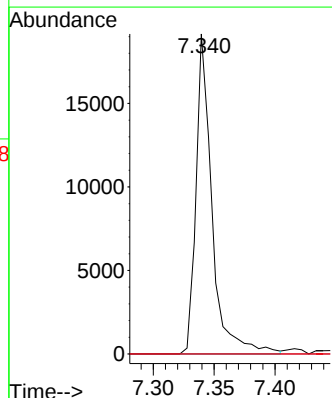
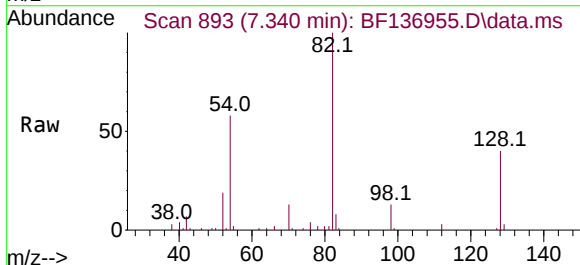




#31
Naphthalene
Concen: 35.113 ng
RT: 8.081 min Scan# 1019
Delta R.T. -0.012 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52




Instrument :
BNA_F
ClientSampleId :
GHL-SS-18-2-4DL


Tgt Ion:128 Resp: 310493
Ion Ratio Lower Upper
128 100
129 11.1 8.7 13.1
127 13.3 10.8 16.2

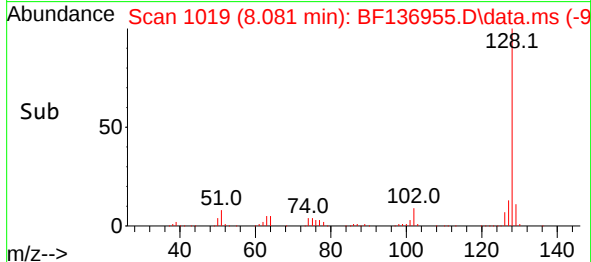

#33
4-Chloroaniline
Concen: 12.402 ng
RT: 8.081 min Scan# 1019
Delta R.T. -0.065 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52

Tgt Ion:127 Resp: 40491
Ion Ratio Lower Upper
127 100
129 83.1 26.3 39.5#
65 0.0 25.8 38.8#
92 0.0 15.8 23.6#


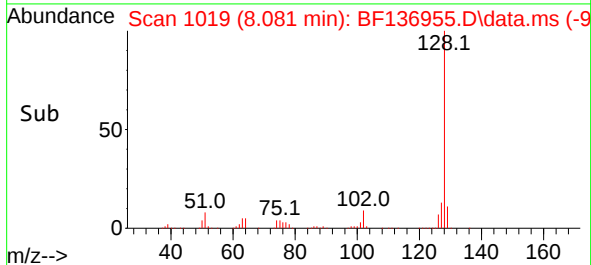
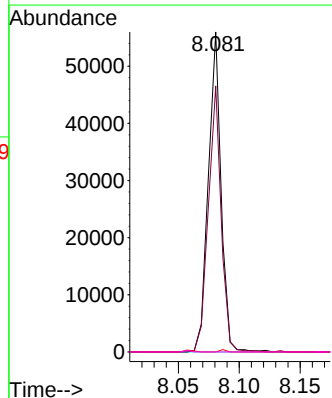





#35
Caprolactam
Concen: 4.104 ng
RT: 8.769 min Scan# 1136
Delta R.T. 0.247 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52




Instrument :
BNA_F
ClientSampleId :
GHL-SS-18-2-4DL


Tgt Ion:113 Resp: 3199
Ion Ratio Lower Upper
113 100
55 16.8 163.1 203.1#
56 8.9 121.7 161.7#

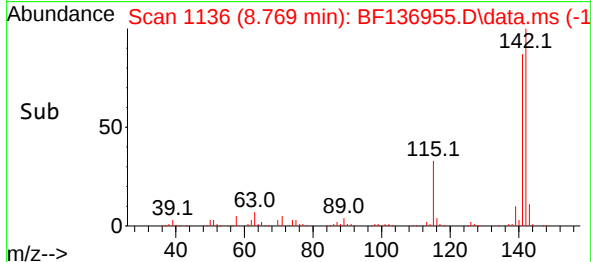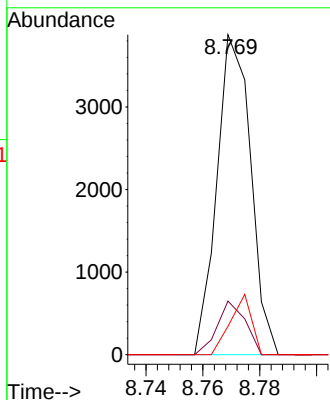

#37
2-Methylnaphthalene
Concen: 28.535 ng
RT: 8.769 min Scan# 1136
Delta R.T. -0.017 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52

Tgt Ion:142 Resp: 162392
Ion Ratio Lower Upper
142 100
141 86.7 71.1 106.7



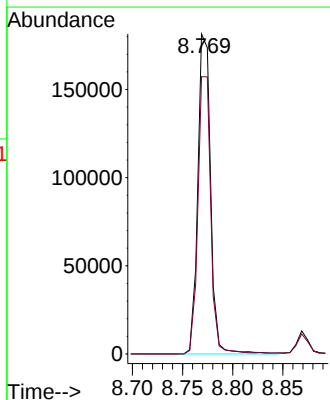
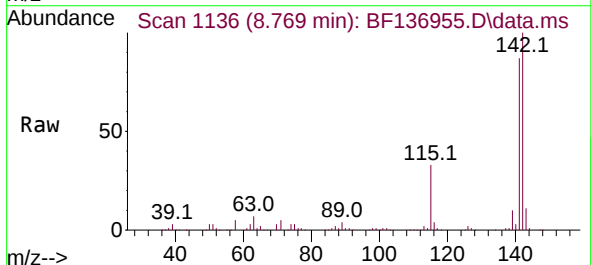




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.816 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52




Instrument :
BNA_F
ClientSampleId :
GHL-SS-18-2-4DL


Tgt Ion:164 Resp: 81999
Ion Ratio Lower Upper
164 100
162 102.5 81.6 122.4
160 44.7 34.9 52.3

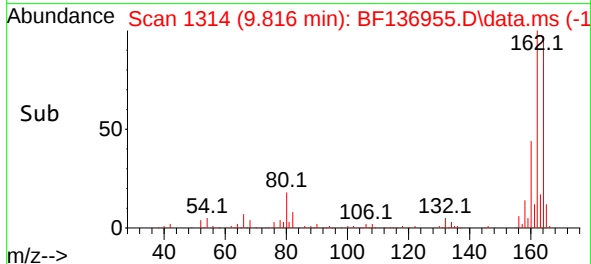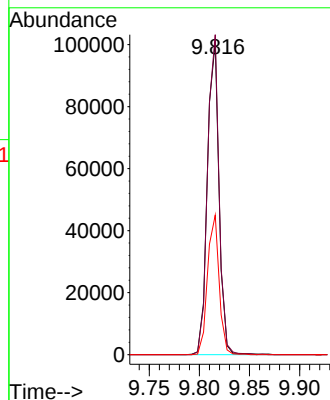

#42
2,4,6-Tribromophenol
Concen: 8.365 ng
RT: 10.610 min Scan# 1449
Delta R.T. -0.012 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52

Tgt Ion:330 Resp: 8078
Ion Ratio Lower Upper
330 100
332 101.9 77.4 116.0
141 35.3 23.4 35.2#

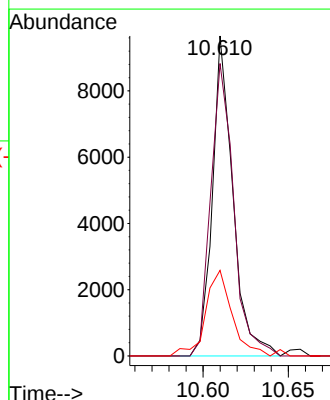

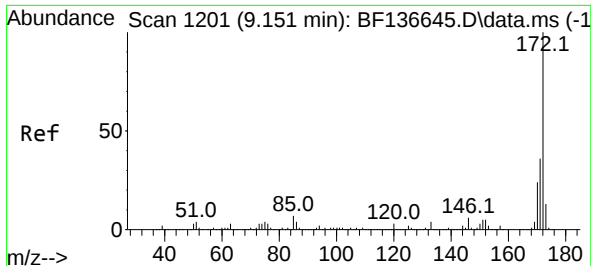

#45

2-Fluorobiphenyl

Concen: 6.944 ng

RT: 9.134 min Scan# 1198

Delta R.T. -0.017 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52

Instrument :

BNA_F

ClientSampleId :

GHL-SS-18-2-4DL





Tgt Ion:172 Resp: 42334

Ion Ratio Lower Upper

172 100

171 34.1 29.0 43.6

170 22.1 19.0 28.4

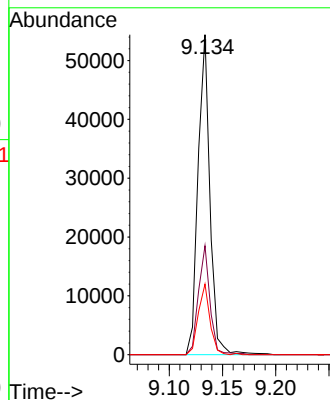

#46

1,1'-Biphenyl

Concen: 5.006 ng

RT: 9.234 min Scan# 1215

Delta R.T. -0.017 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52




Tgt Ion:154 Resp: 34447


Ion Ratio Lower Upper

154 100

153 42.1 21.1 61.1

76 11.1 0.0 31.7

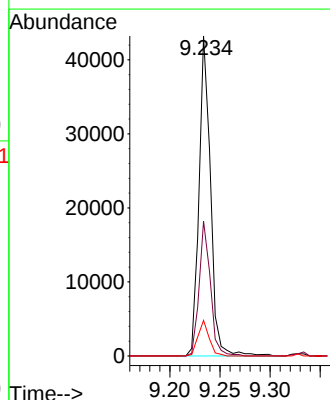



#51

2,6-Dinitrotoluene

Concen: 8.416 ng

RT: 9.816 min Scan# 1

Delta R.T. 0.194 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52

Instrument :

BNA_F

ClientSampleId :

GHL-SS-18-2-4DL





Tgt Ion:165 Resp: 11440

Ion Ratio Lower Upper

165 100

63 1.6 39.8 59.6#

89 1.2 38.8 58.2#

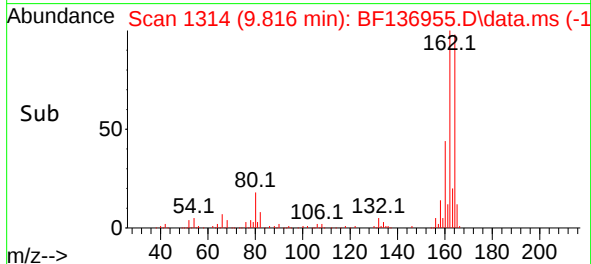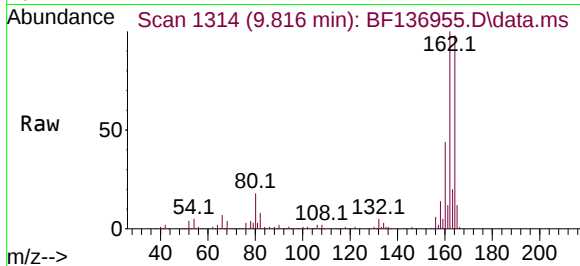

#52

Acenaphthene

Concen: 11.731 ng

RT: 9.845 min Scan# 1319

Delta R.T. -0.017 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52




Tgt Ion:154 Resp: 58141


Ion Ratio Lower Upper

154 100

153 110.5 90.7 136.1

152 51.4 43.7 65.5




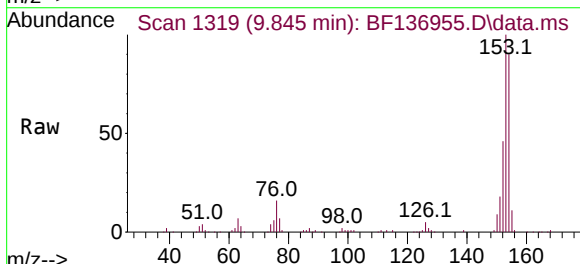




#53
3-Nitroaniline
Concen: 2.667 ng
RT: 10.022 min Scan# 1349
Delta R.T. 0.235 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52




Instrument :
BNA_F
ClientSampleId :
GHL-SS-18-2-4DL


Tgt Ion:138 Resp: 3840
Ion Ratio Lower Upper
138 100
108 0.0 8.6 12.8#
92 10.1 95.2 142.8#

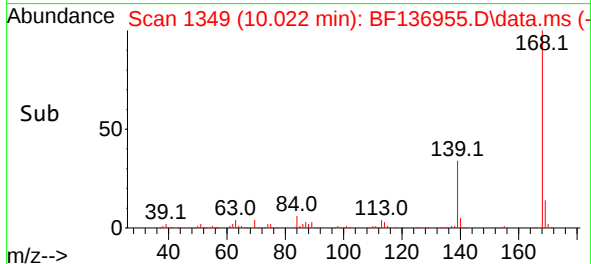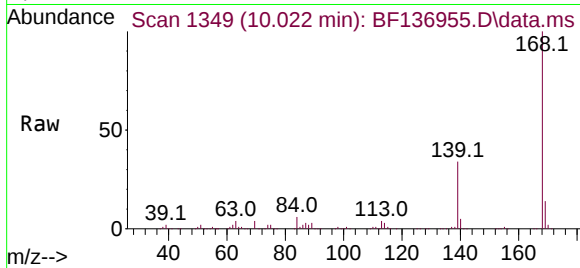

#55
Dibenzofuran
Concen: 35.178 ng
RT: 10.022 min Scan# 1349
Delta R.T. -0.012 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52

Tgt Ion:168 Resp: 264294
Ion Ratio Lower Upper
168 100
139 34.0 29.3 43.9
169 13.6 11.0 16.4




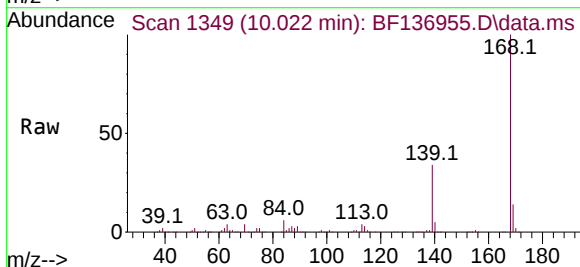




#56
4-Nitrophenol
Concen: 92.976 ng
RT: 10.022 min Scan# 11
Delta R.T. 0.065 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52




Instrument :
BNA_F
ClientSampleId :
GHL-SS-18-2-4DL


Tgt Ion:139 Resp: 90376
Ion Ratio Lower Upper
139 100
109 0.8 45.8 85.8#
65 1.7 77.8 117.8#

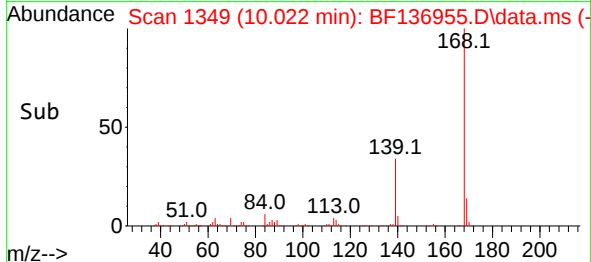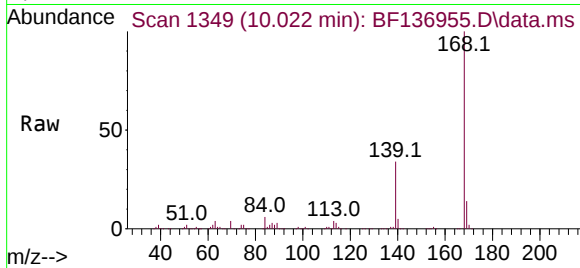

#58
Fluorene
Concen: 93.971 ng
RT: 10.369 min Scan# 1408
Delta R.T. -0.012 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52

Tgt Ion:166 Resp: 560193
Ion Ratio Lower Upper
166 100
165 92.6 73.7 110.5
167 13.5 10.4 15.6




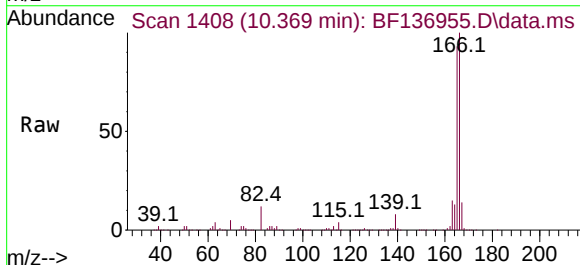




#62
4-Nitroaniline
Concen: 4.209 ng
RT: 10.369 min Scan# 1414
Delta R.T. -0.035 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52




Instrument :
BNA_F
ClientSampleId :
GHL-SS-18-2-4DL


Tgt Ion:138 Resp: 5843
Ion Ratio Lower Upper
138 100
92 0.0 32.1 72.1#
108 2.6 50.1 90.1#

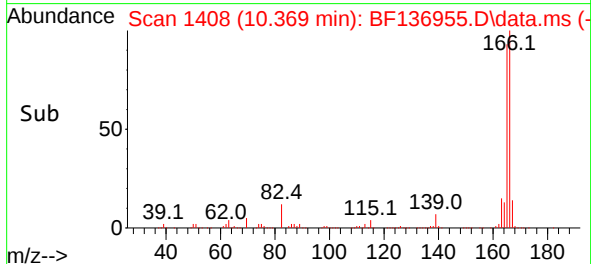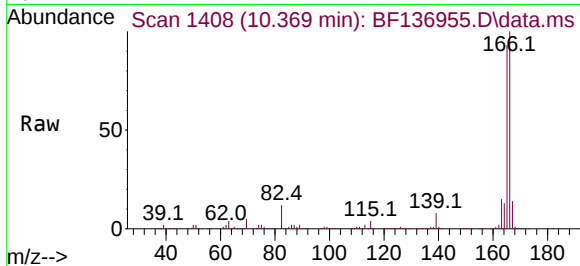

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.310 min Scan# 1568
Delta R.T. -0.006 min
Lab File: BF136955.D
Acq: 04 Jan 2024 22:52

Tgt Ion:188 Resp: 152088
Ion Ratio Lower Upper
188 100
94 8.1 7.5 11.3
80 9.2 8.1 12.1

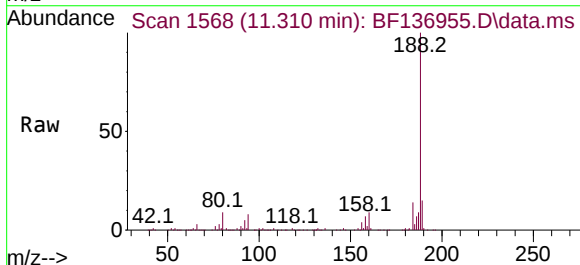



#71

Phenanthrene

Concen: 162.250 ng

RT: 11.345 min Scan# 1

Delta R.T. 0.000 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52

Instrument :

BNA_F

ClientSampleId :

GHL-SS-18-2-4DL





Tgt Ion:178 Resp: 1266161

Ion Ratio Lower Upper

178 100

176 18.8 15.3 22.9

179 14.6 11.9 17.9

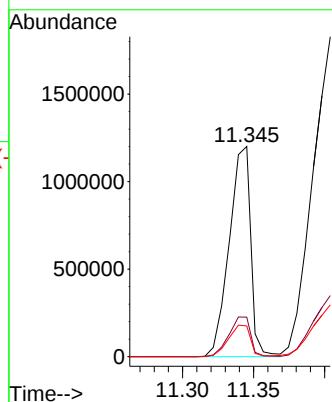

#72

Anthracene

Concen: 679.694 ng

RT: 11.427 min Scan# 1588

Delta R.T. 0.030 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52




Tgt Ion:178 Resp: 5371686


Ion Ratio Lower Upper

178 100

176 19.4 14.9 22.3

179 15.9 11.8 17.6


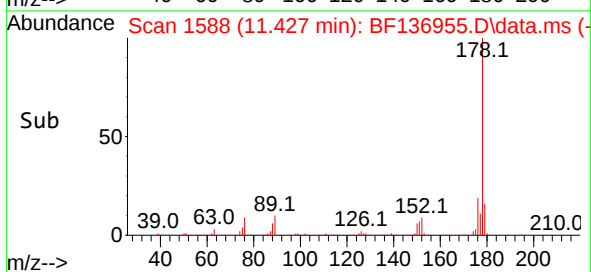
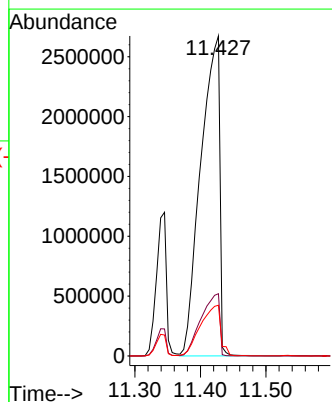





#73
 Carbazole
 Concen: 333.887 ng
 RT: 11.575 min Scan# 1610
 Delta R.T. 0.018 min
 Lab File: BF136955.D
 Acq: 04 Jan 2024 22:52




Instrument :
 BNA_F
 ClientSampleId :
 GHL-SS-18-2-4DL


Tgt Ion:167 Resp: 2487855
 Ion Ratio Lower Upper
 167 100
 166 22.4 17.3 25.9
 139 12.6 9.8 14.6

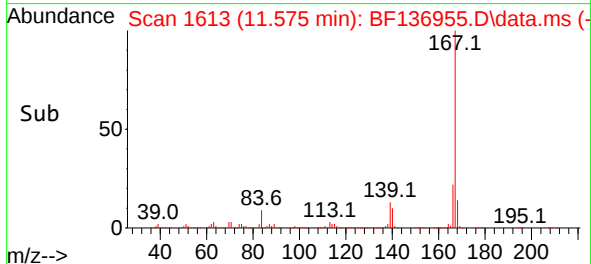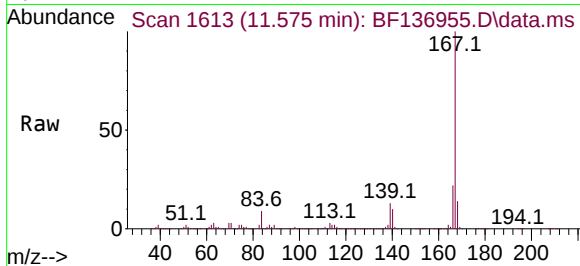

#75
 Fluoranthene
 Concen: 67.924 ng
 RT: 12.533 min Scan# 1776
 Delta R.T. -0.006 min
 Lab File: BF136955.D
 Acq: 04 Jan 2024 22:52

Tgt Ion:202 Resp: 566986
 Ion Ratio Lower Upper
 202 100
 101 11.1 0.0 29.3
 203 17.4 0.0 37.1

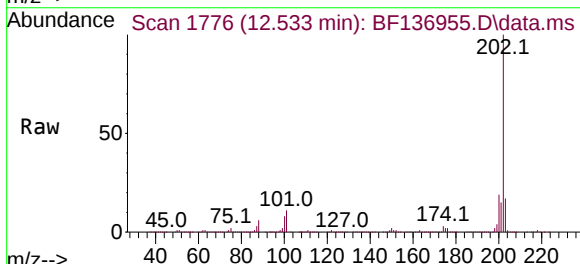



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.969 min Scan# 20

Delta R.T. 0.000 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52

Instrument :

BNA_F

ClientSampleId :

GHL-SS-18-2-4DL





Tgt Ion:240 Resp: 105935

Ion Ratio Lower Upper

240 100

120 9.9 10.3 15.5#

236 25.0 19.4 29.2

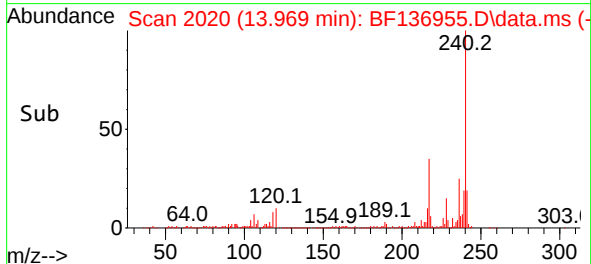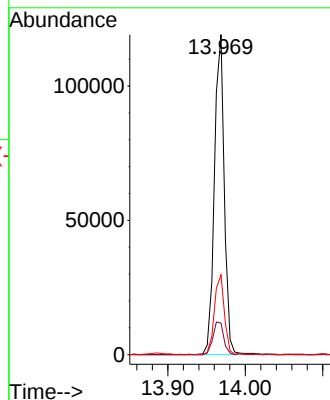

#78

Pyrene

Concen: 36.892 ng

RT: 12.763 min Scan# 1815

Delta R.T. -0.006 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52




Tgt Ion:202 Resp: 383650


Ion Ratio Lower Upper

202 100

200 19.6 15.9 23.9

203 17.4 13.8 20.6

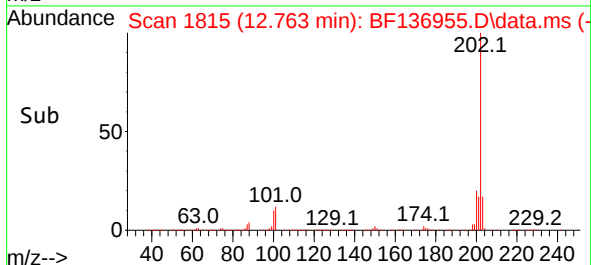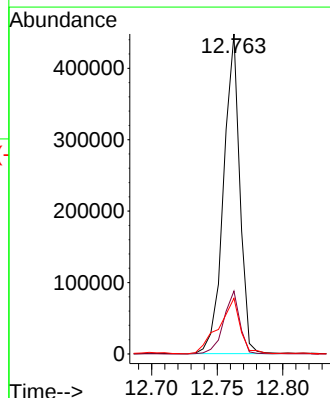



#79

Terphenyl-d14

Concen: 6.130 ng

RT: 12.898 min Scan# 11

Delta R.T. -0.017 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52

Instrument :

BNA_F

ClientSampleId :

GHL-SS-18-2-4DL





Tgt Ion:244 Resp: 46465

Ion Ratio Lower Upper

244 100

212 5.7 5.0 7.4

122 10.1 9.0 13.4

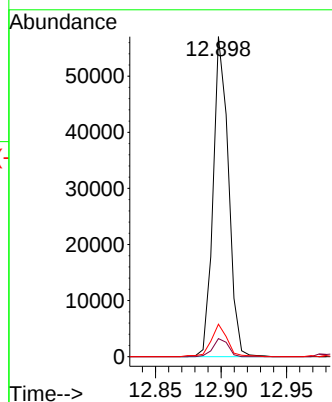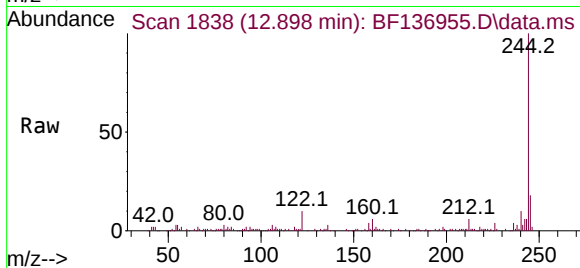

#81

Benzo(a)anthracene

Concen: 18.425 ng

RT: 13.957 min Scan# 2018

Delta R.T. -0.006 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52




Tgt Ion:228 Resp: 135533


Ion Ratio Lower Upper

228 100

226 27.5 21.4 32.0

229 19.6 14.9 22.3

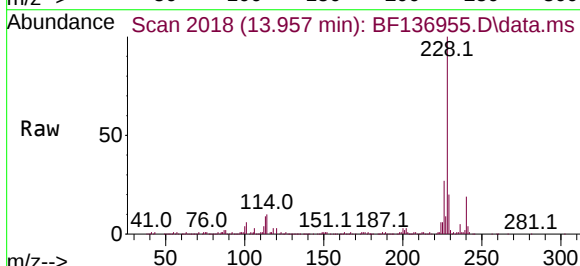



#83

Chrysene

Concen: 33.075 ng

RT: 13.992 min Scan# 2016

Delta R.T. -0.006 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52

Instrument :

BNA_F

ClientSampleId :

GHL-SS-18-2-4DL





Tgt Ion:228 Resp: 237922

Ion Ratio Lower Upper

228 100

226 29.4 24.7 37.1

229 20.1 15.4 23.0

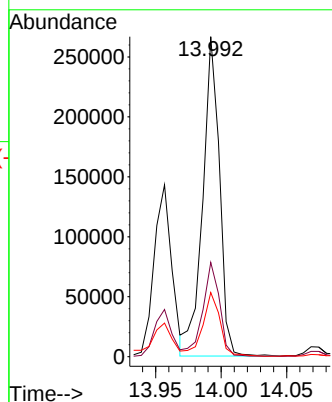

#84

Bis(2-ethylhexyl)phthalate

Concen: 6.206 ng

RT: 13.945 min Scan# 2016

Delta R.T. -0.006 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52




Tgt Ion:149 Resp: 29547


Ion Ratio Lower Upper

149 100

167 26.7 20.9 31.3

279 5.2 2.9 4.3#





#86

Perylene-d12

Concen: 20.000 ng

RT: 15.451 min Scan# 21

Delta R.T. 0.006 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52

Instrument :

BNA_F

ClientSampleId :

GHL-SS-18-2-4DL





Tgt Ion:264 Resp: 119762

Ion Ratio Lower Upper

264 100

260 22.6 18.3 27.5

265 22.0 17.0 25.6

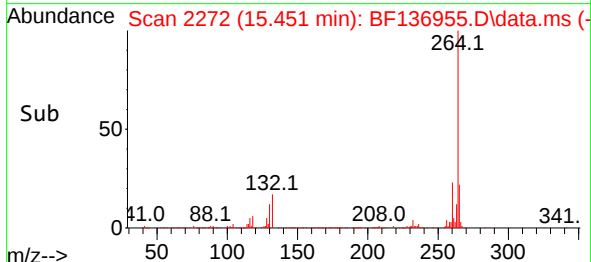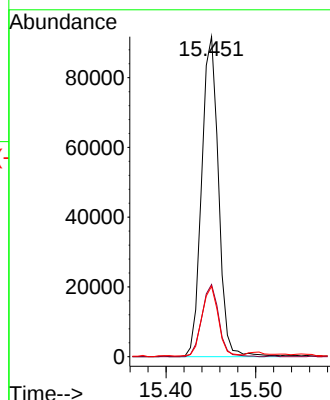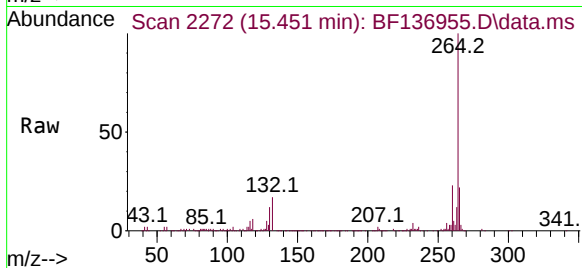

#87

Indeno(1,2,3-cd)pyrene

Concen: 2.614 ng

RT: 16.962 min Scan# 2529

Delta R.T. 0.012 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52




Tgt Ion:276 Resp: 22607


Ion Ratio Lower Upper

276 100

138 21.4 18.7 28.1

277 25.6 20.2 30.2

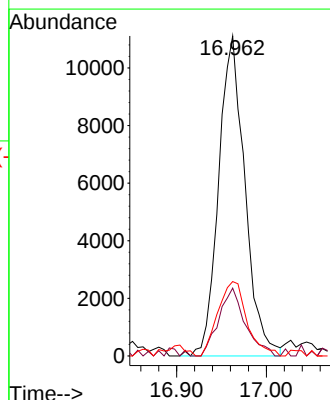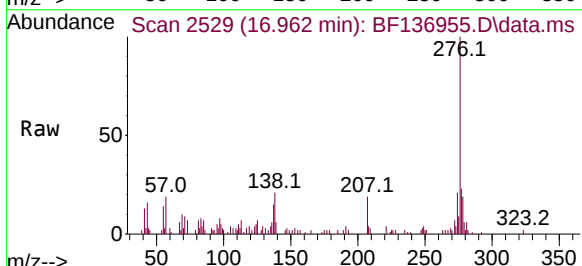



#88

Benzo(b)fluoranthene

Concen: 15.000 ng

RT: 15.015 min Scan# 2198

Delta R.T. 0.000 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52

Instrument :

BNA_F

ClientSampleId :

GHL-SS-18-2-4DL





Tgt Ion:252 Resp: 119986

Ion Ratio Lower Upper

252 100

253 22.3 17.4 26.0

125 10.0 7.4 11.2

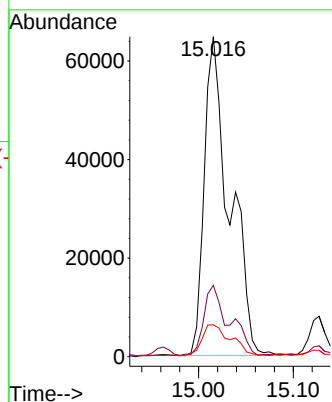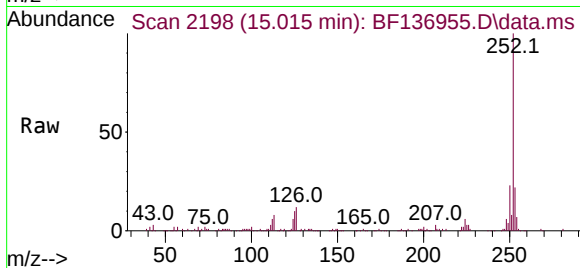

#89

Benzo(k)fluoranthene

Concen: 15.875 ng

RT: 15.015 min Scan# 2198

Delta R.T. -0.029 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52




Tgt Ion:252 Resp: 119986


Ion Ratio Lower Upper

252 100

253 22.3 17.0 25.6

125 10.0 8.2 12.4

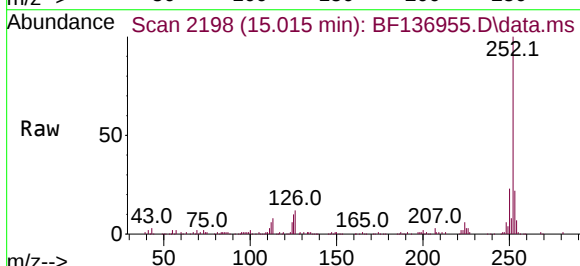



#90

Benzo(a)pyrene

Concen: 7.017 ng

RT: 15.386 min Scan# 21

Delta R.T. 0.000 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52

Instrument :

BNA_F

ClientSampleId :

GHL-SS-18-2-4DL





Tgt Ion:252 Resp: 47382

Ion Ratio Lower Upper

252 100

253 21.2 17.0 25.6

125 10.5 8.8 13.2

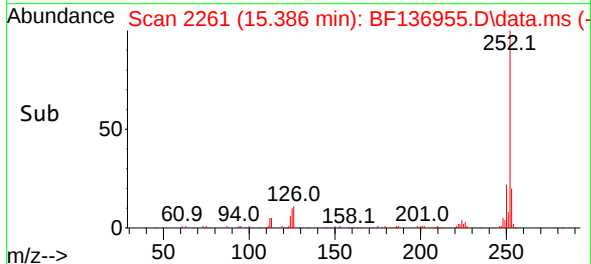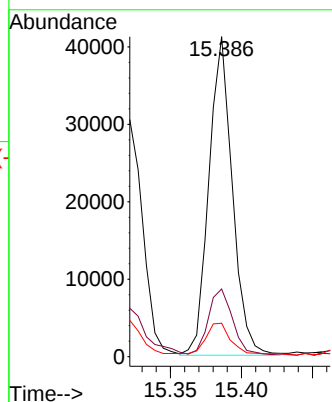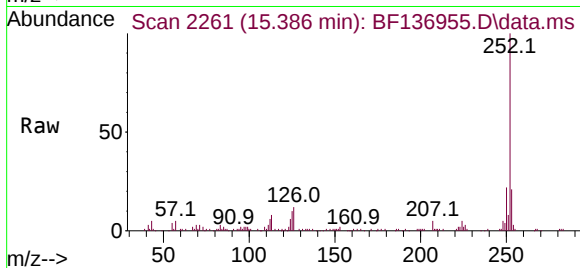

#92

Benzo(g,h,i)perylene

Concen: 2.549 ng

RT: 17.427 min Scan# 2608

Delta R.T. 0.018 min

Lab File: BF136955.D

Acq: 04 Jan 2024 22:52

Tgt Ion:276 Resp: 18520

Ion Ratio Lower Upper

276 100

277 22.4 18.3 27.5

138 18.1 15.6 23.4

