
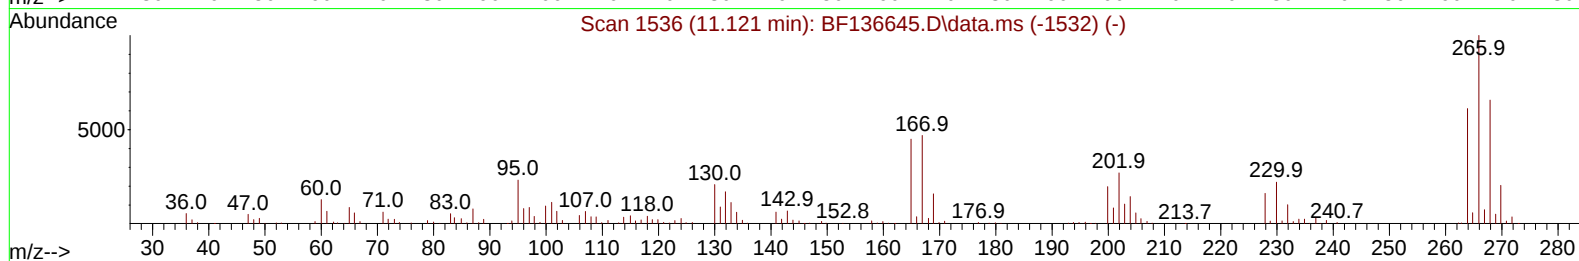
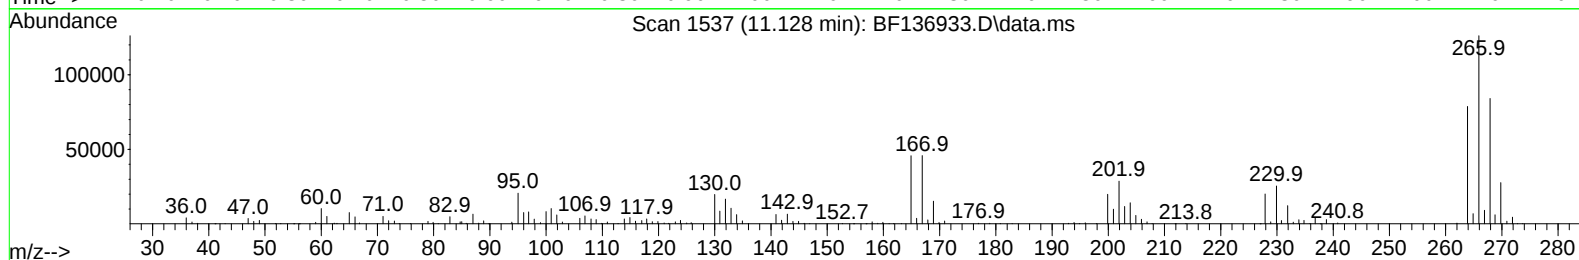


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010424\
Data File : BF136933.D
Acq On : 04 Jan 2024 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 12:22:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

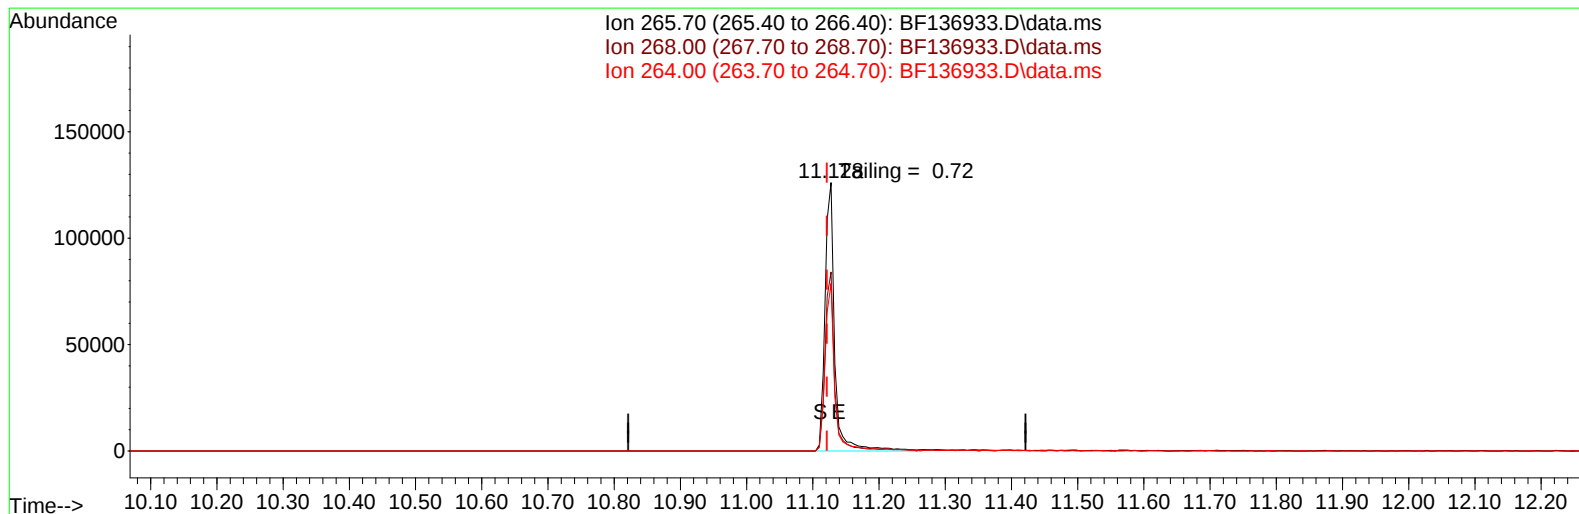




TIC: BF136933.D\data.ms

(70) Pentachlorophenol (C)**11.128min (+ 0.006) 29185.24 ng****response 128966**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	66.67
264.00	61.20	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010424\
Data File : BF136933.D
Acq On : 04 Jan 2024 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 12:22:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

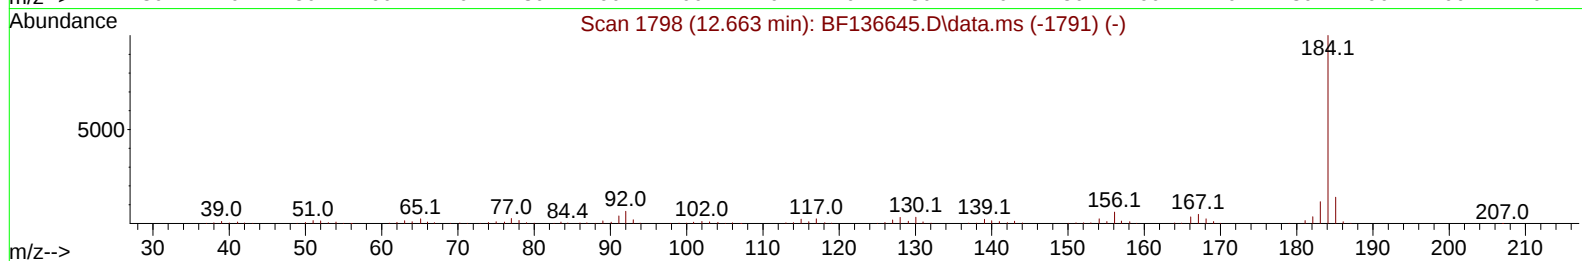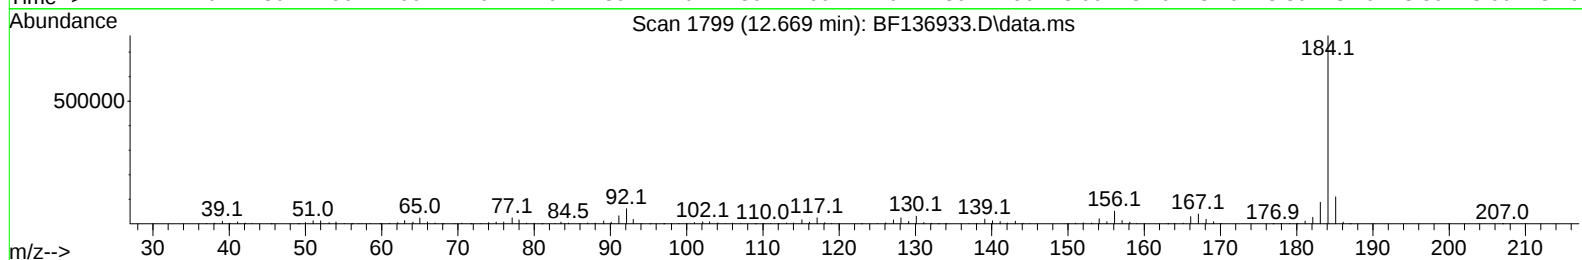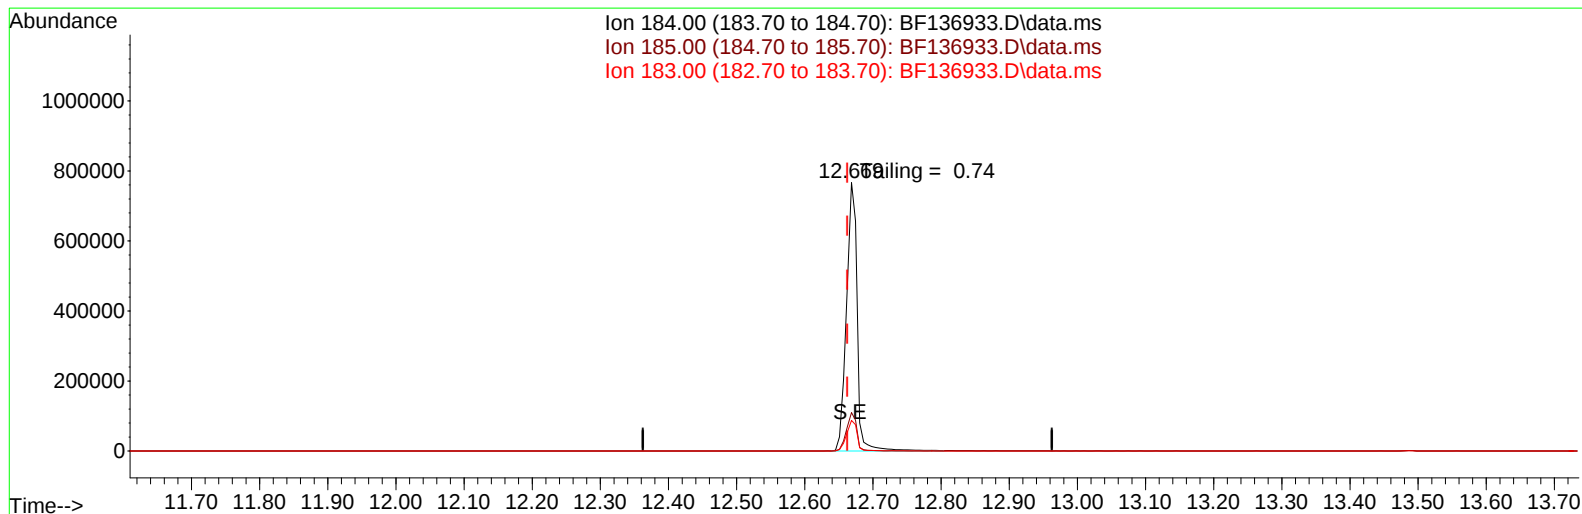

TIC: BF136933.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 79753.25 ng m

response 832460

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.31
183.00	11.60	11.39
0.00	0.00	0.00