
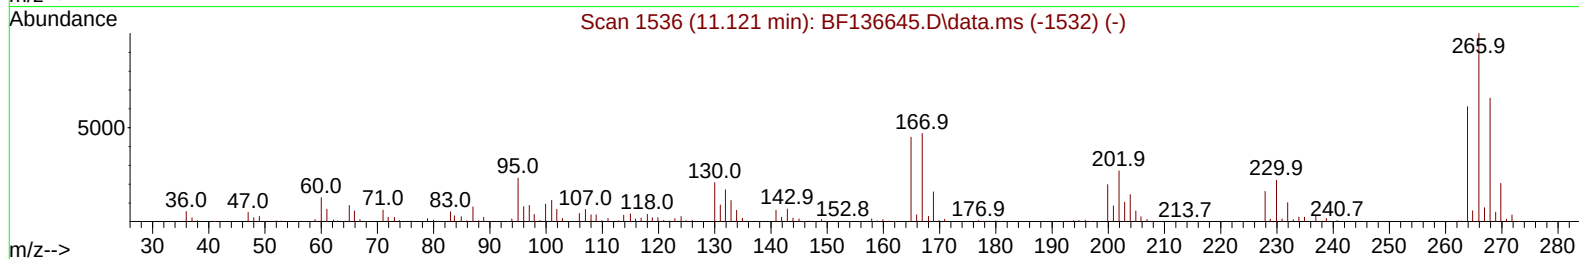
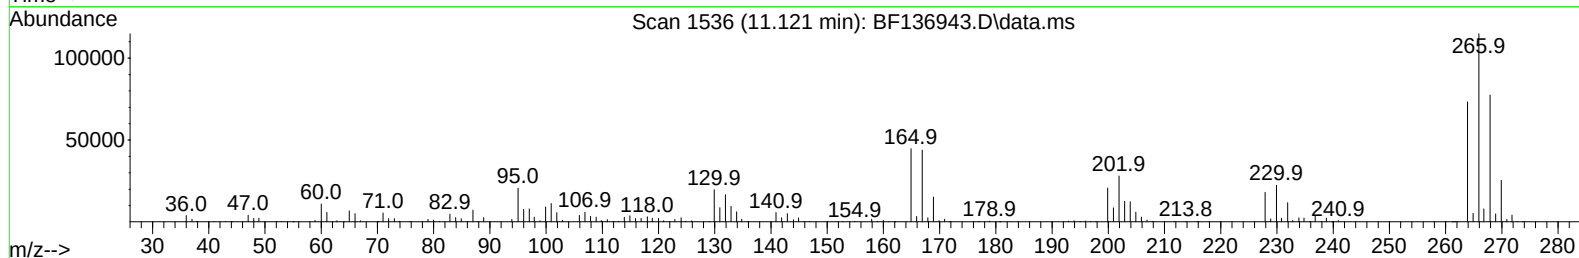


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010424\
Data File : BF136943.D
Acq On : 04 Jan 2024 16:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 16:54:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

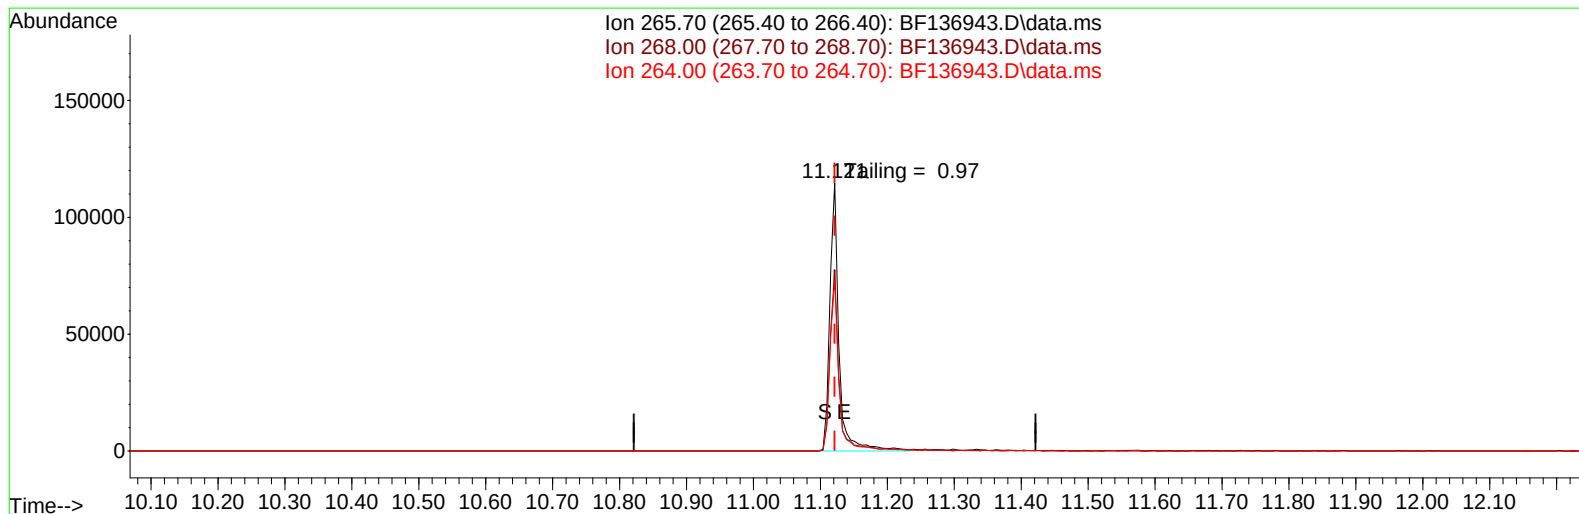

TIC: BF136943.D\data.ms




(70) Pentachlorophenol (C)

11.121min (-0.000) 28846.55 ng

response 109830

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	67.48
264.00	61.20	63.78
0.00	0.00	0.00

Quant Time: Jan 04 16:54:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

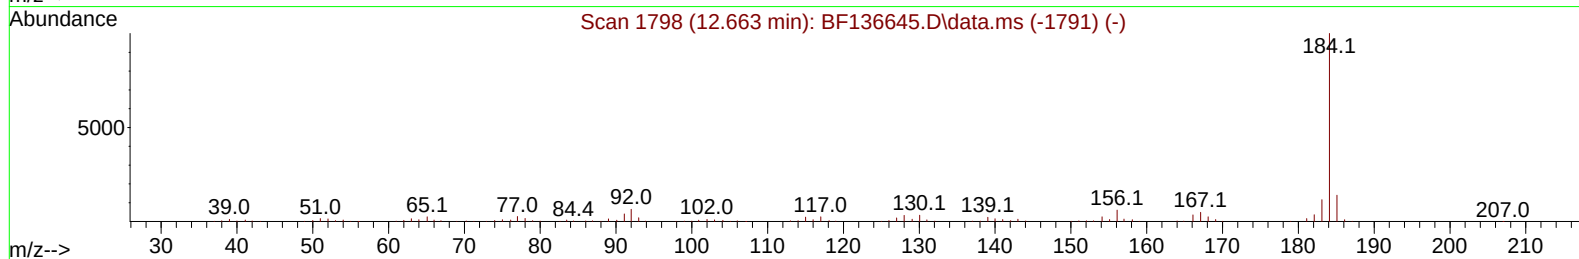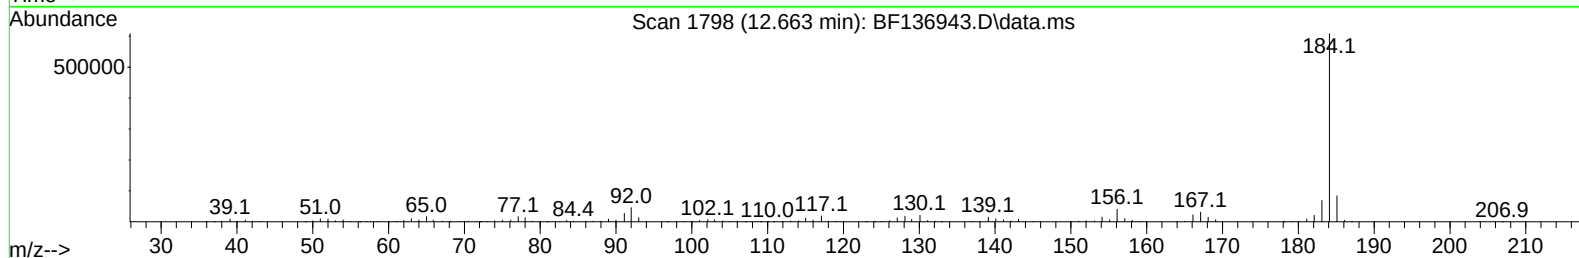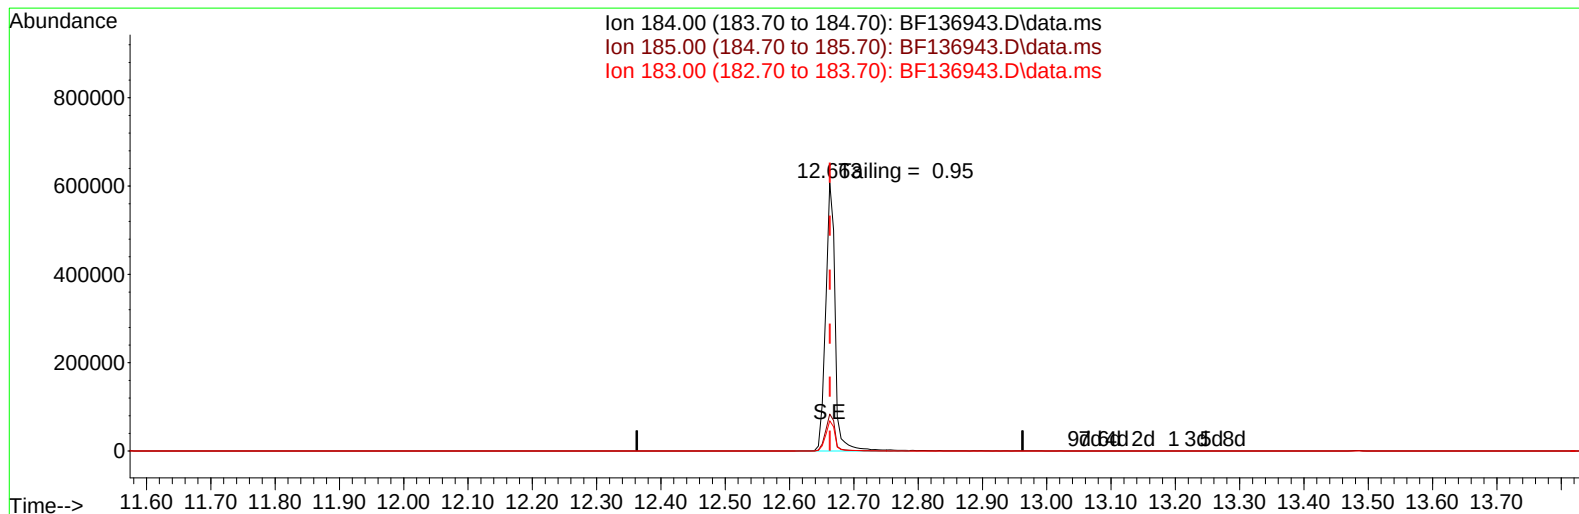

TIC: BF136943.D\data.ms

(77) Benzidine

12.663min (-0.000) 295105.68 ng m

response **626501**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.00	13.79
--------	-------	-------

183.00	11.60	11.31
--------	-------	-------

0.00 0.00 0.00