
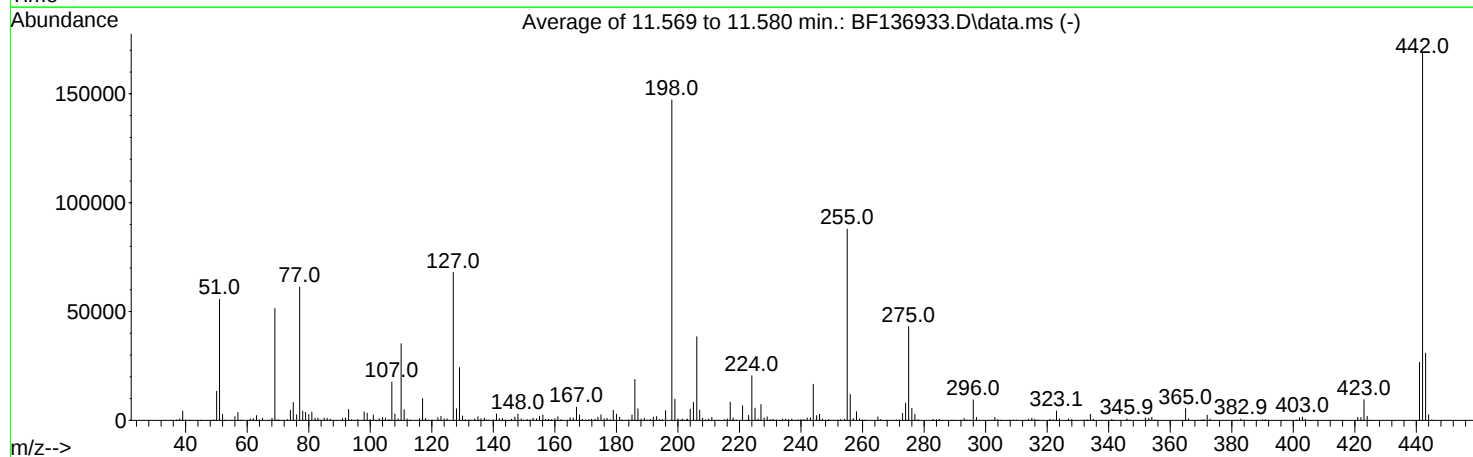


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010424\
Data File : BF136933.D
Acq On : 04 Jan 2024 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

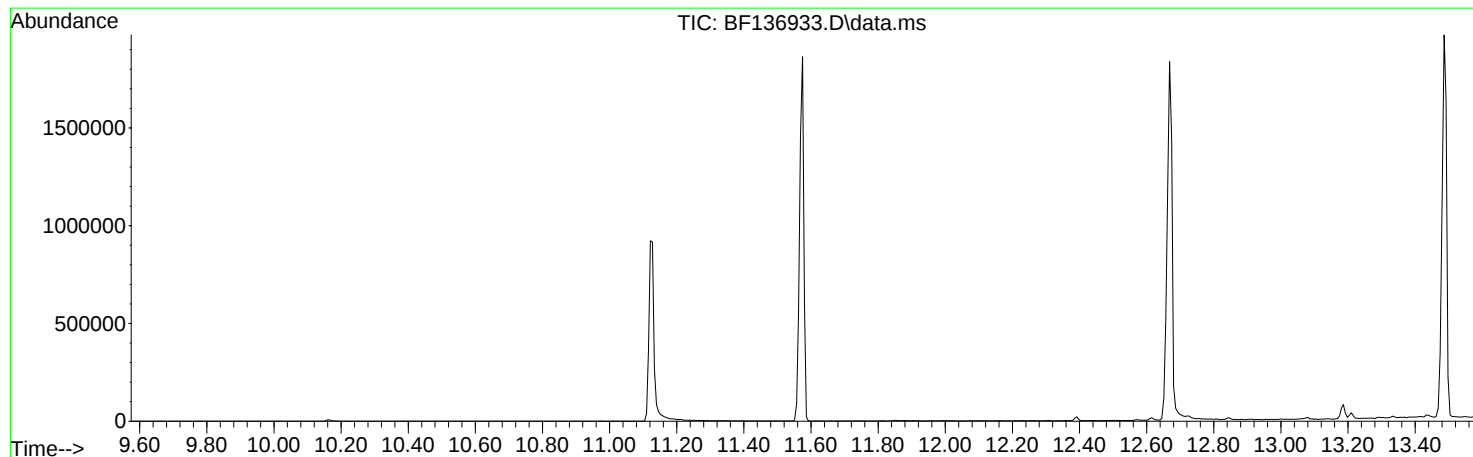

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	55603	PASS
68	69	0.00	2	1.8	940	PASS
69	198	0.00	100	34.9	51396	PASS
70	69	0.00	2	0.5	278	PASS
127	198	10	80	46.2	67995	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	147216	PASS
199	198	5	9	6.6	9783	PASS
275	198	10	60	29.3	43085	PASS
365	198	1	100	3.7	5445	PASS
441	198	0.01	100	18.1	26677	PASS
442	442	50	100	100.0	169000	PASS
443	442	15	24	18.3	30917	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/4/2024	BNA_F	<u>BF136933.D</u>
Compound Name	Response	Retention Time
DDT	391573	13.486
DDD	19046	13.186
DDE	1041	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20087	411660	4.88

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010424\
Data File : BF136933.D
Acq On : 04 Jan 2024 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 04 12:22:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

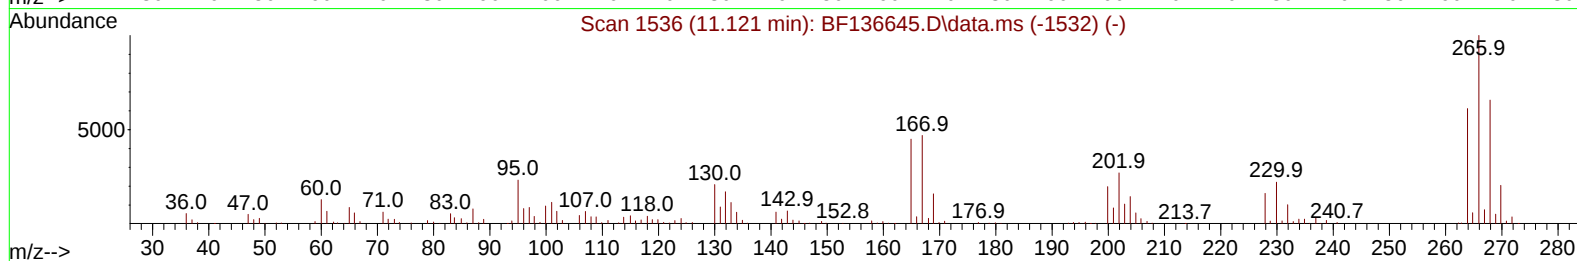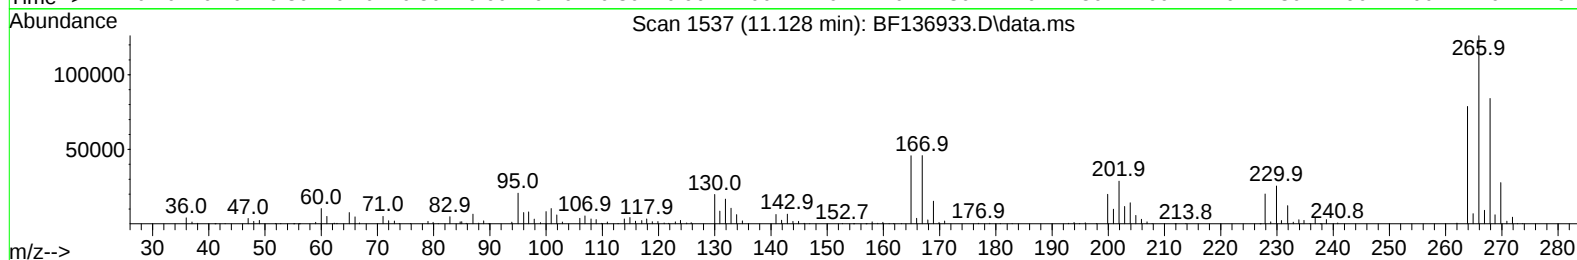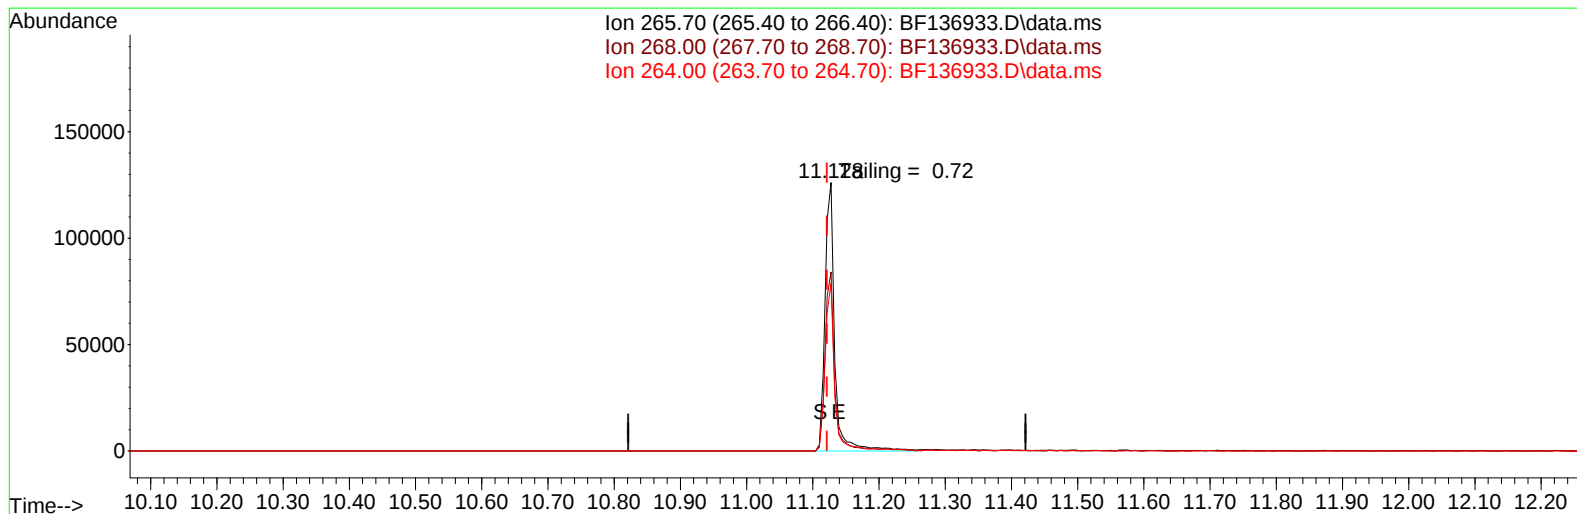

TIC: BF136933.D\data.ms

(70) Pentachlorophenol (C)

11.128min (+ 0.006) 29185.24 ng




response 128966

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	66.67
264.00	61.20	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010424\
Data File : BF136933.D
Acq On : 04 Jan 2024 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 04 12:22:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

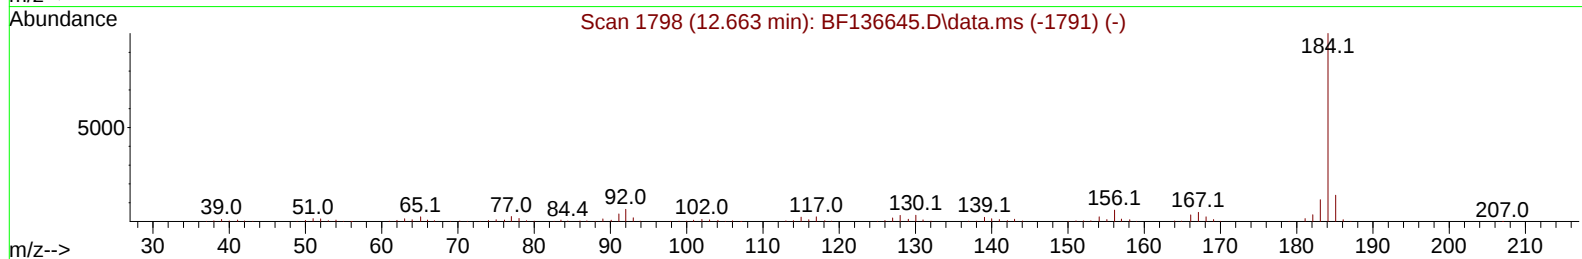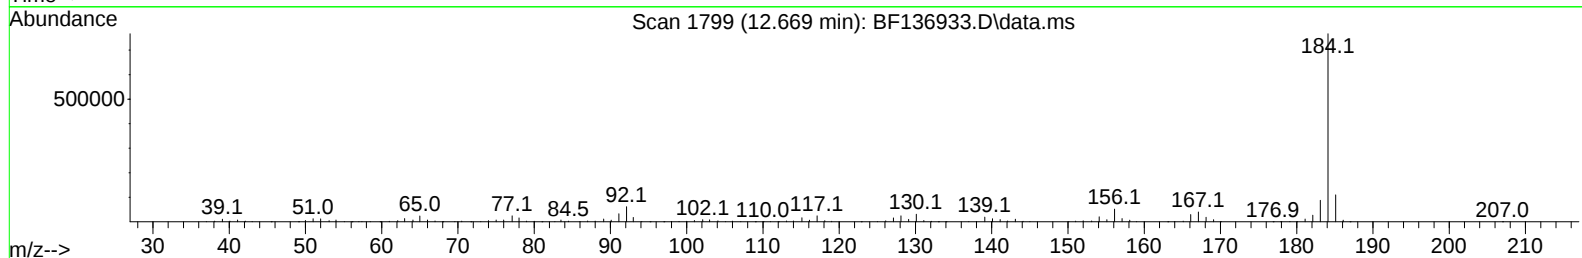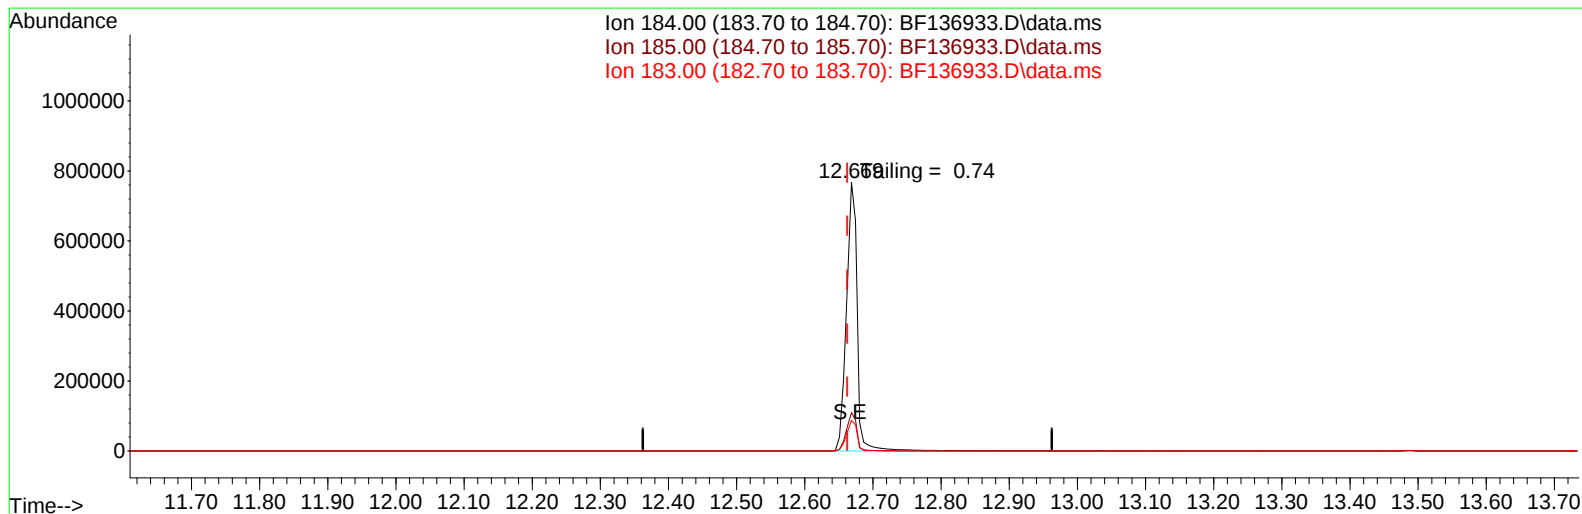

TIC: BF136933.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 79753.25 ng m

response 832460

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.31
183.00	11.60	11.39
0.00	0.00	0.00