
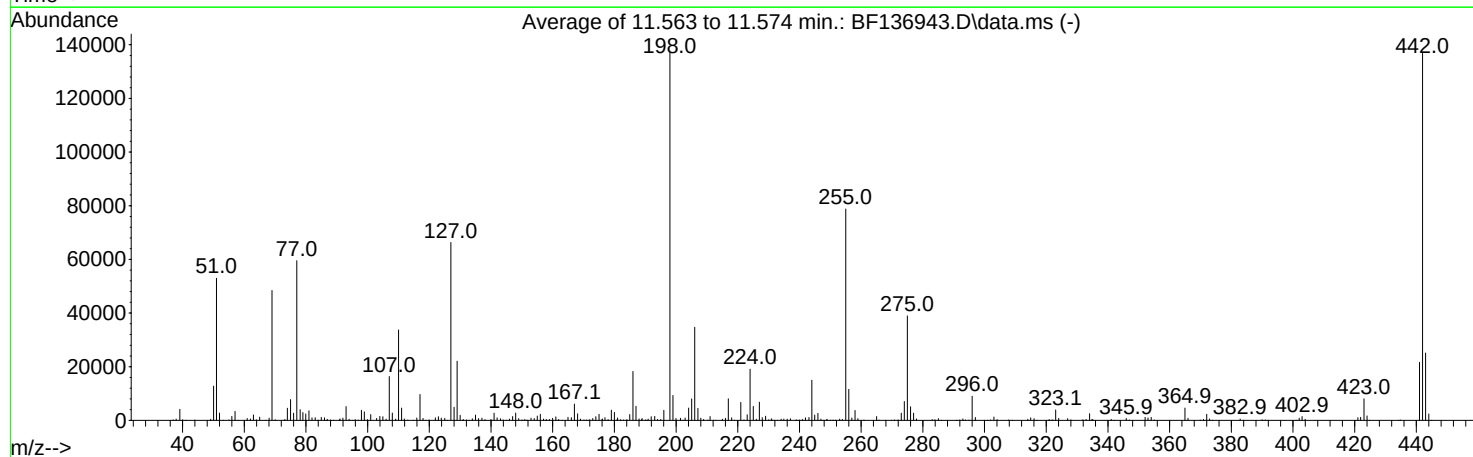


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010424\
Data File : BF136943.D
Acq On : 04 Jan 2024 16:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

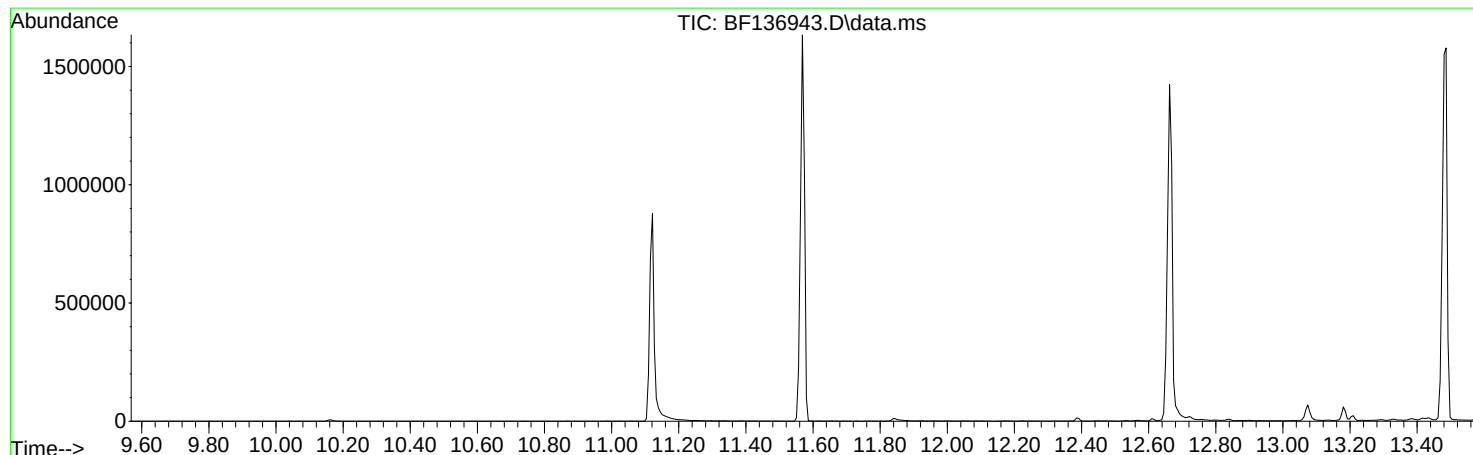

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	52989	PASS
68	69	0.00	2	1.7	822	PASS
69	198	0.00	100	35.3	48403	PASS
70	69	0.00	2	0.5	223	PASS
127	198	10	80	48.4	66312	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	137107	PASS
199	198	5	9	6.8	9299	PASS
275	198	10	60	28.4	38936	PASS
365	198	1	100	3.4	4614	PASS
441	198	0.01	100	15.8	21644	PASS
442	442	50	100	100.0	136749	PASS
443	442	15	24	18.3	25082	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/4/2024	BNA_F	<u>BF136943.D</u>
Compound Name	Response	Retention Time
DDT	330682	13.486
DDD	14605	13.18
DDE	1115	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15720	346402	4.54

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010424\
Data File : BF136943.D
Acq On : 04 Jan 2024 16:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 04 16:54:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

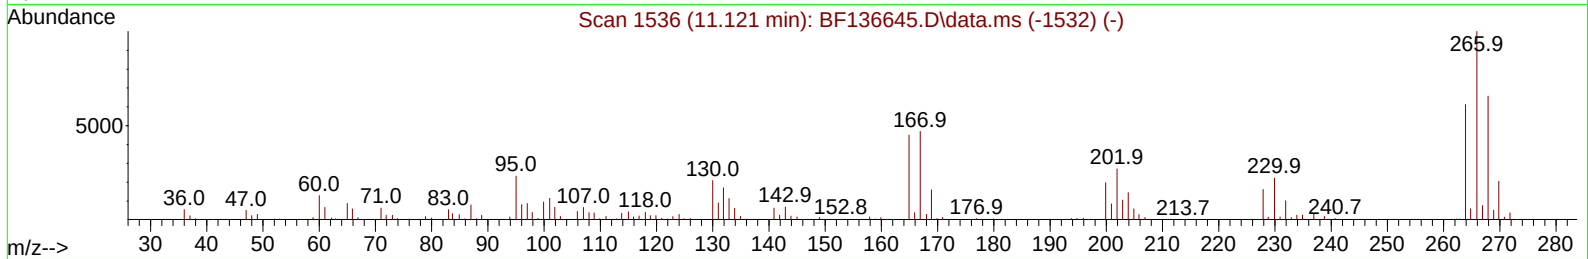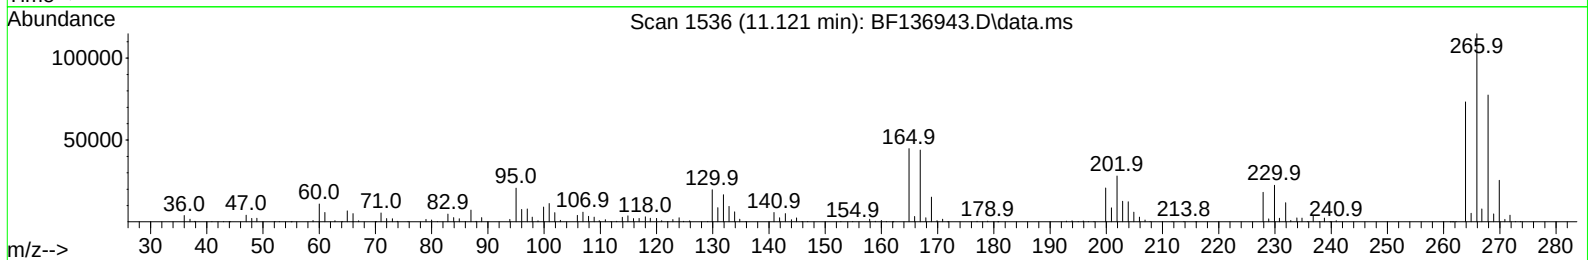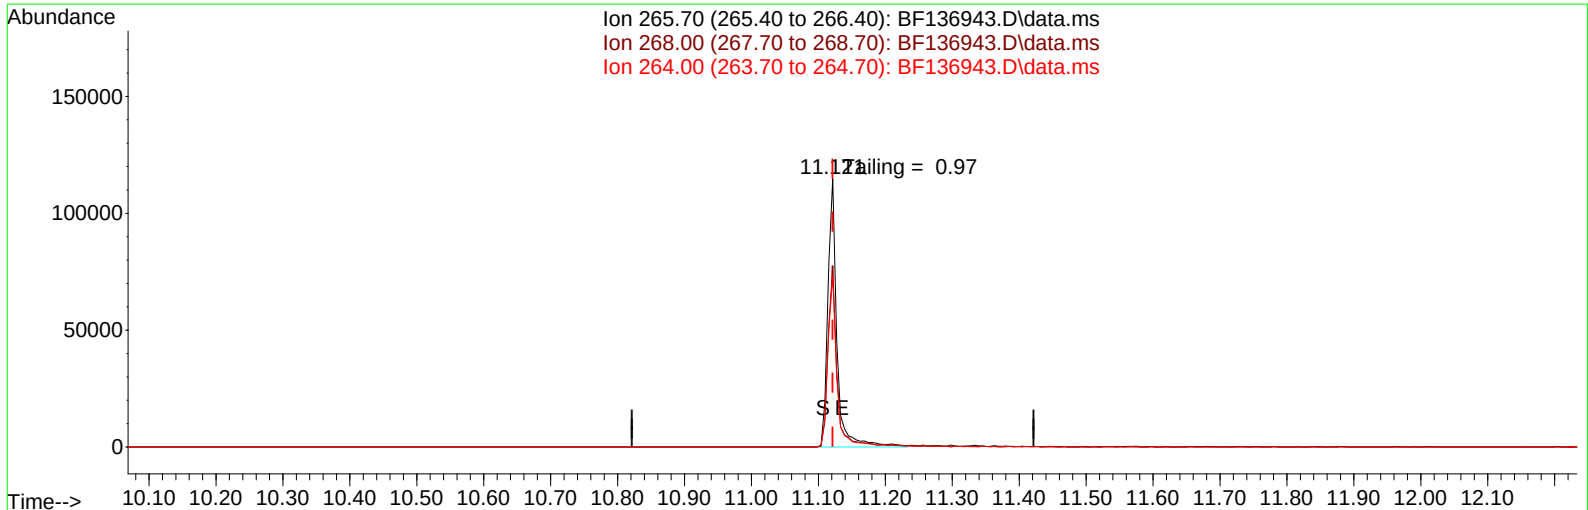

TIC: BF136943.D\data.ms

(70) Pentachlorophenol (C)

11.121min (-0.000) 28846.55 ng




response 109830

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	67.48
264.00	61.20	63.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010424\
Data File : BF136943.D
Acq On : 04 Jan 2024 16:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 04 16:54:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

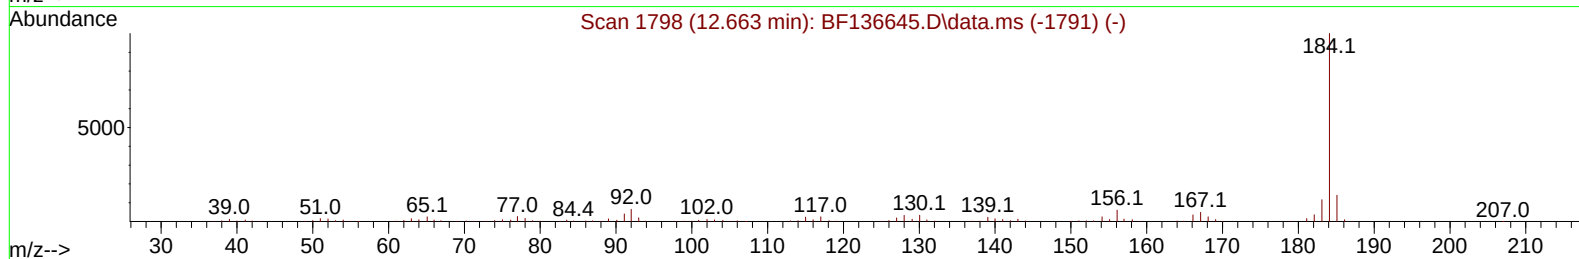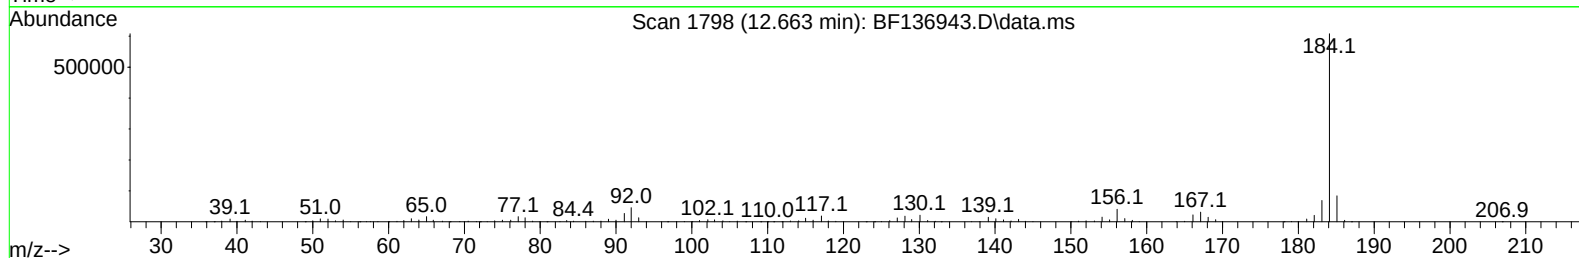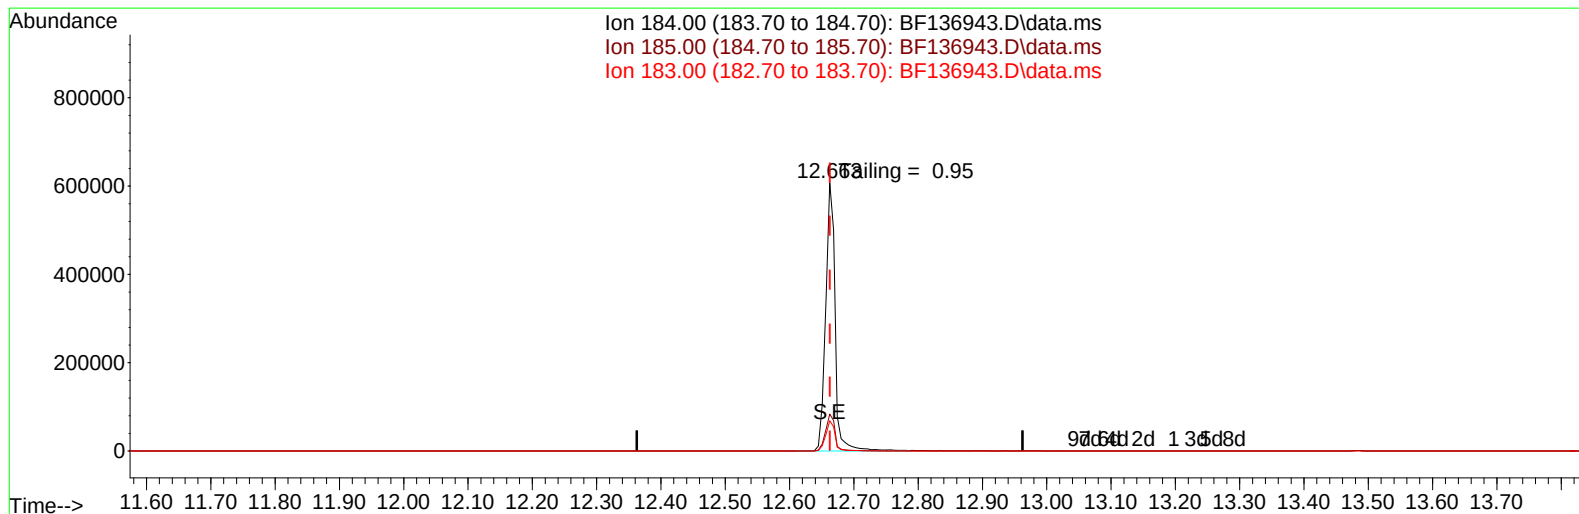

TIC: BF136943.D\data.ms

(77) Benzidine

12.663min (-0.000) 295105.68 ng m

response 626501

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.79
183.00	11.60	11.31
0.00	0.00	0.00