
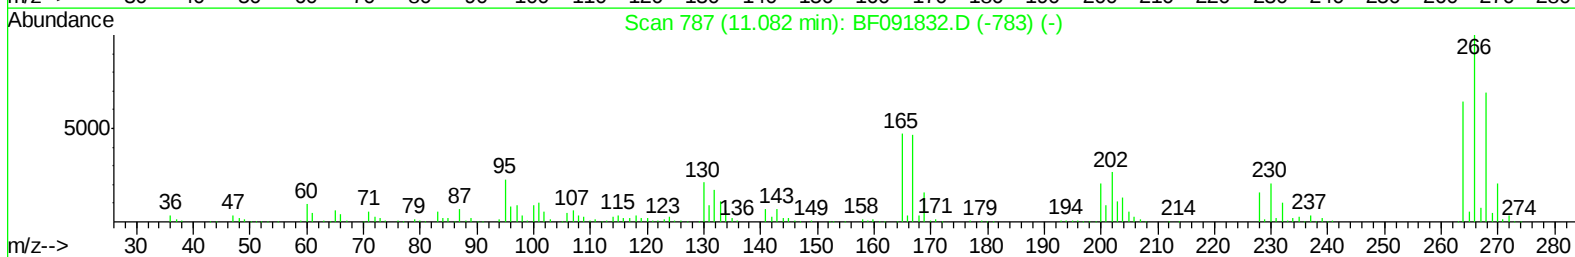
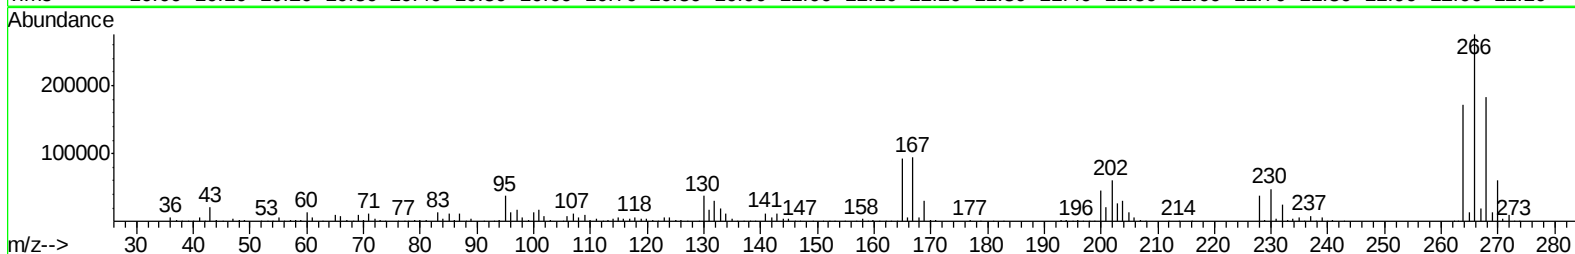


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010517\
Data File : BF092096.D
Acq On : 5 Jan 2017 17:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 01:26:24 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 00:13:42 2017
Response via : Initial Calibration

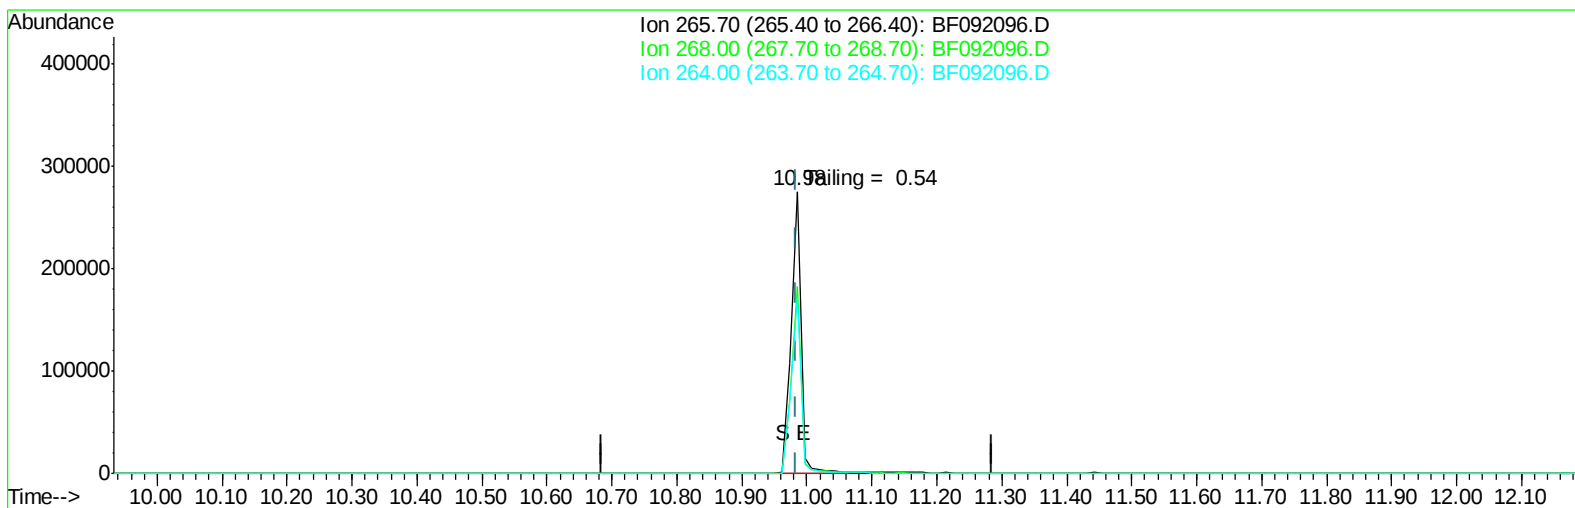

TIC: BF092096.D

(69) Pentachlorophenol (C)




10.985min (+0.000) 0.00ng

response 292483

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.33
264.00	62.90	62.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010517\
 Data File : BF092096.D
 Acq On : 5 Jan 2017 17:42
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 01:26:24 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 06 00:13:42 2017
 Response via : Initial Calibration

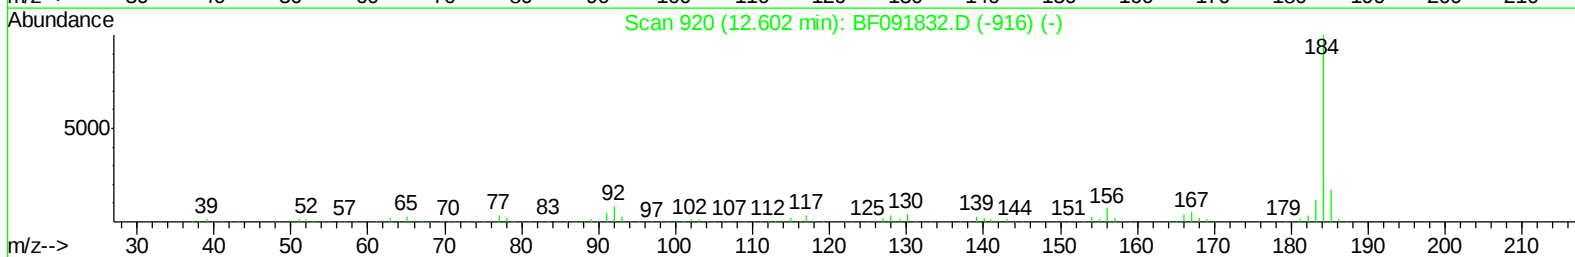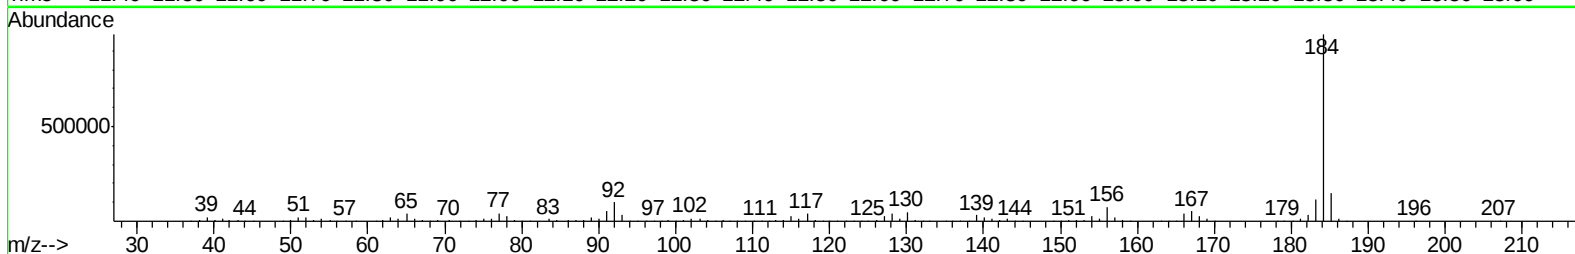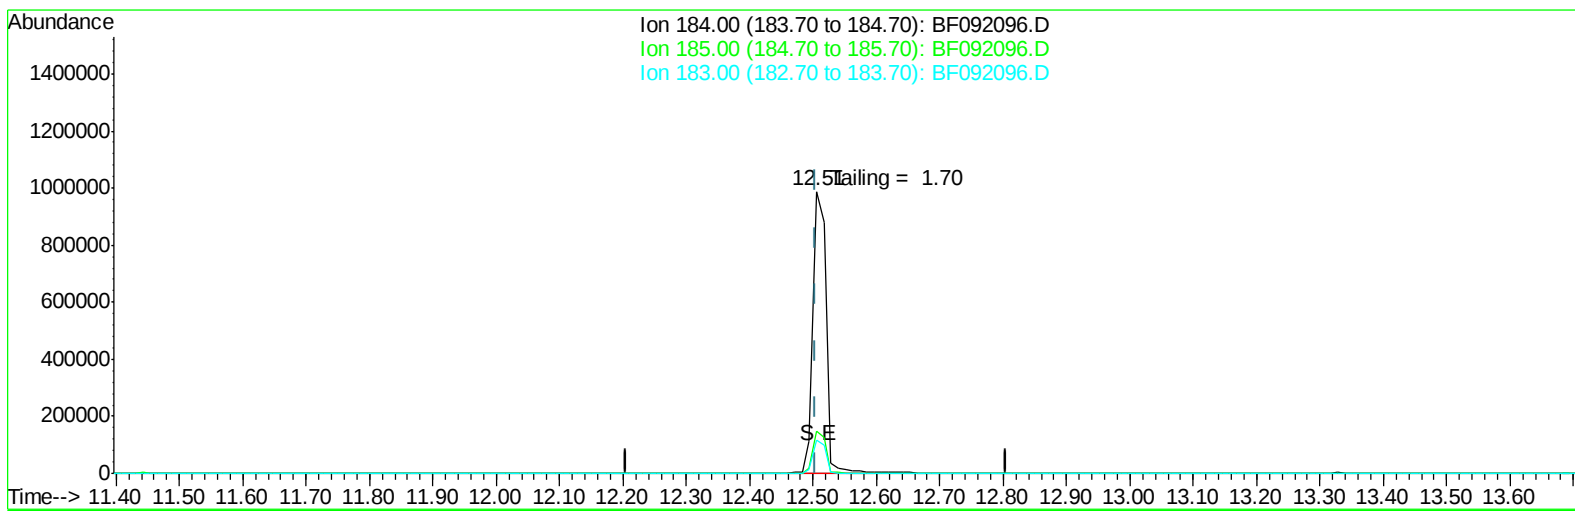

TIC: BF092096.D

(76) Benzidine

12.505min (+0.000) -20.00ng

response 1445027

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.11
183.00	11.50	11.61
0.00	0.00	0.00