

Data Path : Z:\HPCHEM1\BNA F\DATA\BF010517\
 Data File : BF092102.D
 Acq On : 5 Jan 2017 21:25
 Operator : UM/SJ
 Sample : I1003-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DSN001

Quant Time: Jan 06 00:31:17 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 06 00:13:42 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.65	152	192146	20.00	ng	0.00
21) Naphthalene-d8	7.93	136	737579	20.00	ng	-0.01
38) Acenaphthene-d10	9.68	164	397381	20.00	ng	-0.01
63) Phenanthrene-d10	11.17	188	706043	20.00	ng	0.00
75) Chrysene-d12	13.80	240	562618	20.00	ng	0.00
86) Perylene-d12	15.17	264	390064	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	911515	79.21	ng	0.00
7) Phenol-d6	6.31	99	676377	48.14	ng	-0.01
23) Nitrobenzene-d5	7.22	82	1332024	100.42	ng	0.00
41) 2,4,6-Tribromophenol	10.48	330	519470	157.96	ng	0.00
44) 2-Fluorobiphenyl	9.02	172	1993966	106.00	ng	0.00
78) Terphenyl-d14	12.76	244	1918160	82.69	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF010517\
Data File : BF092102.D
Acq On : 5 Jan 2017 21:25
Operator : UM/SJ
Sample : I1003-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN001

Quant Time: Jan 06 00:31:17 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 00:13:42 2017
Response via : Initial Calibration

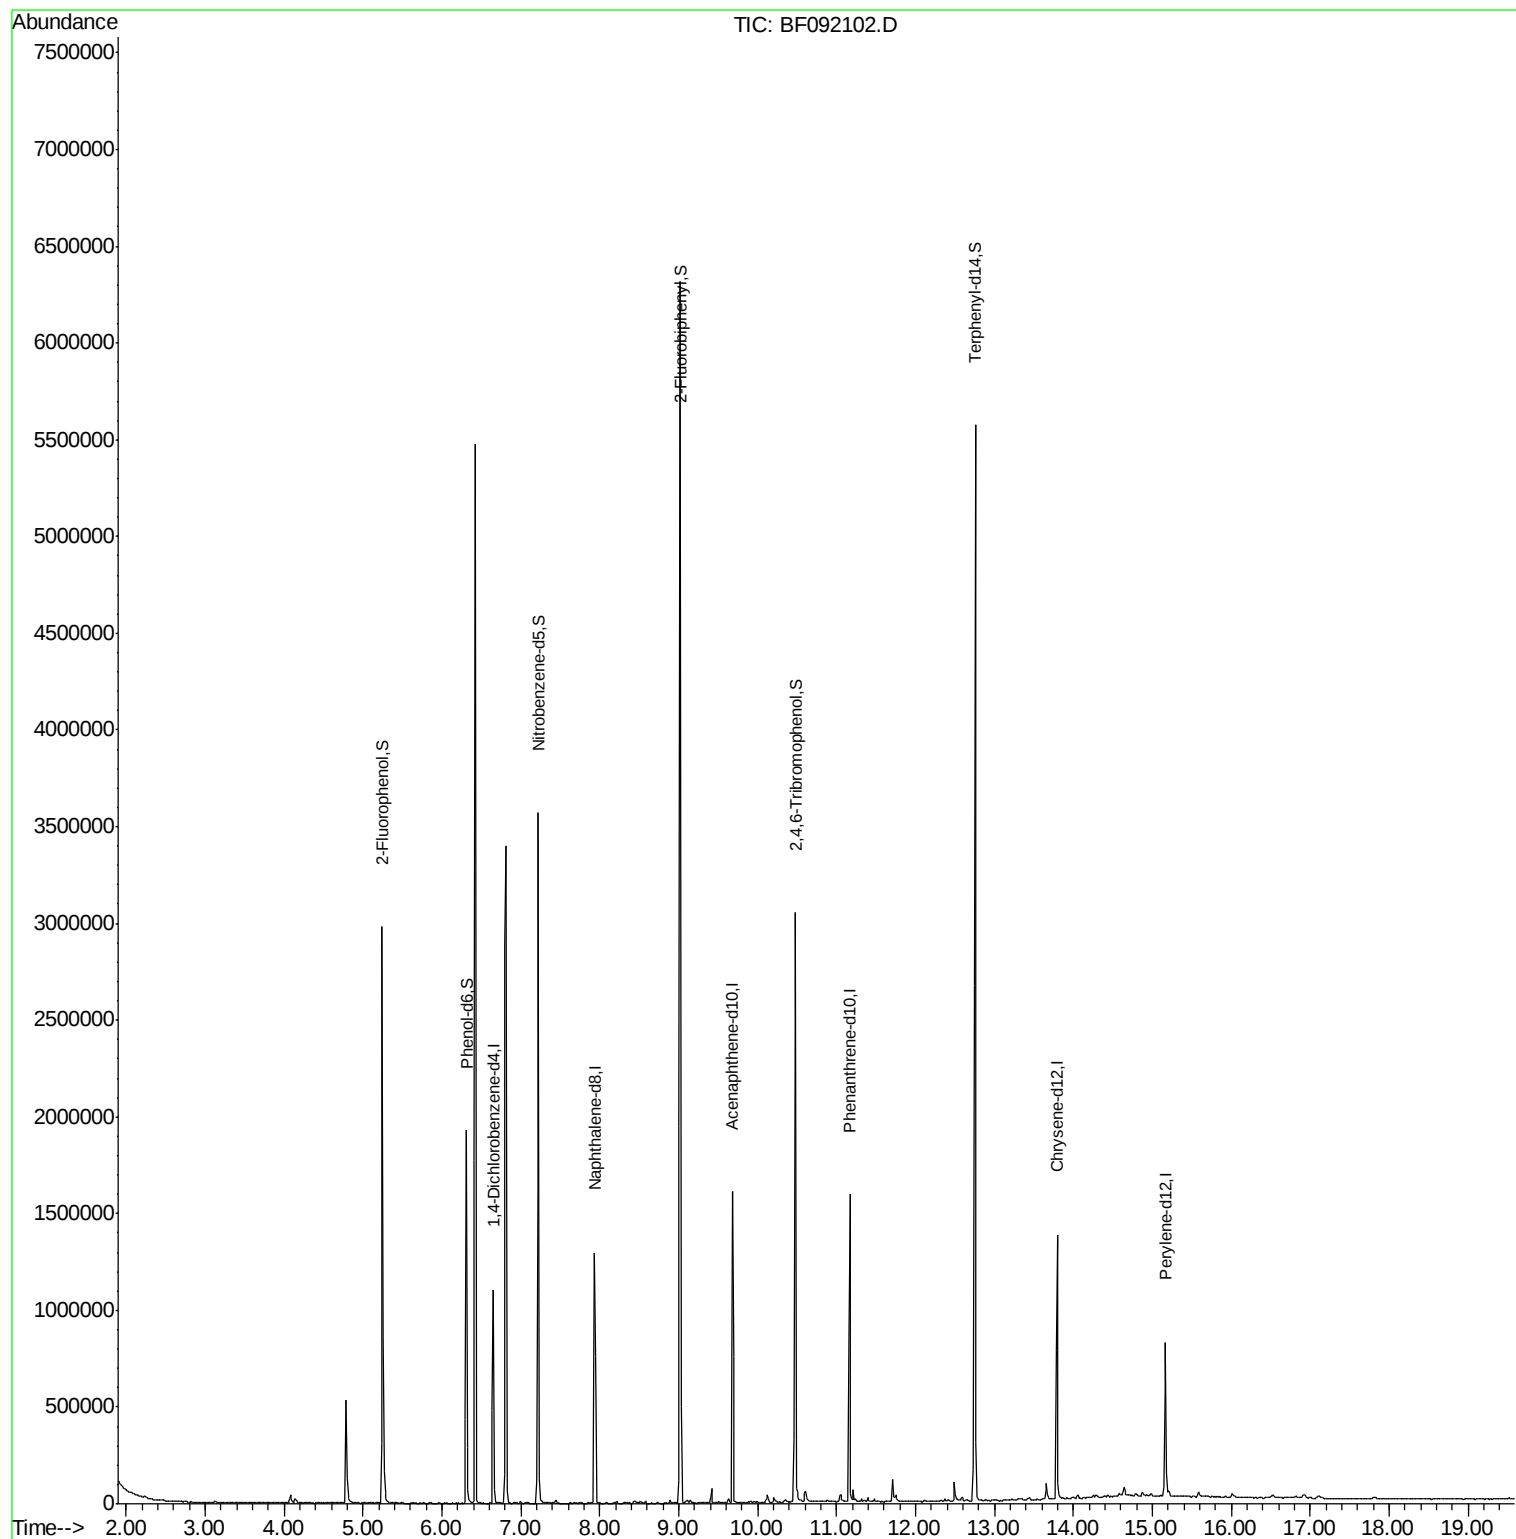

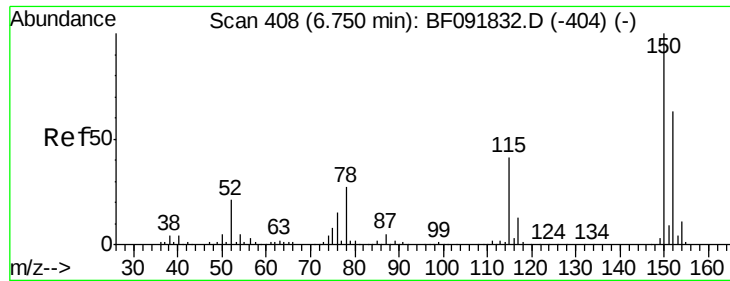

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.65 min Scan# 417

Delta R.T. -0.00 min

Lab File: BF092102.D

Acq: 5 Jan 2017 21:25

Instrument :

BNA_F

ClientSampleId :

DSN001


Tot Ion:152 Resp: 192146

Ion Ratio Lower Upper

152 100

150 153.8 124.9 187.3




115 57.2 46.0 69.0

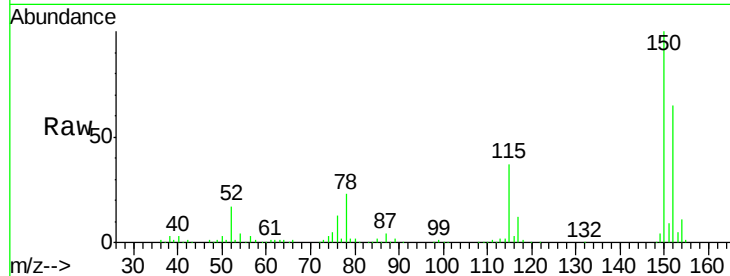

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

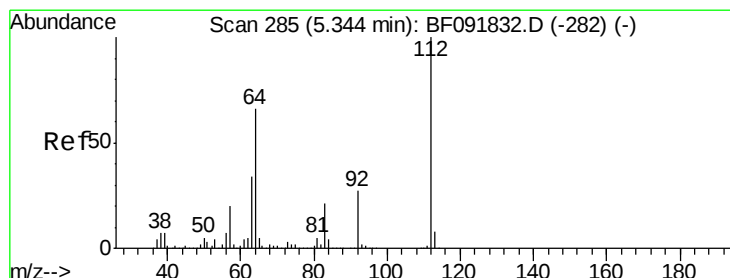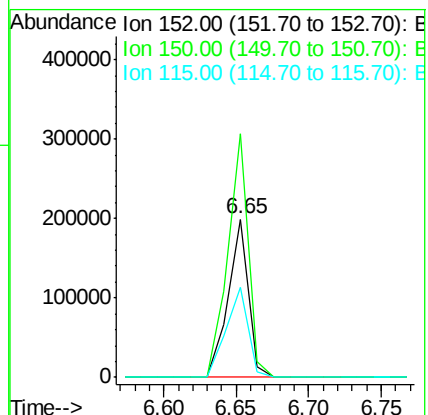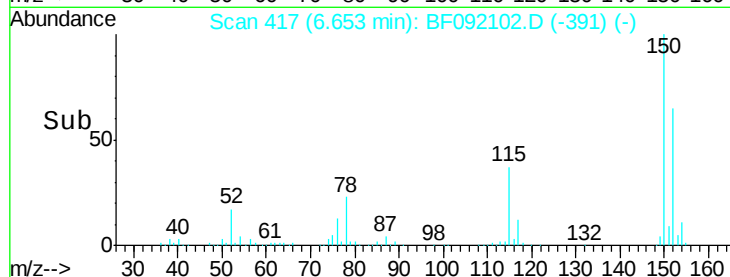

#5

2-Fluorophenol

Concen: 79.21 ng

RT: 5.25 min Scan# 294

Delta R.T. -0.00 min

Lab File: BF092102.D

Acq: 5 Jan 2017 21:25


Tgt Ion:112 Resp: 911515

Ion Ratio Lower Upper

112 100

64 60.4 46.1 69.1



63 30.1 23.8 35.6

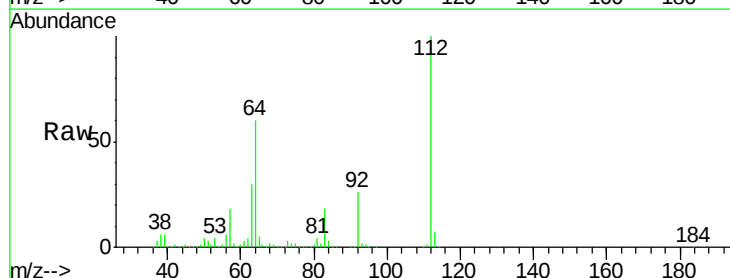


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

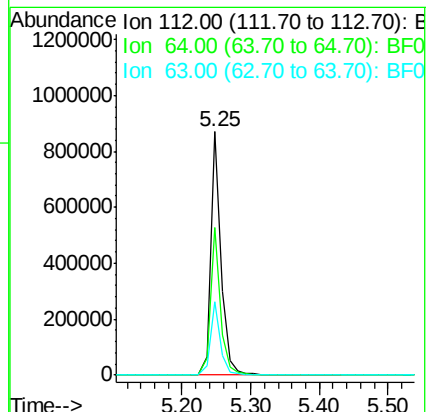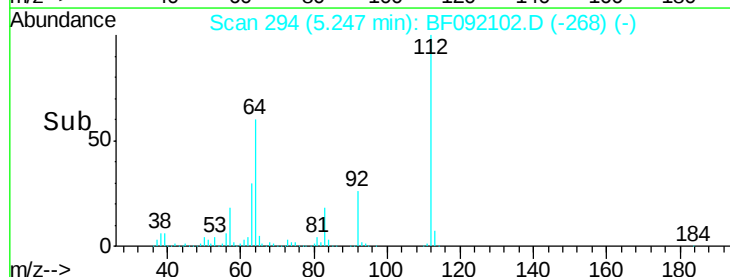

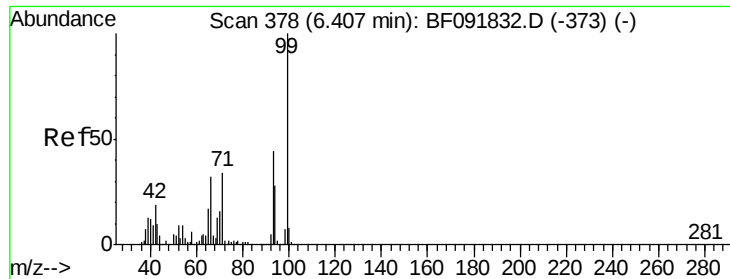

#7

Phenol-d6

Concen: 48.14 ng

RT: 6.31 min Scan# 387

Delta R.T. -0.01 min

Lab File: BF092102.D

Acq: 5 Jan 2017 21:25

Instrument :

BNA_F

ClientSampleId :

DSN001


Tot Ion: 99 Resp: 676377

Ion Ratio Lower Upper

99 100

42 15.7 15.6 23.4




71 29.7 27.5 41.3

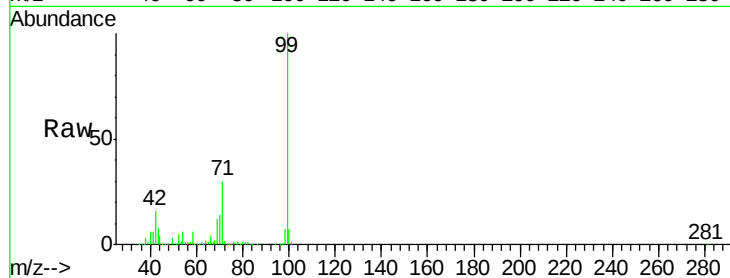

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

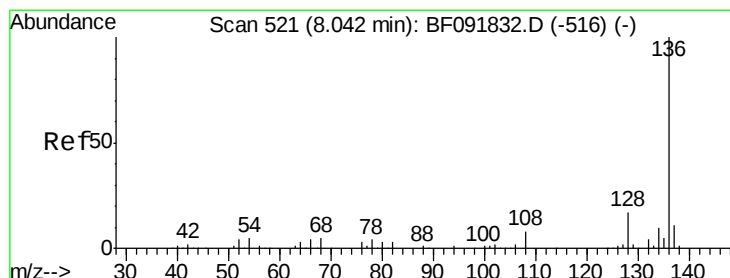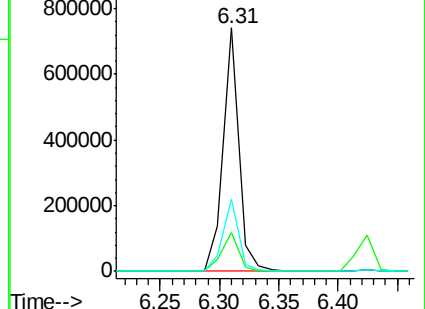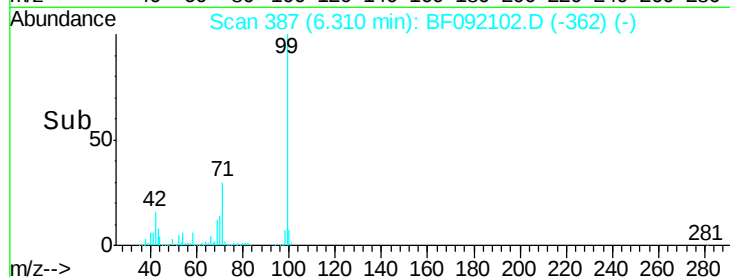

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.93 min Scan# 529

Delta R.T. -0.01 min

Lab File: BF092102.D

Acq: 5 Jan 2017 21:25

Tgt Ion: 136 Resp: 737579


Ion Ratio Lower Upper

136 100

137 11.5 8.4 12.6

54 9.9 4.5 6.7#

68 7.4 3.6 5.4#


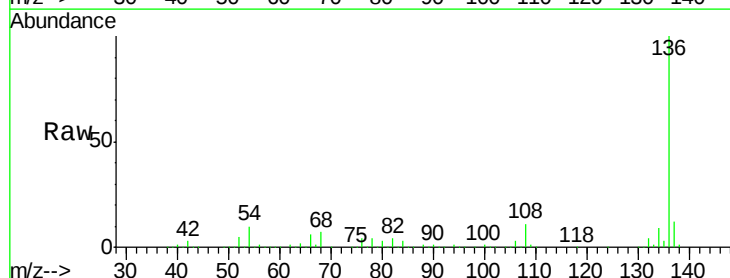



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

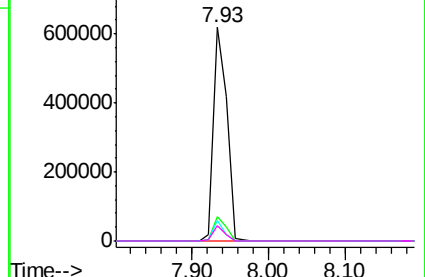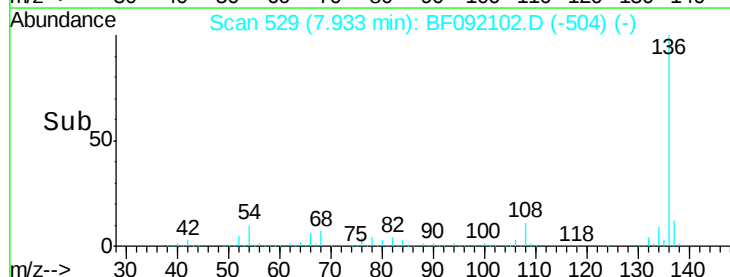




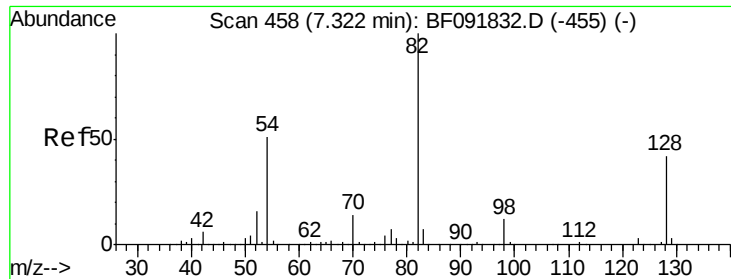


#23
 Nitrobenzene-d5
 Concen: 100.42 ng
 RT: 7.22 min Scan# 467
 Delta R.T. -0.00 min
 Lab File: BF092102.D
 Acq: 5 Jan 2017 21:25

Instrument :
 BNA_F
 ClientSampleId :
 DSN001

Tot Ion: 82 Resp: 1332024




Ion	Ratio	Lower	Upper
82	100		
128	42.0	34.6	52.0
54	49.6	39.5	59.3

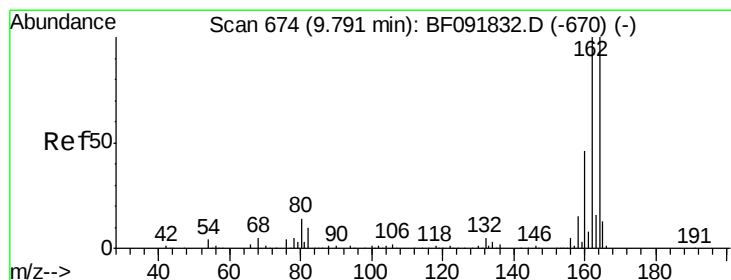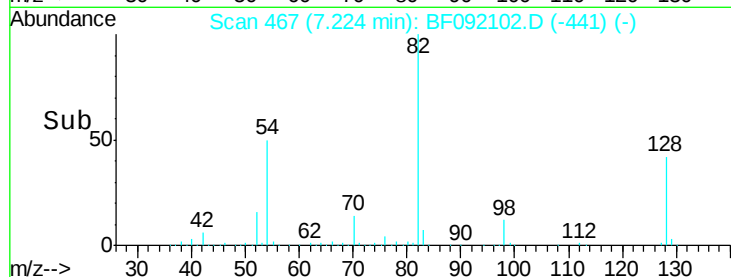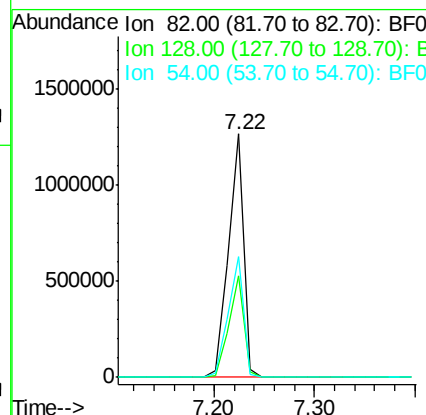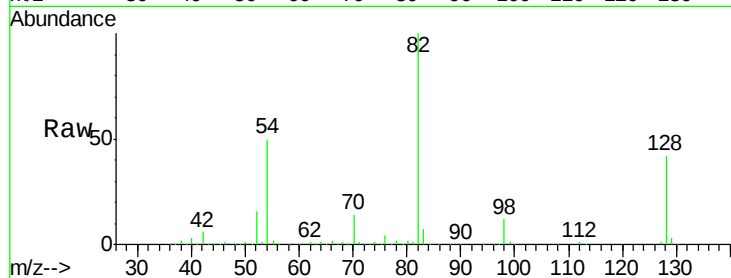


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.68 min Scan# 682
 Delta R.T. -0.01 min
 Lab File: BF092102.D
 Acq: 5 Jan 2017 21:25

Tgt Ion: 164 Resp: 397381

Ion	Ratio	Lower	Upper
164	100		
162	102.0	80.2	120.2
160	46.3	36.9	55.3

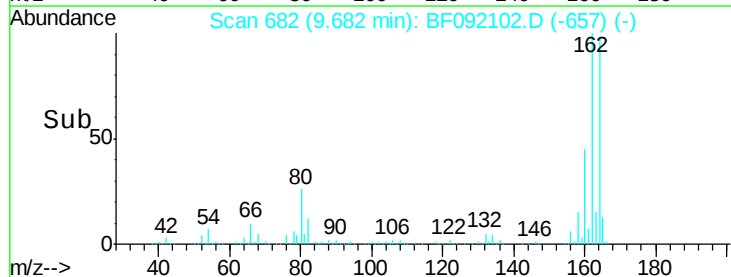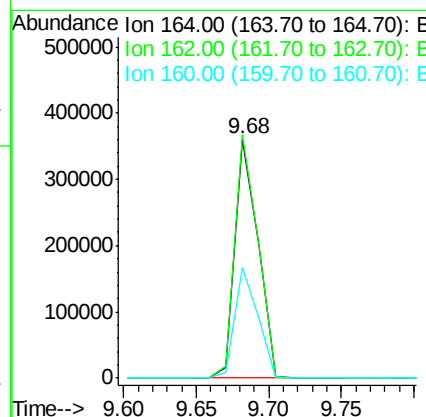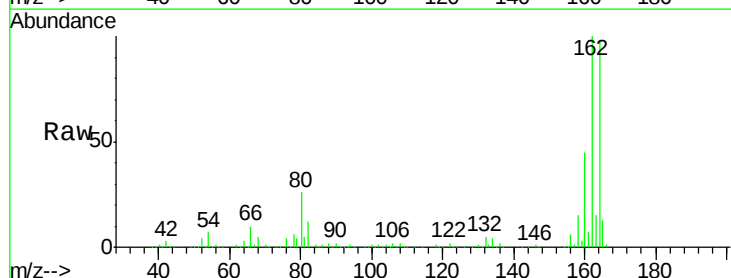


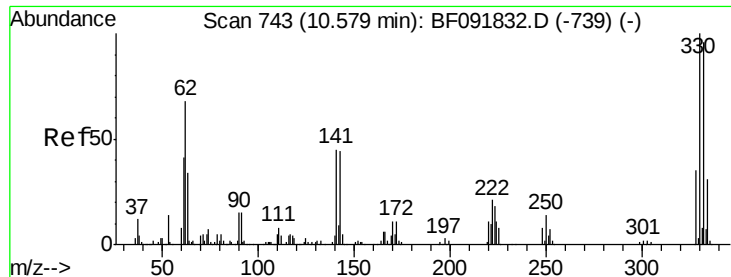




#41
 2,4,6-Tribromophenol
 Concen: 157.96 ng
 RT: 10.48 min Scan# 752
 Delta R.T. -0.00 min
 Lab File: BF092102.D
 Acq: 5 Jan 2017 21:25

Instrument :
 BNA_F
 ClientSampleId :
 DSN001

Tot Ion:330 Resp: 519470
 Ion Ratio Lower Upper
 330 100
 332 96.1 77.4 116.2
 141 36.4 34.1 51.1

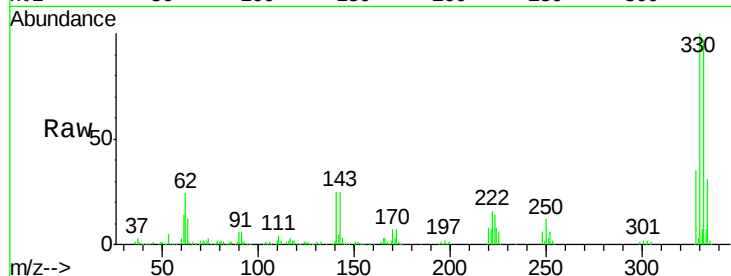


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

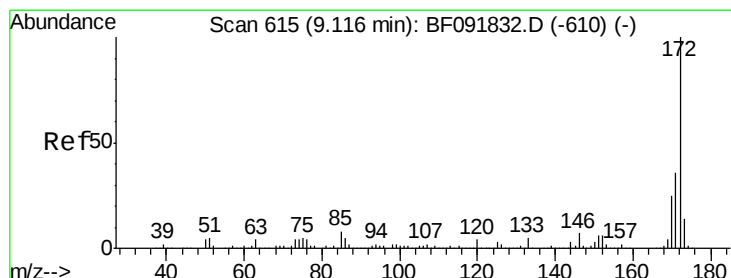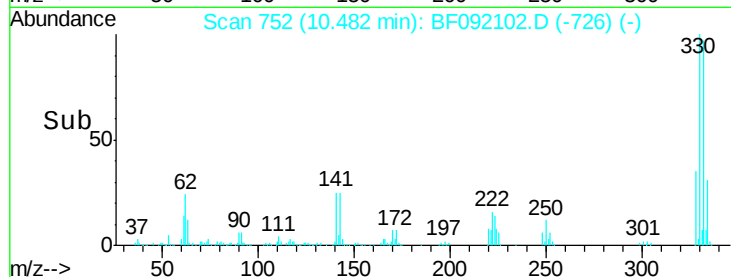
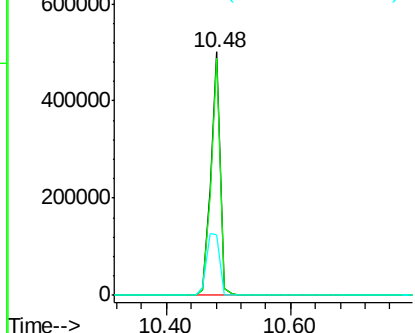



#44
 2-Fluorobiphenyl
 Concen: 106.00 ng
 RT: 9.02 min Scan# 624
 Delta R.T. -0.00 min
 Lab File: BF092102.D
 Acq: 5 Jan 2017 21:25

Tgt Ion:172 Resp: 1993966
 Ion Ratio Lower Upper
 172 100
 171 36.1 29.4 44.0
 170 24.8 20.2 30.4

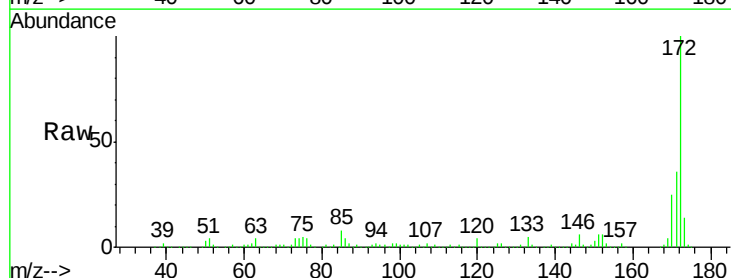

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

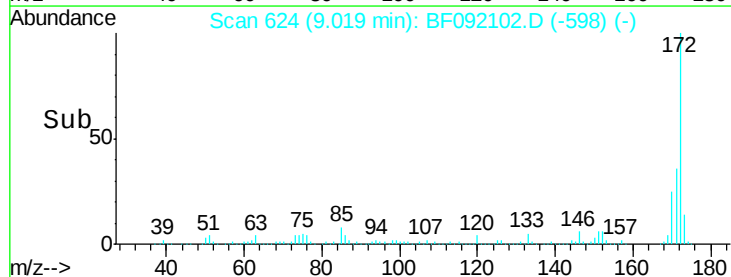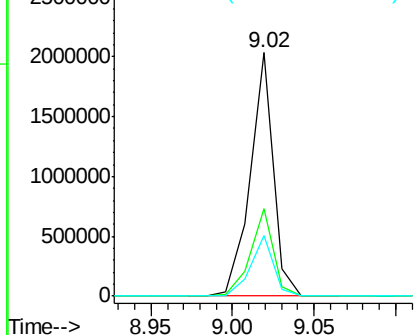


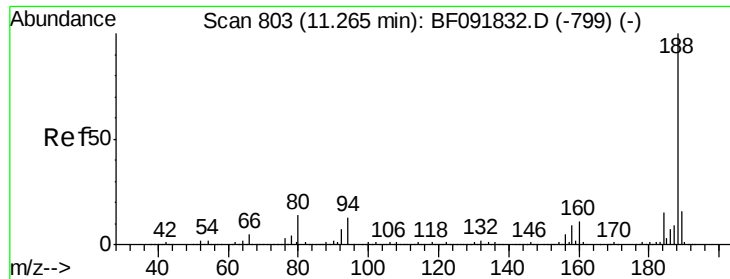




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.17 min Scan# 812
Delta R.T. -0.00 min
Lab File: BF092102.D
Acq: 5 Jan 2017 21:25

Instrument :
BNA_F
ClientSampleId :
DSN001

Tot Ion:188 Resp: 706043
Ion Ratio Lower Upper
188 100
94 7.3 10.0 15.0#
80 7.7 11.2 16.8#

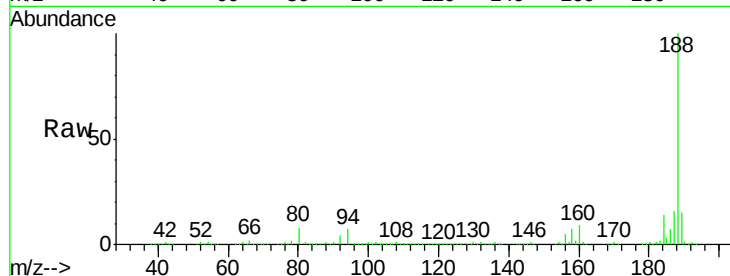


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

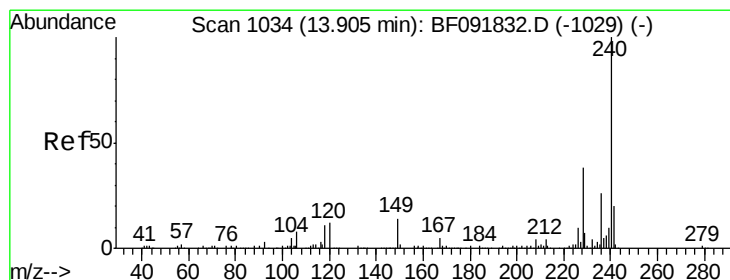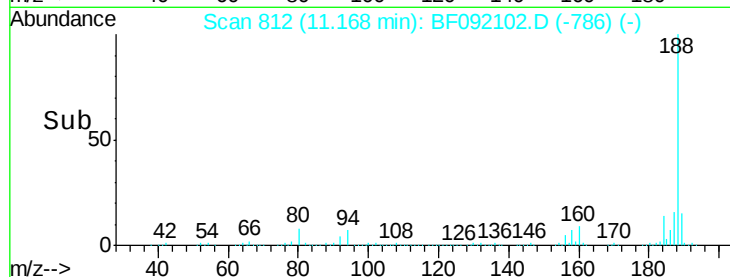
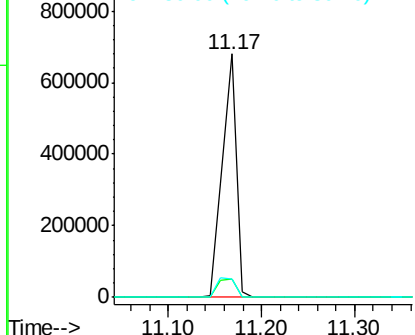



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.80 min Scan# 1042
Delta R.T. -0.00 min
Lab File: BF092102.D
Acq: 5 Jan 2017 21:25

Tgt Ion:240 Resp: 562618
Ion Ratio Lower Upper
240 100
120 9.3 12.9 19.3#
236 25.4 20.9 31.3

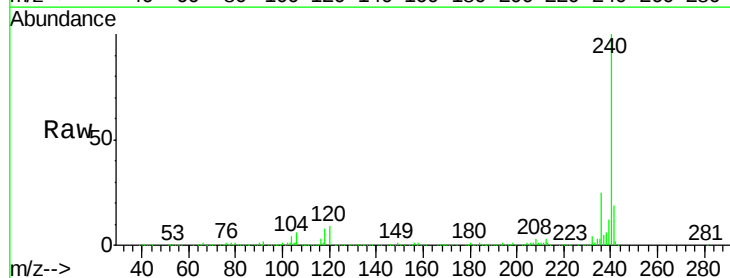

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

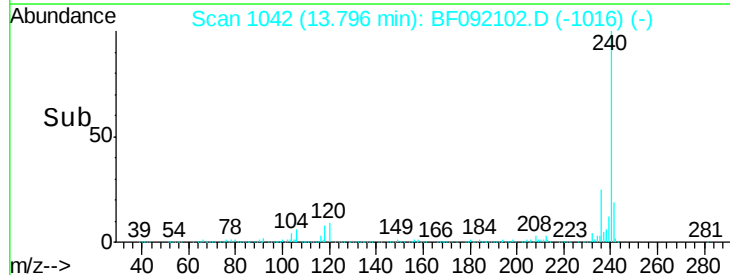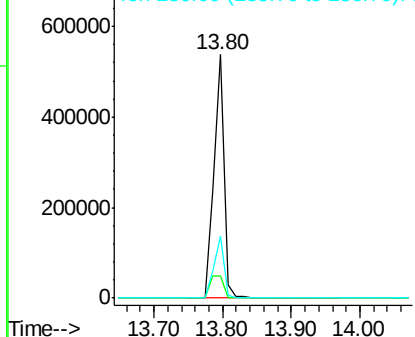




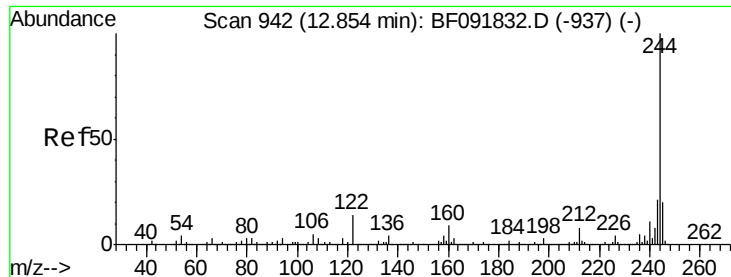


#78
 Terphenyl-d14
 Concen: 82.69 ng
 RT: 12.76 min Scan# 951
 Delta R.T. -0.00 min
 Lab File: BF092102.D
 Acq: 5 Jan 2017 21:25

Instrument :
 BNA_F
 ClientSampleId :
 DSN001

Tot Ion:244 Resp: 1918160

Ion	Ratio	Lower	Upper
244	100		
212	7.4	6.2	9.2
122	12.7	11.4	17.2

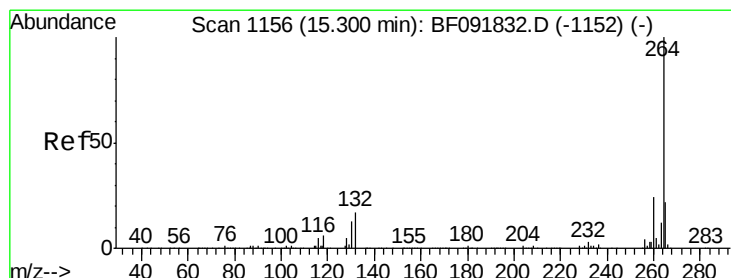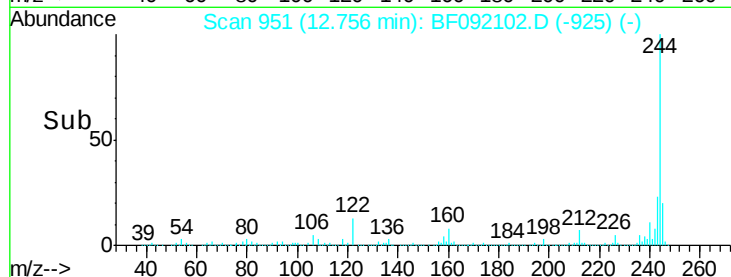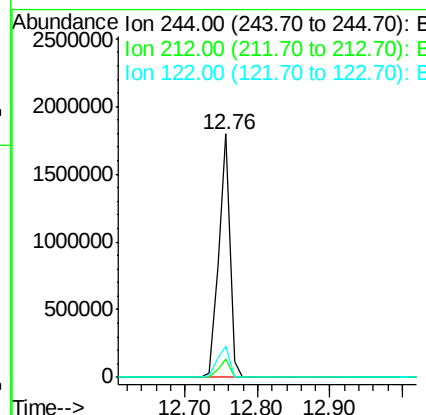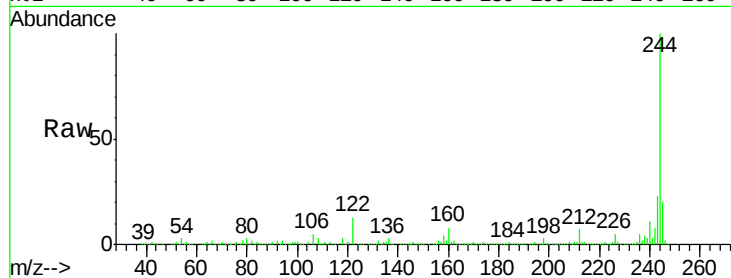

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.17 min Scan# 1162
 Delta R.T. -0.00 min
 Lab File: BF092102.D
 Acq: 5 Jan 2017 21:25

Tgt Ion:264 Resp: 390064

Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.2	28.8
265	21.9	17.4	26.0

