


Data Path : Z:\HPCHEM1\BNA F\Data\BF010517\
 Data File : BF092096.D
 Acq On : 5 Jan 2017 17:42
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 28 17:32:10 2016

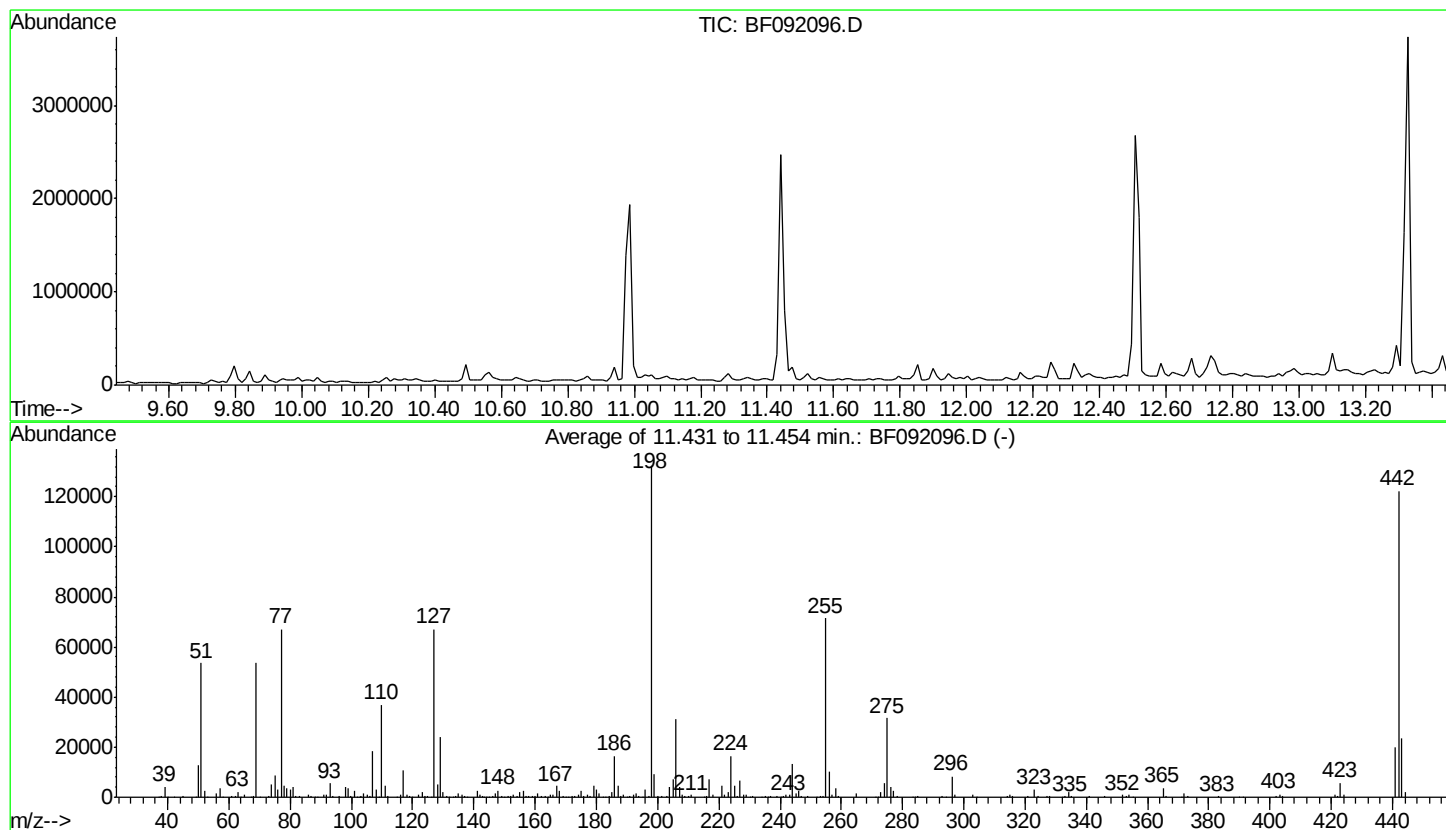

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	53534	PASS
68	69	0.00	2	0.8	442	PASS
69	198	0.00	100	40.4	53478	PASS
70	69	0.00	2	0.3	171	PASS
127	198	10	80	50.6	66973	PASS
197	198	0.00	2	0.6	759	PASS
198	198	100	100	100.0	132426	PASS
199	198	5	9	6.9	9100	PASS
275	198	10	60	23.8	31540	PASS
365	198	1	100	2.9	3789	PASS
441	442	0.01	24	16.2	19764	PASS
442	198	50	100	92.4	122314	PASS
443	442	15	24	19.1	23330	PASS