
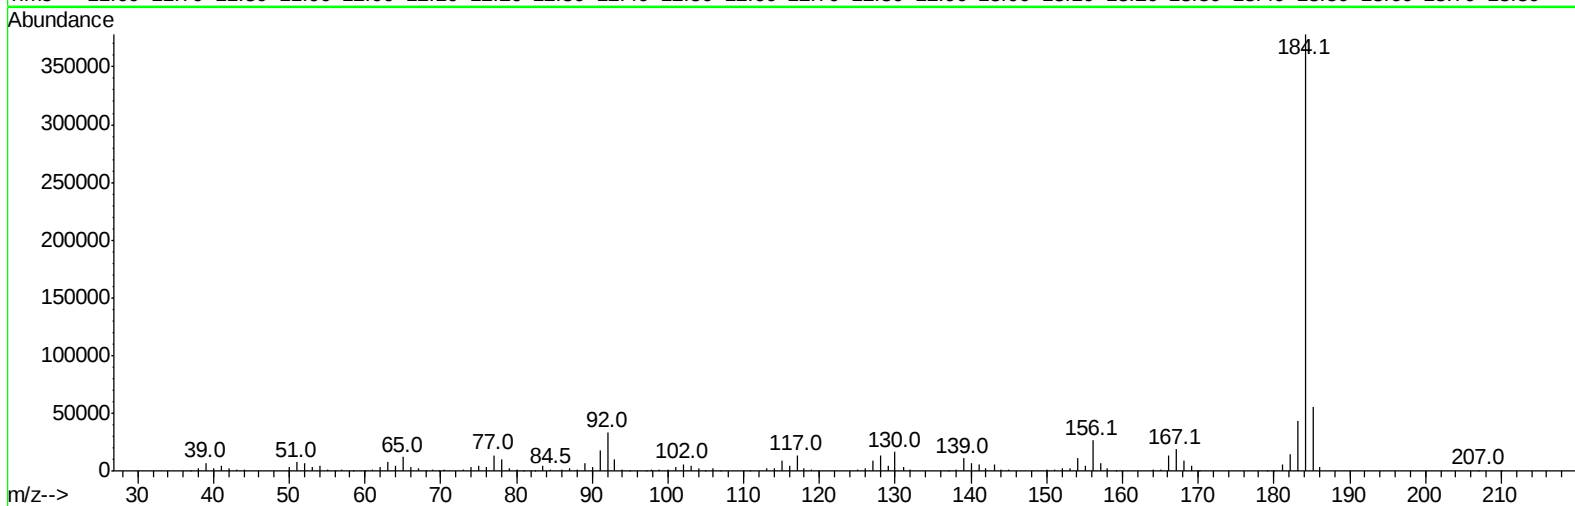


Data Path : U:\HPCHEM1\BNA F\DATA\BF010518\
Data File : BF101916.D
Acq On : 5 Jan 2018 9:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 22:54:01 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 05 12:29:26 2018
Response via : Initial Calibration

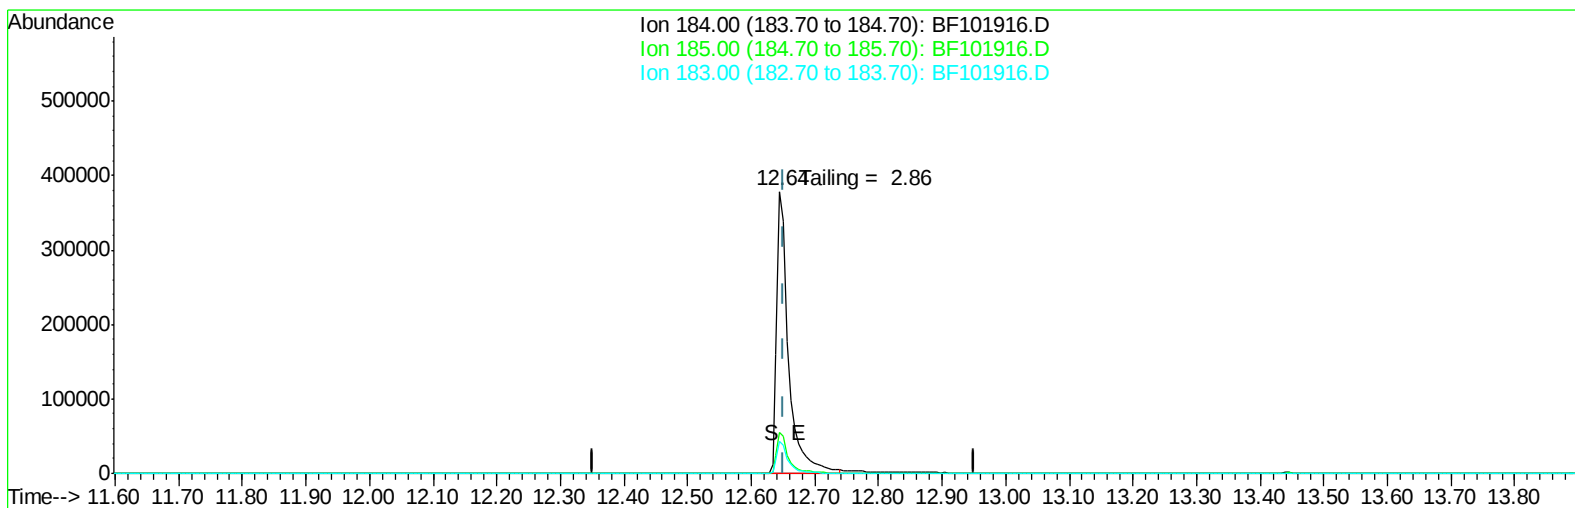

TIC: BF101916.D

(76) Benzidine



12.645min (-0.006) 18707.38ng

response 512781

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.68
183.00	11.60	11.54
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF010518\
Data File : BF101916.D
Acq On : 5 Jan 2018 9:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 22:54:01 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 05 12:29:26 2018
Response via : Initial Calibration

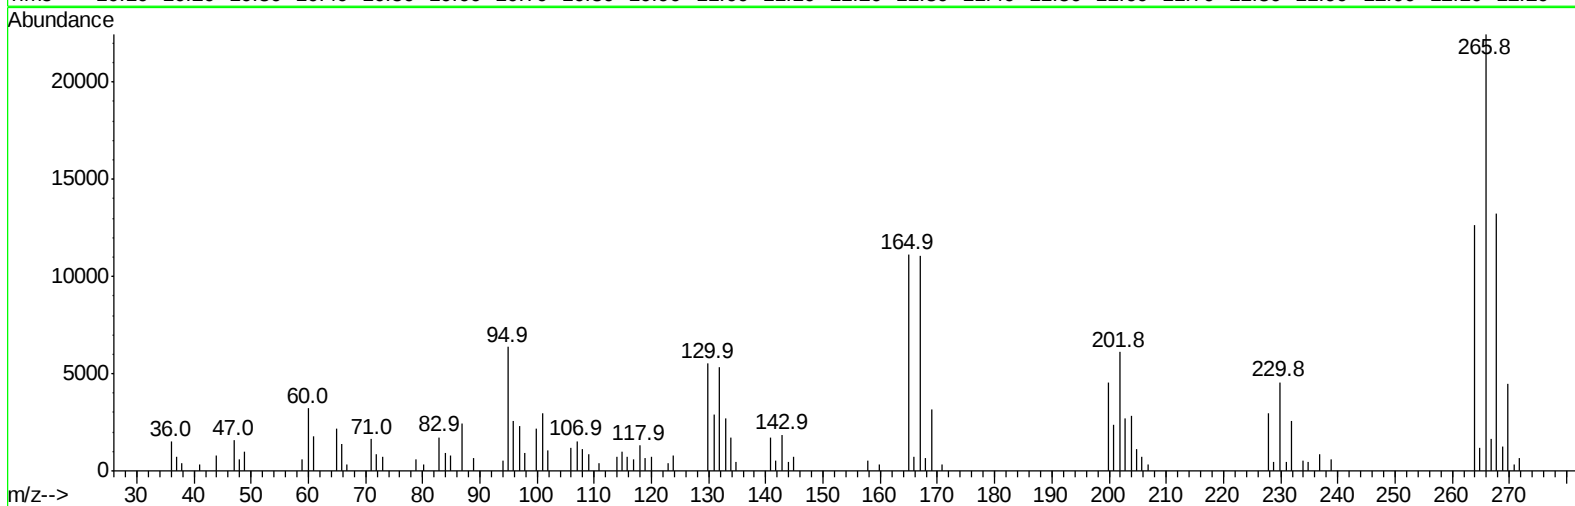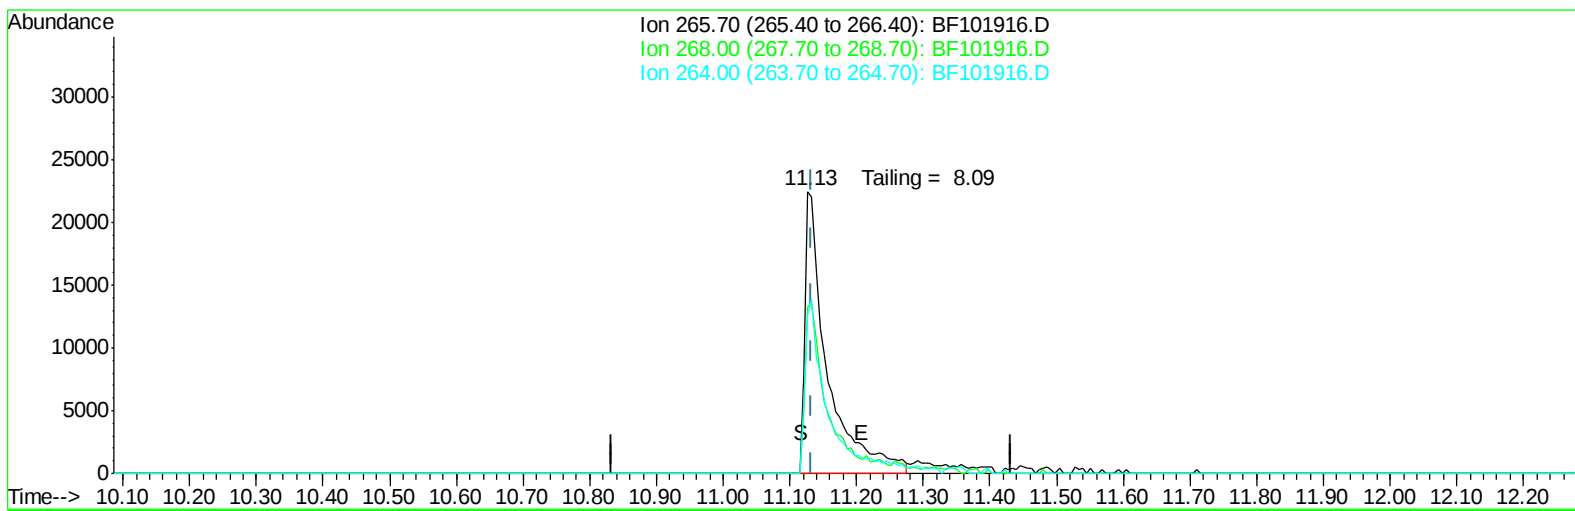

TIC: BF101916.D

(69) Pentachlorophenol (C)

11.127min (-0.006) 37505.84ng

response 51003

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.88
264.00	61.90	56.18
0.00	0.00	0.00