

Data Path : U:\HPCHEM1\BNA F\DATA\BF010518\
 Data File : BF101925.D
 Acq On : 5 Jan 2018 13:13
 Operator : SJ/JU
 Sample : J1004-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-15-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.810	288	293	299	rBV	18732	41790	1.16%	0.136%
2	5.004	492	496	510	rBV	123515	259513	7.22%	0.846%
3	5.398	560	563	597	rBV	2099256	3596436	100.00%	11.722%
4	6.422	734	737	755	rBV	2169340	3551241	98.74%	11.574%
5	6.545	755	758	764	rVV	2723265	3279035	91.17%	10.687%
6	6.587	764	765	782	rVB	75229	105161	2.92%	0.343%
7	6.769	793	796	804	rBV	807706	880899	24.49%	2.871%
8	6.834	804	807	811	rVV	127265	126455	3.52%	0.412%
9	6.928	819	823	840	rBV	2238123	2469990	68.68%	8.050%
10	7.345	890	894	916	rBV	1825323	2325696	64.67%	7.580%
11	8.016	1005	1008	1011	rBV	51085	51639	1.44%	0.168%
12	8.057	1011	1015	1035	rVB	932644	1203568	33.47%	3.923%
13	8.622	1106	1111	1123	rBV2	76841	118723	3.30%	0.387%
14	9.122	1193	1196	1205	rBV	2640940	2687756	74.73%	8.760%
15	9.192	1205	1208	1212	rVB	56099	53892	1.50%	0.176%
16	9.527	1262	1265	1270	rVB	201592	188048	5.23%	0.613%
17	9.722	1294	1298	1302	rVB	61155	58087	1.62%	0.189%
18	9.810	1309	1313	1324	rVB	1112241	1097215	30.51%	3.576%
19	10.216	1379	1382	1385	rBV2	58039	49212	1.37%	0.160%
20	10.522	1432	1434	1439	rBV	124376	118058	3.28%	0.385%
21	10.610	1445	1449	1460	rBV	1340261	1558413	43.33%	5.079%
22	10.692	1460	1463	1472	rVB2	43367	65728	1.83%	0.214%
23	11.304	1563	1567	1570	rBV	1032198	982414	27.32%	3.202%
24	11.327	1570	1571	1577	rVV	203228	170348	4.74%	0.555%
25	11.392	1579	1582	1589	rVB	41141	58256	1.62%	0.190%
26	11.810	1650	1653	1657	rBV	303935	339464	9.44%	1.106%
27	11.921	1669	1672	1675	rBV	39985	41880	1.16%	0.136%
28	12.133	1705	1708	1712	rVB3	40581	41500	1.15%	0.135%
29	12.357	1743	1746	1751	rBV2	74801	95969	2.67%	0.313%
30	12.527	1771	1775	1781	rBV	302327	328935	9.15%	1.072%
31	12.598	1784	1787	1796	rBV	240942	310020	8.62%	1.010%
32	12.680	1798	1801	1807	rVB4	48333	59472	1.65%	0.194%
33	12.733	1807	1810	1812	rBV2	89198	102743	2.86%	0.335%
34	12.757	1812	1814	1819	rVB	255831	235846	6.56%	0.769%

Data Path : U:\HPCHEM1\BNA_F\DATA\BF010518\
Data File : BF101925.D
Acq On : 5 Jan 2018 13:13
Operator : SJ/JU
Sample : J1004-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-15-COMP

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.880	1831	1835	1839	rBV	1941926	1774751	49.35%	5.784%
36	13.015	1856	1858	1861	rBV2	44775	51078	1.42%	0.166%
37	13.068	1864	1867	1868	rVV3	86029	79290	2.20%	0.258%
38	13.086	1868	1870	1875	rVB	110663	111069	3.09%	0.362%
39	13.427	1926	1928	1930	rBV	70060	52911	1.47%	0.172%
40	13.757	1981	1984	1991	rVB2	241633	275533	7.66%	0.898%
41	13.957	2014	2018	2021	rBV2	793249	909040	25.28%	2.963%
42	15.004	2193	2196	2204	rBV2	129862	240177	6.68%	0.783%
43	15.433	2265	2269	2274	rVB	423175	535005	14.88%	1.744%


Sum of corrected areas: 30682256

Data Path : U:\HPCHEM1\BNA_F\DATA\BF010518\
Data File : BF101925.D
Acq On : 5 Jan 2018 13:13
Operator : SJ/JU
Sample : J1004-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-15-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

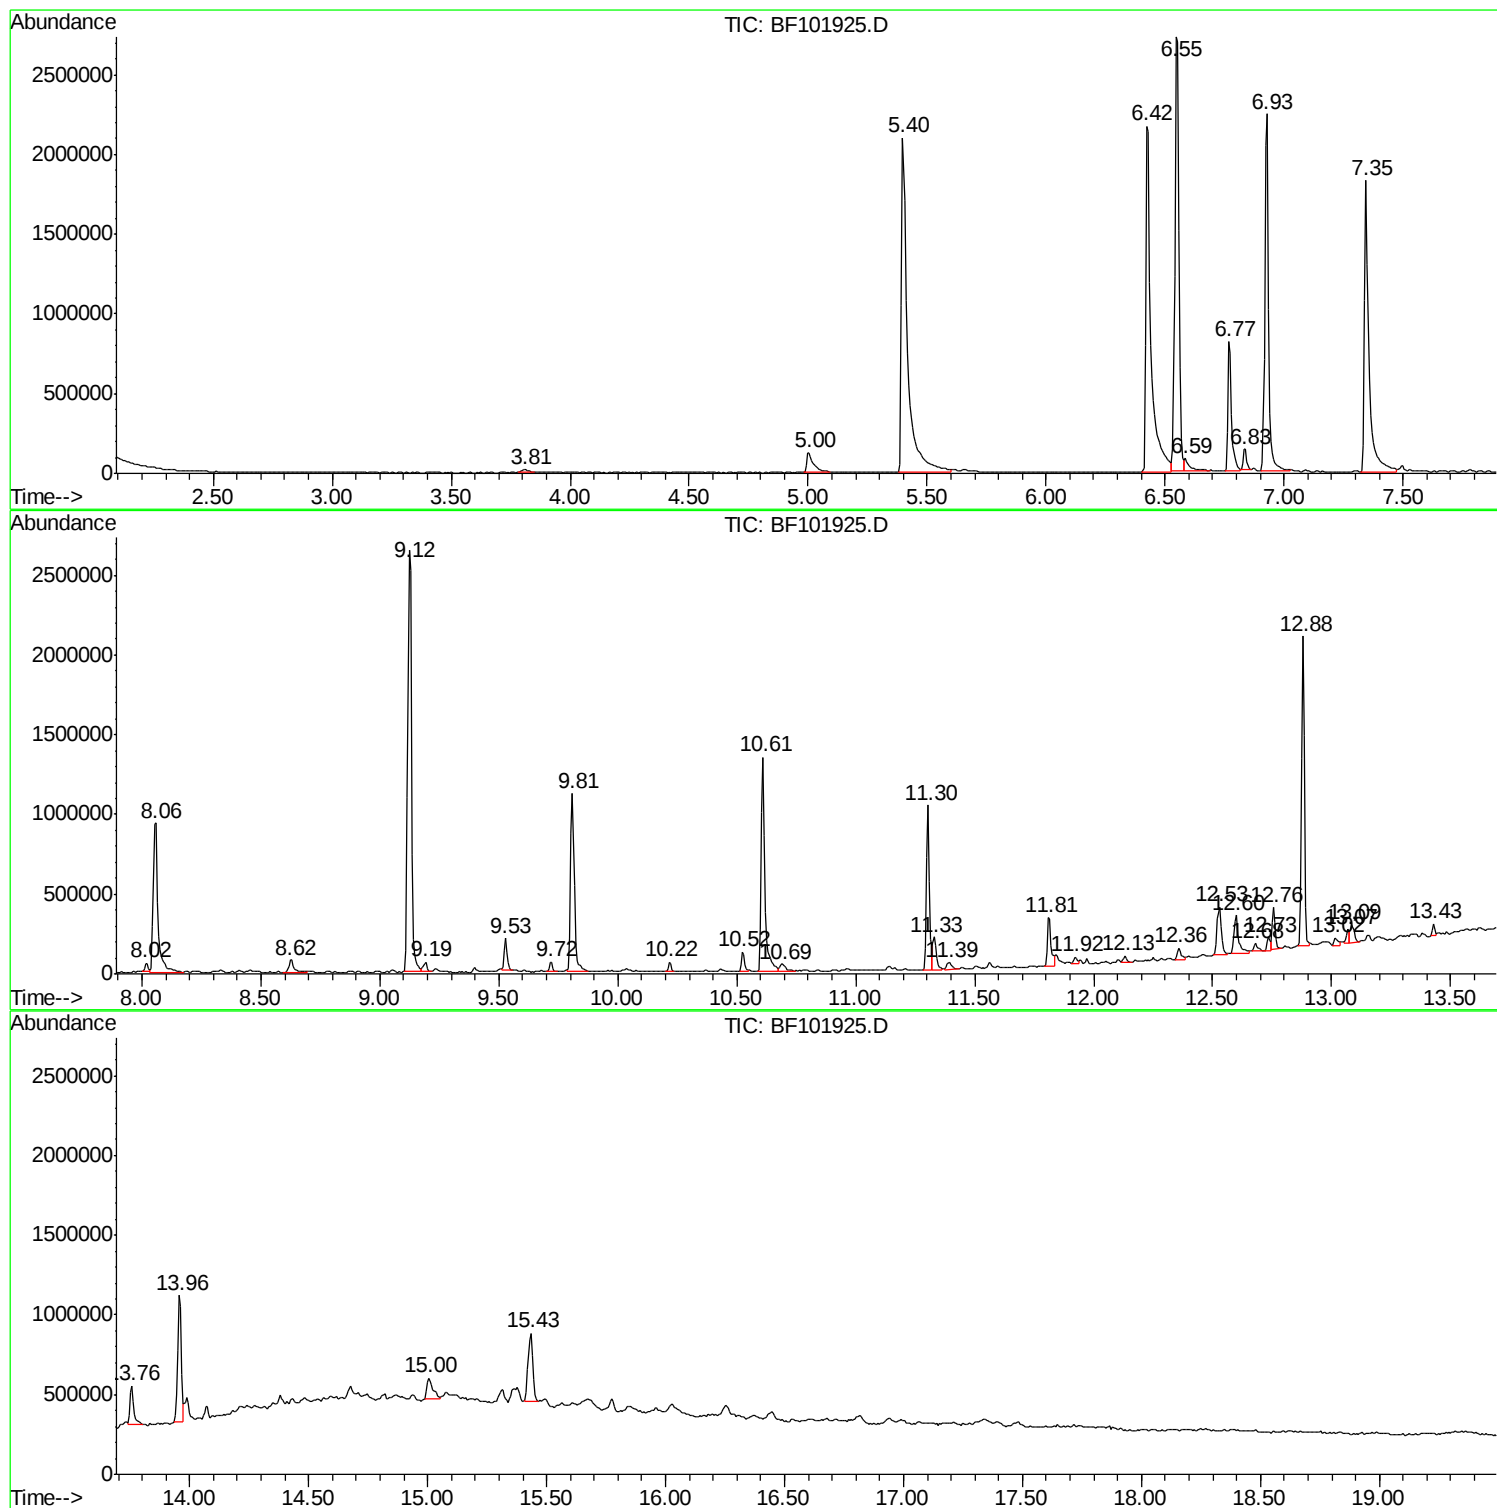

Data_Path : U:\HPCHEM1\BNA_F\DATA\BF010518\
Data_File : BF101925.D
Acq_On : 5-Jan-2018 13:133
Operator : SJ/JUU
Sample : J1004-122
Misc :
ALS_Vial : 10 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SB-15-COMP

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
