
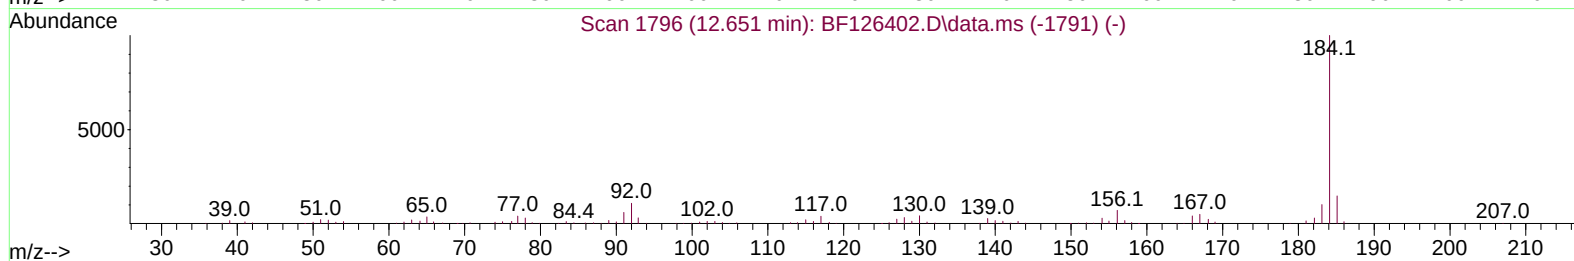
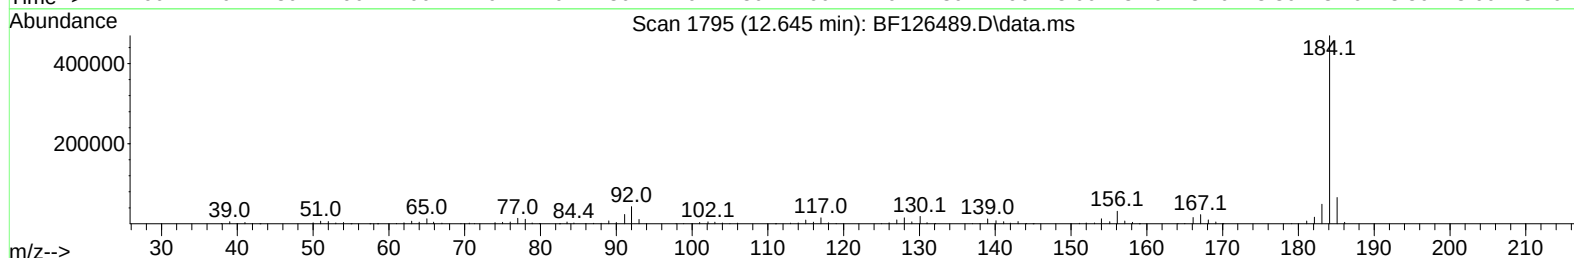


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
Data File : BF126489.D
Acq On : 5 Jan 2022 11:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 02:21:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 01:57:07 2022
Response via : Initial Calibration

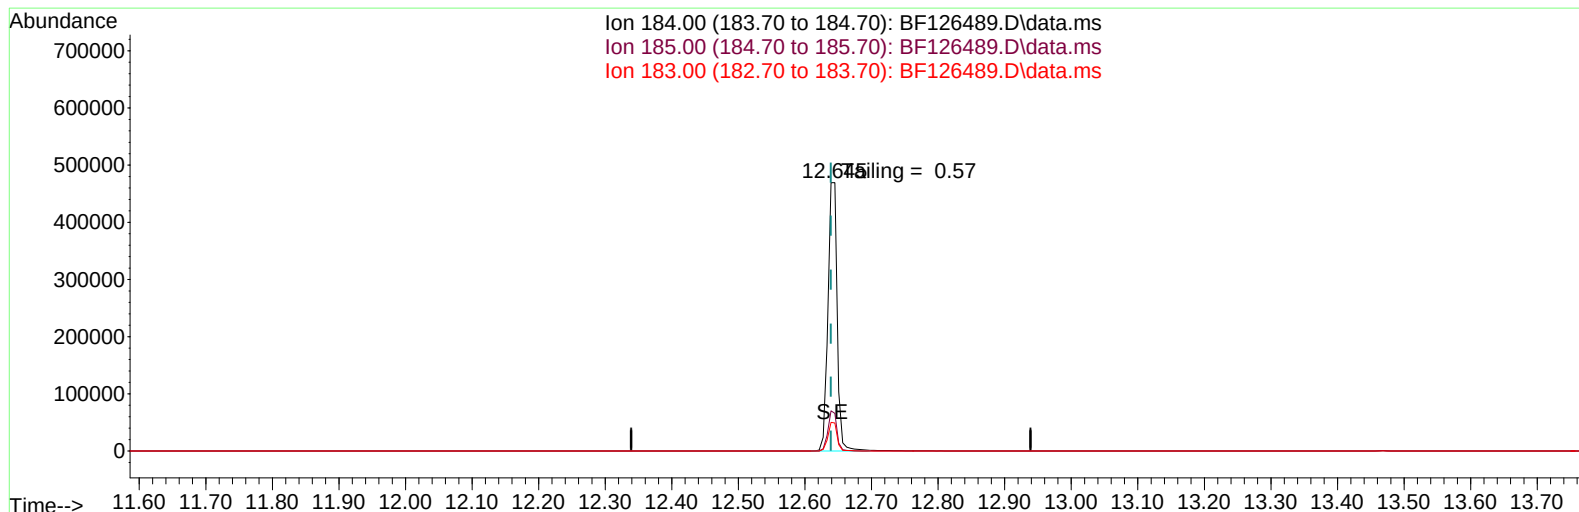

TIC: BF126489.D\data.ms

(77) Benzidine




12.645min (+ 0.006) 0.00 ng

response 458242

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.05
183.00	10.20	10.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
Data File : BF126489.D
Acq On : 5 Jan 2022 11:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 02:21:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 01:57:07 2022
Response via : Initial Calibration

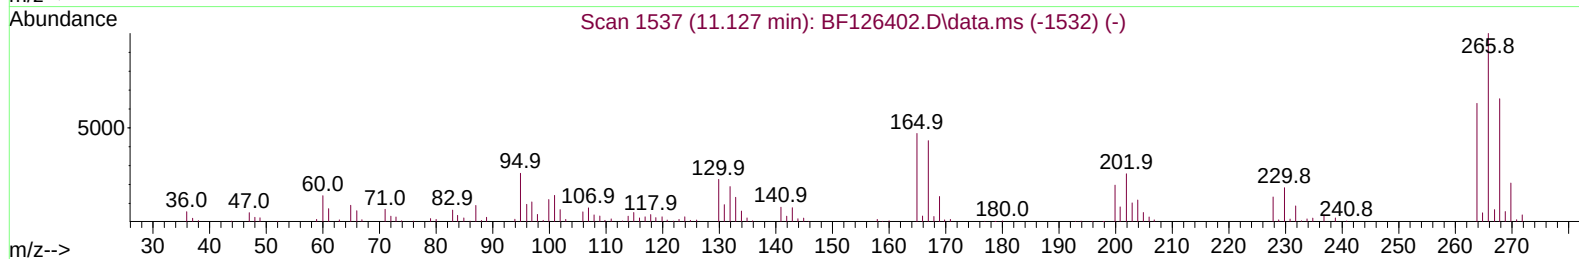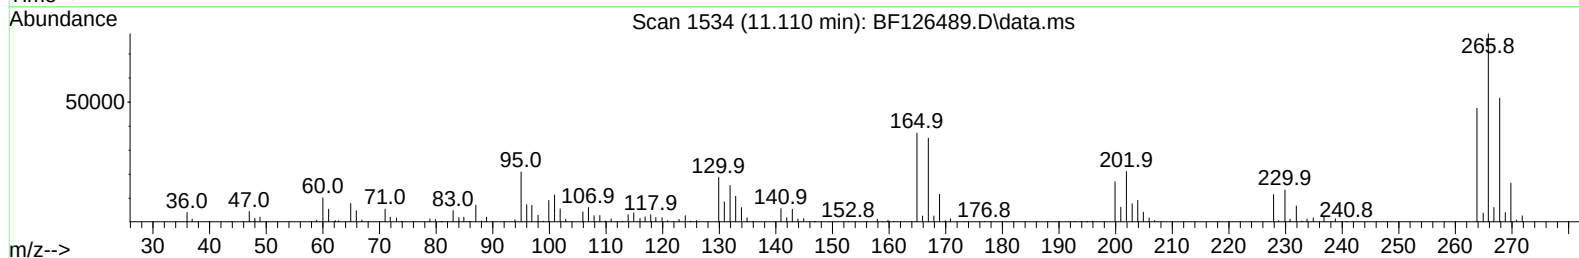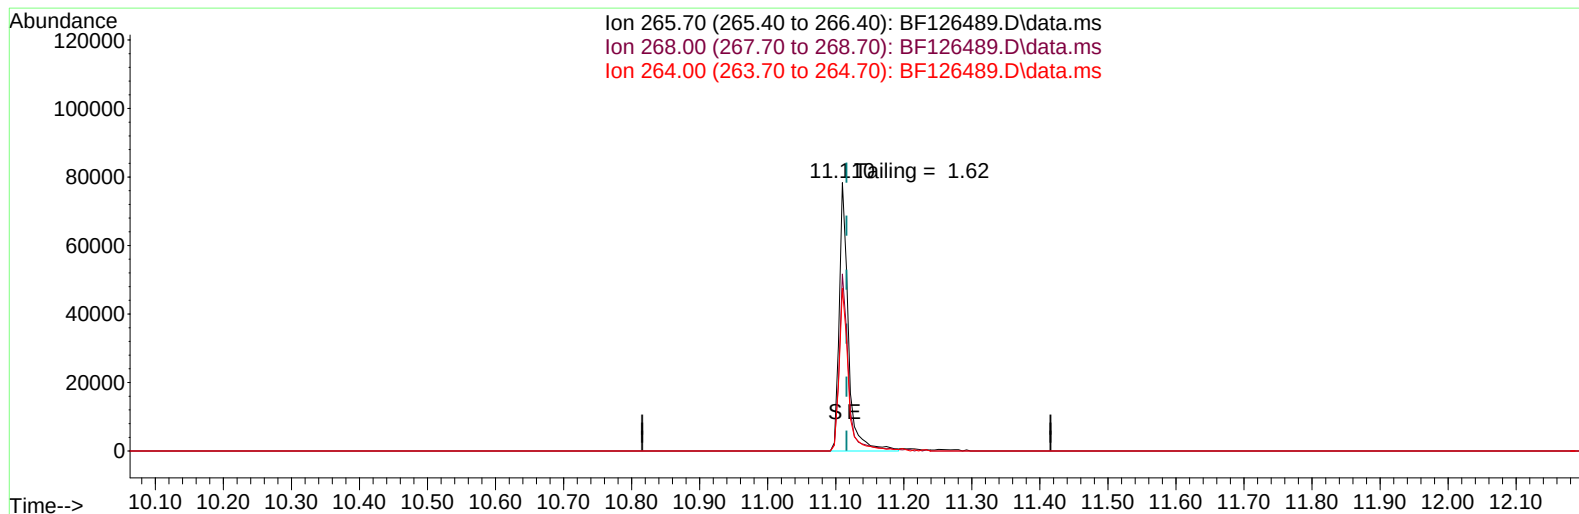

TIC: BF126489.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.006) 85282.01 ng

response 73607

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	65.96
264.00	63.00	60.53
0.00	0.00	0.00