

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
 Data File : BF126493.D
 Acq On : 5 Jan 2022 13:17
 Operator : JU/CG
 Sample : PB141734BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB141734BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126493.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	494	498	507	rVB	30293	40439	1.20%	0.191%
2	5.404	559	564	567	rBV	3195891	3293790	98.14%	15.586%
3	6.416	730	736	739	rBV	2851745	3356310	100.00%	15.882%
4	6.781	794	798	802	rBB	889091	698304	20.81%	3.304%
5	7.345	888	894	897	rBV	2141892	2233945	66.56%	10.571%
6	8.063	1011	1016	1020	rBV	1091112	978708	29.16%	4.631%
7	9.145	1194	1200	1203	rBV	3457994	3264989	97.28%	15.450%
8	9.822	1310	1315	1318	rBV	1103973	1007753	30.03%	4.769%
9	10.610	1444	1449	1452	rBV	1984800	1805272	53.79%	8.542%
10	11.304	1563	1567	1571	rBV	1072880	896173	26.70%	4.241%
11	12.892	1833	1837	1841	rBV	2261708	2364784	70.46%	11.190%
12	13.939	2011	2015	2019	rBV	605398	524292	15.62%	2.481%
13	14.039	2027	2032	2039	rBV	100279	112992	3.37%	0.535%
14	15.380	2255	2260	2264	rBV	437653	518243	15.44%	2.452%
15	16.333	2415	2422	2428	rBV2	22036	37235	1.11%	0.176%




Sum of corrected areas: 21133229

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
Data File : BF126493.D
Acq On : 5 Jan 2022 13:17
Operator : JU/CG
Sample : PB141734BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141734BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

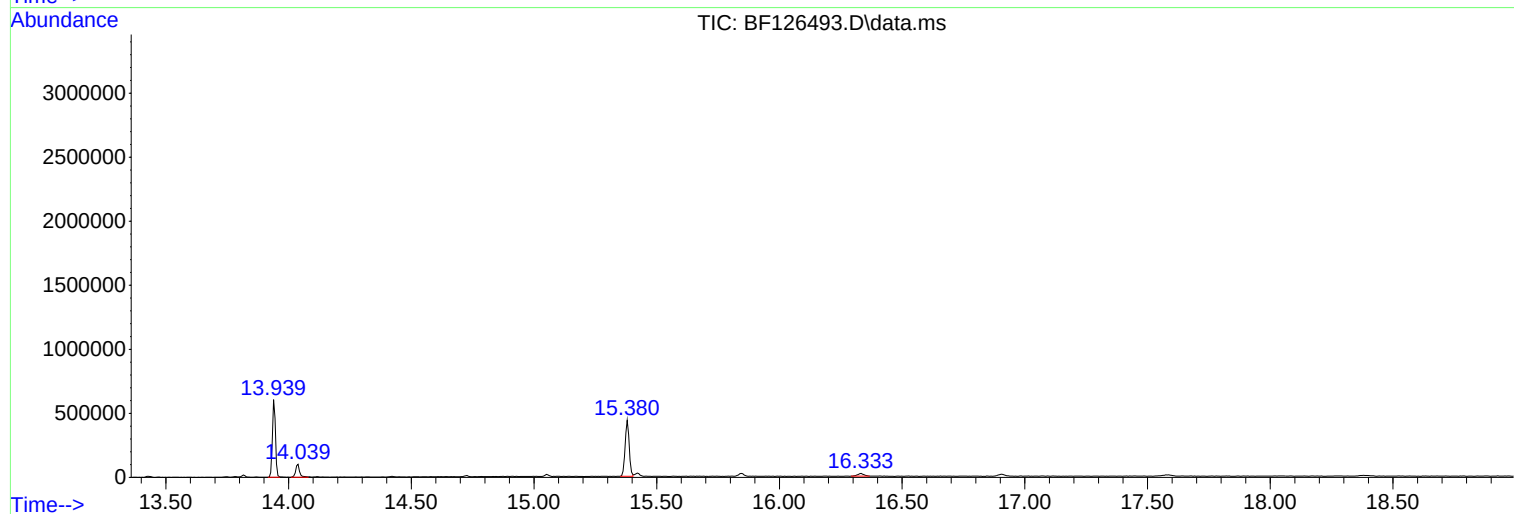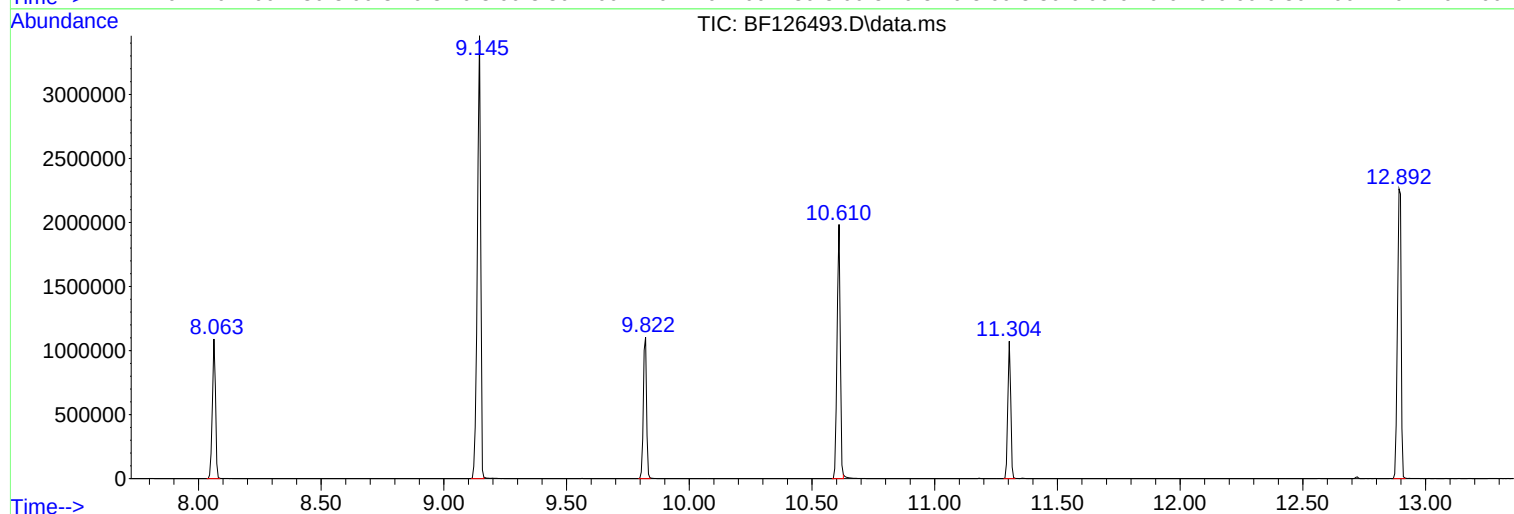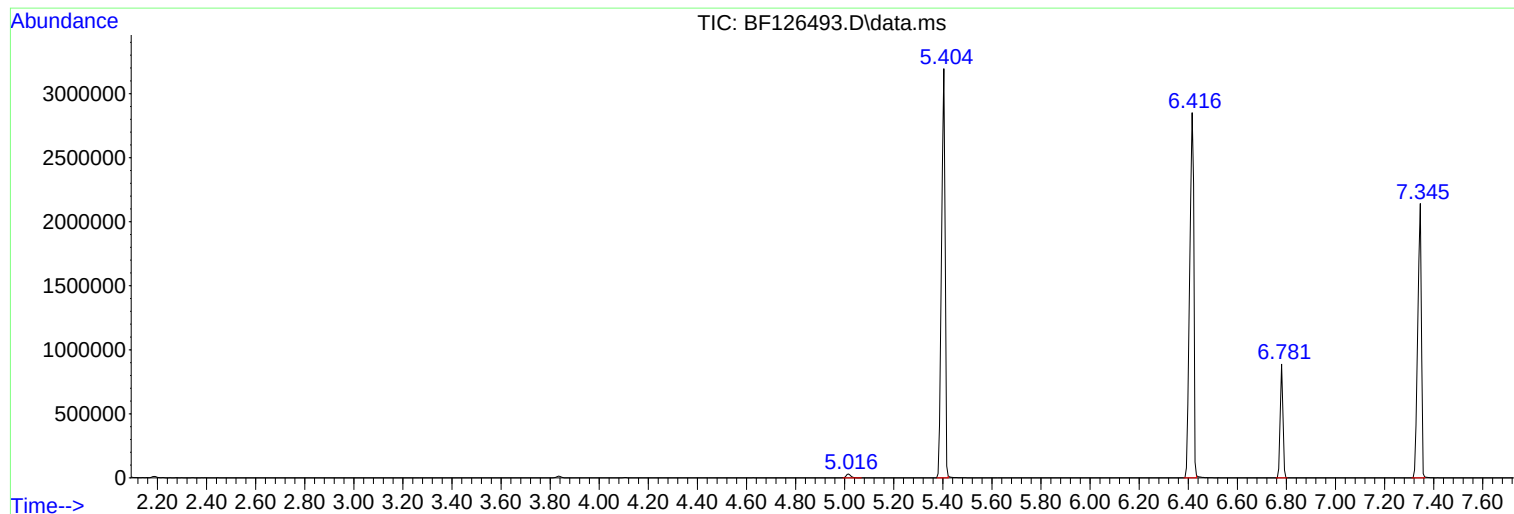

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
Data File : BF126493.D
Acq On : 5 Jan 2022 13:17
Operator : JU/CG
Sample : PB141734BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141734BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.039	4.31 ng	112992	Chrysene-d12	13.939

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	62
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	37
5			1H-Indol-4-ol, 2TMS derivative	277	C14H23NOSi2	1000485-28-1	23

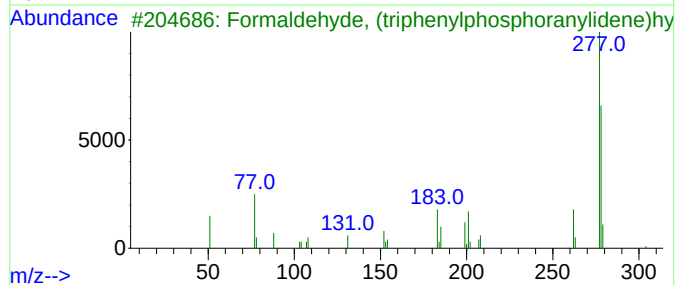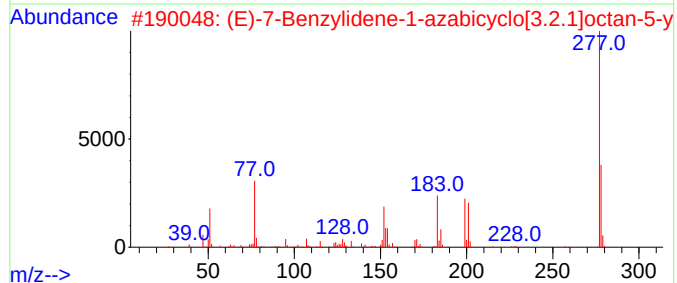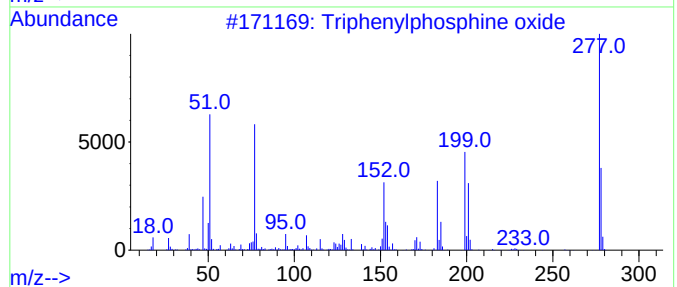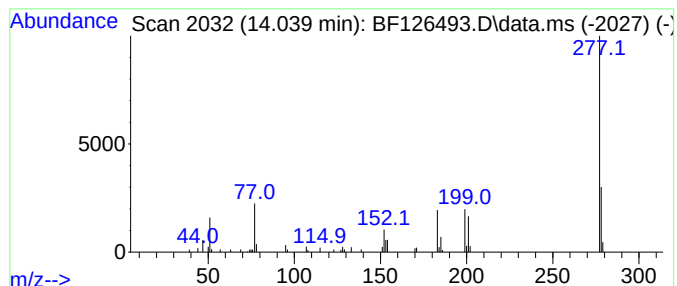

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
Data File : BF126493.D
Acq On : 5 Jan 2022 13:17
Operator : JU/CG
Sample : PB141734BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141734BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.039	4.3	ng	112992	5	13.939	524292	20.0