

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
 Data File : BF126496.D
 Acq On : 5 Jan 2022 14:53
 Operator : JU/CG
 Sample : PB141762BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB141762BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	495	498	507	rVB	31202	39421	1.19%	0.189%
2	5.404	559	564	567	rBV	3010239	3275976	98.73%	15.738%
3	6.416	731	736	739	rBV	2872459	3318081	100.00%	15.940%
4	6.781	794	798	802	rBV	866848	692618	20.87%	3.327%
5	7.345	888	894	897	rBV	2184800	2225889	67.08%	10.693%
6	8.063	1012	1016	1020	rBV	1109825	965321	29.09%	4.637%
7	9.145	1194	1200	1203	rBV	3385588	3250452	97.96%	15.615%
8	9.821	1310	1315	1318	rBV	1096421	990216	29.84%	4.757%
9	10.610	1444	1449	1452	rBV	1924687	1775627	53.51%	8.530%
10	11.304	1563	1567	1570	rBV	1051269	866790	26.12%	4.164%
11	12.892	1833	1837	1841	rBV	2299998	2211003	66.63%	10.622%
12	13.939	2011	2015	2026	rVB	545309	491471	14.81%	2.361%
13	14.039	2026	2032	2039	rBV	69007	76524	2.31%	0.368%
14	15.380	2254	2260	2264	rBV	434082	514120	15.49%	2.470%
15	15.845	2334	2339	2348	rVB	24551	42641	1.29%	0.205%
16	16.327	2416	2421	2430	rVB3	23698	46073	1.39%	0.221%
17	17.580	2626	2634	2642	rBV4	12097	33489	1.01%	0.161%




Sum of corrected areas: 20815712

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
Data File : BF126496.D
Acq On : 5 Jan 2022 14:53
Operator : JU/CG
Sample : PB141762BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141762BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

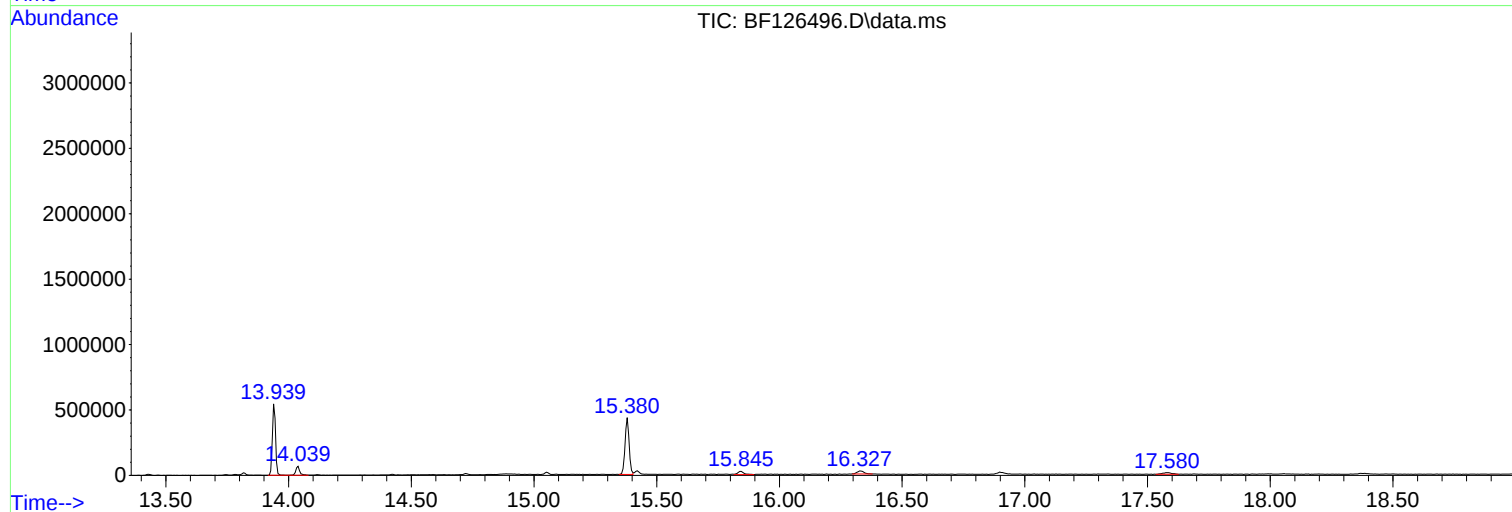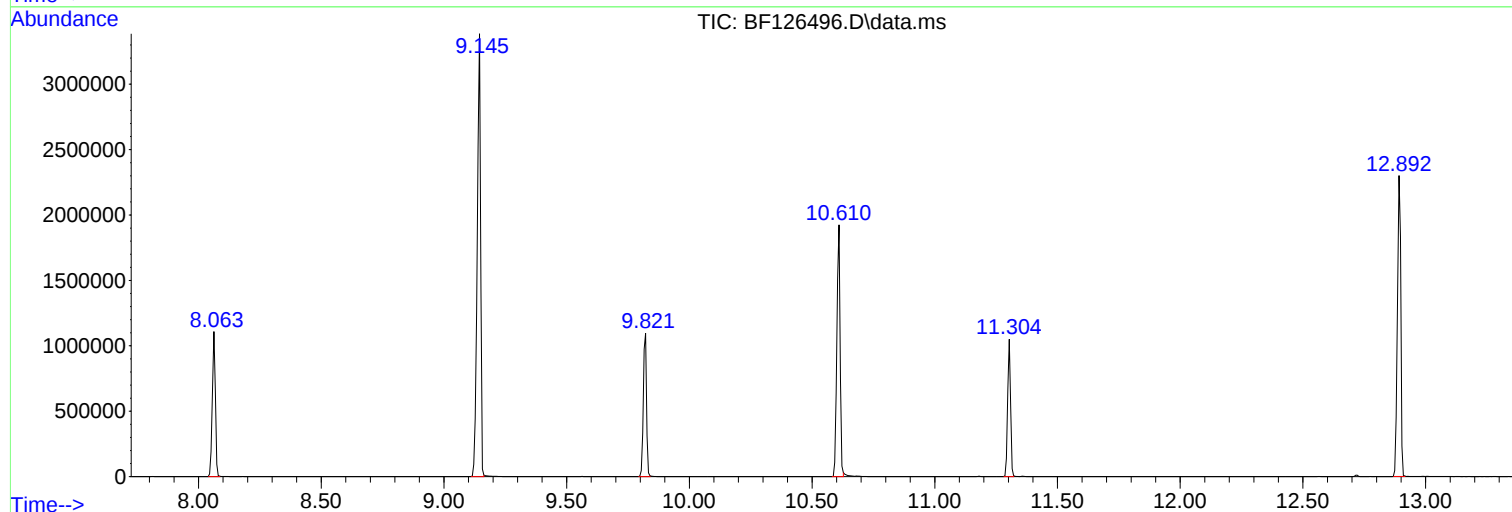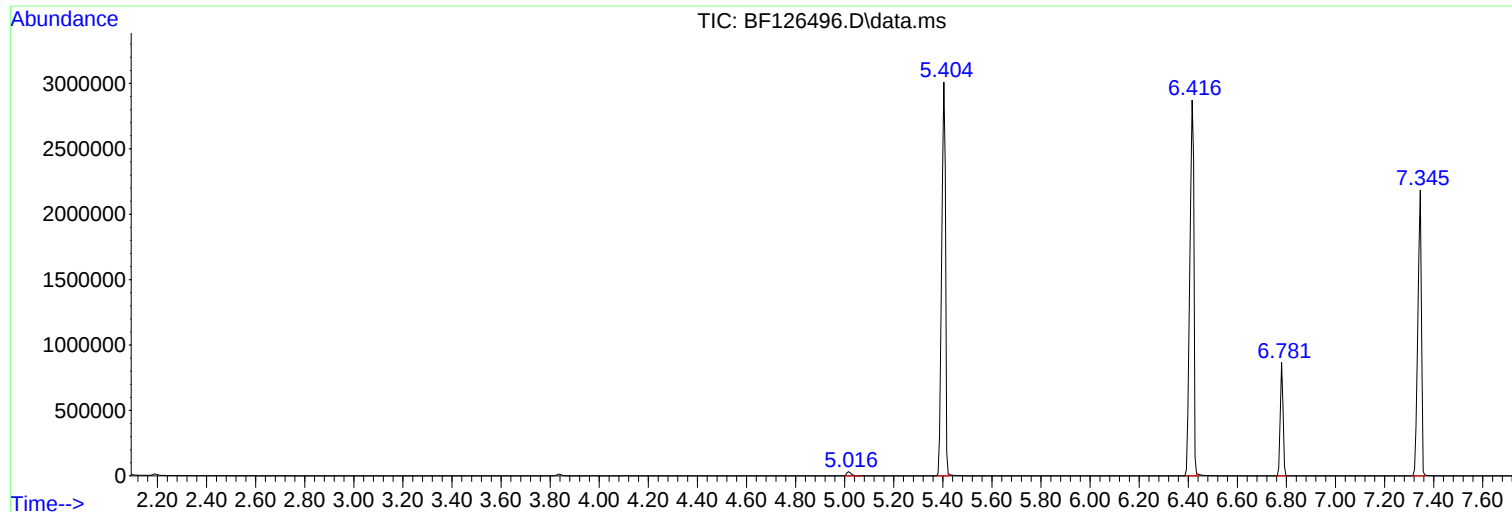

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
Data File : BF126496.D
Acq On : 5 Jan 2022 14:53
Operator : JU/CG
Sample : PB141762BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141762BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.039	3.11 ng	76524	Chrysene-d12	13.939

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	83
2			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
3			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19N03S	1000483-83-4	52
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	38
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15N02	299962-12-2	38

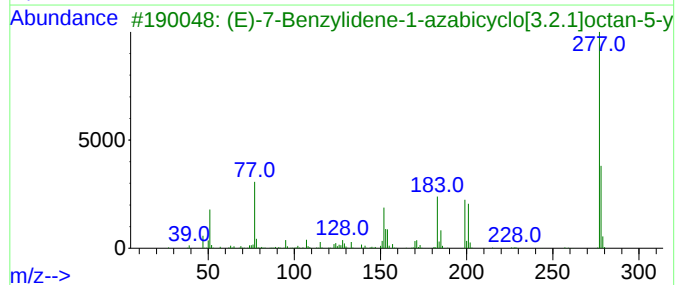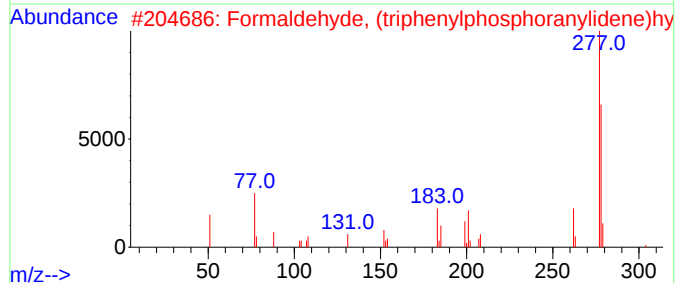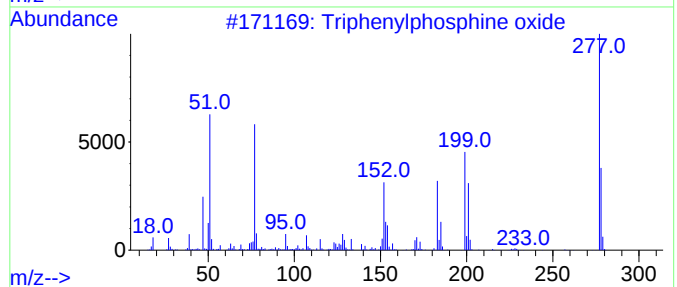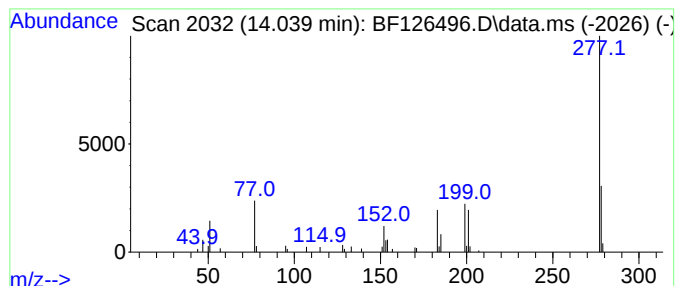

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
Data File : BF126496.D
Acq On : 5 Jan 2022 14:53
Operator : JU/CG
Sample : PB141762BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141762BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.039	3.1	ng	76524	5	13.939	491471	20.0