


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
 Data File : BF126489.D
 Acq On : 5 Jan 2022 11:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 05 01:57:07 2022

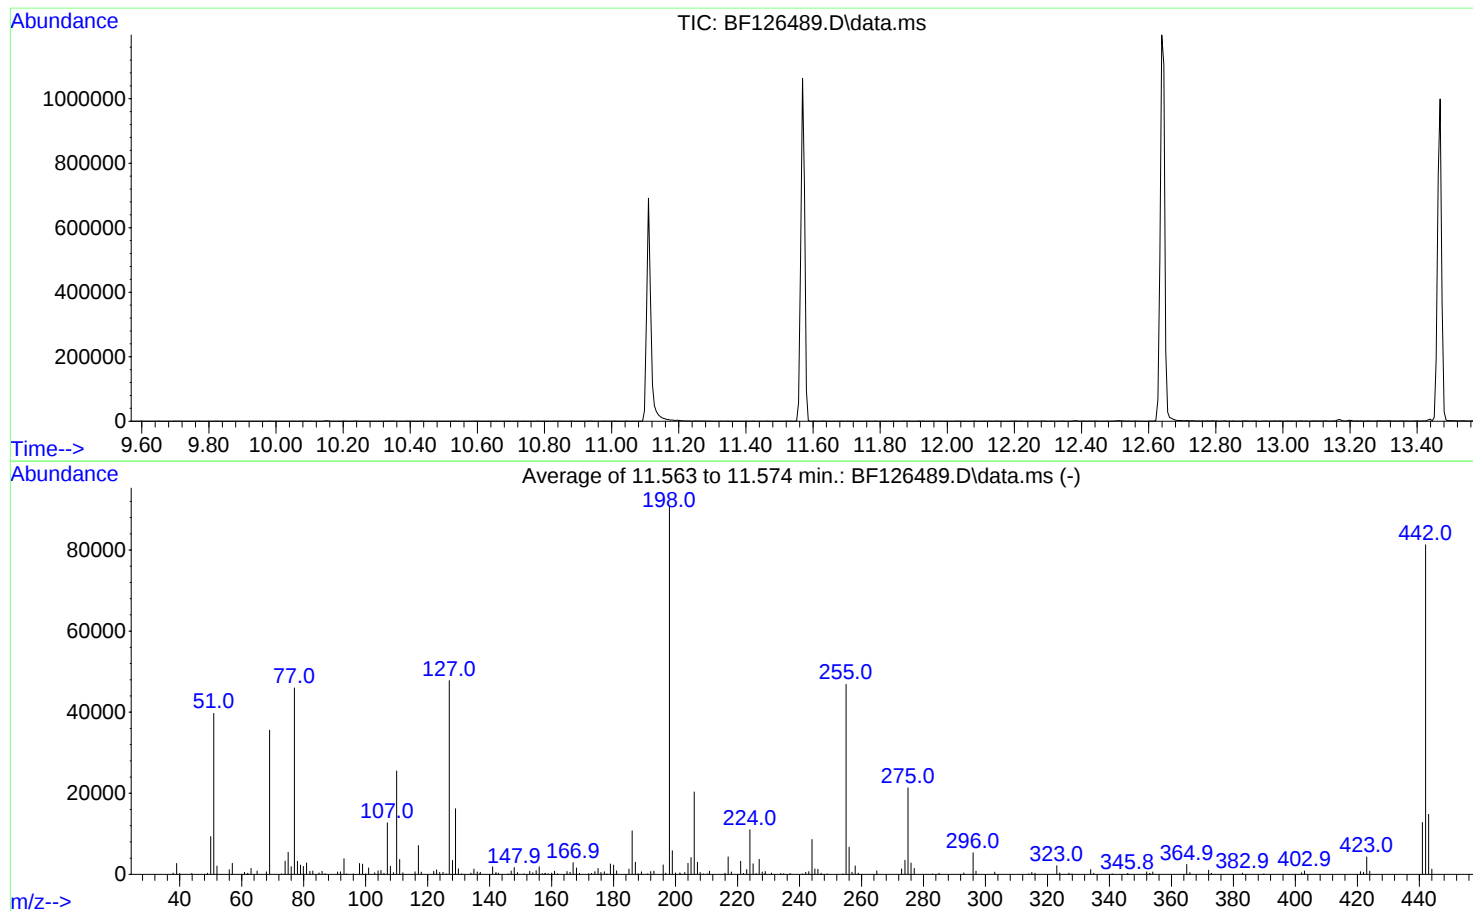




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.8	39717	PASS
68	69	0.00	2	1.8	631	PASS
69	198	0.00	100	39.2	35563	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	47781	PASS
197	198	0.00	2	0.3	309	PASS
198	198	100	100	100.0	90733	PASS
199	198	5	9	6.5	5853	PASS
275	198	10	60	23.5	21338	PASS
365	198	1	100	2.7	2445	PASS
441	198	0.01	100	14.1	12807	PASS
442	442	50	100	100.0	81285	PASS
443	442	15	24	18.2	14812	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
Data File : BF126489.D
Acq On : 5 Jan 2022 11:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 06 02:21:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 01:57:07 2022
Response via : Initial Calibration

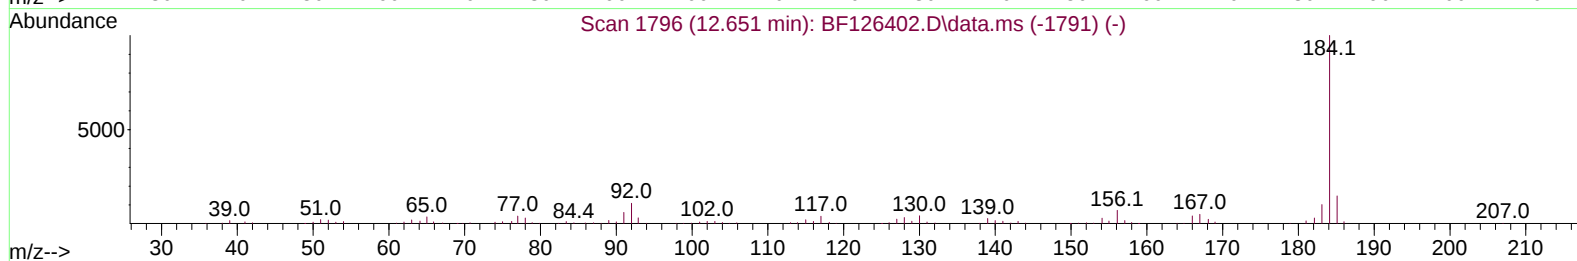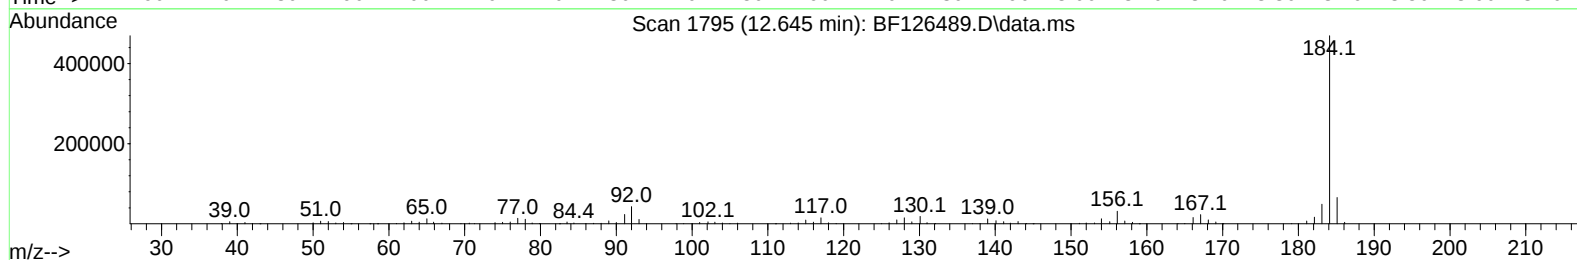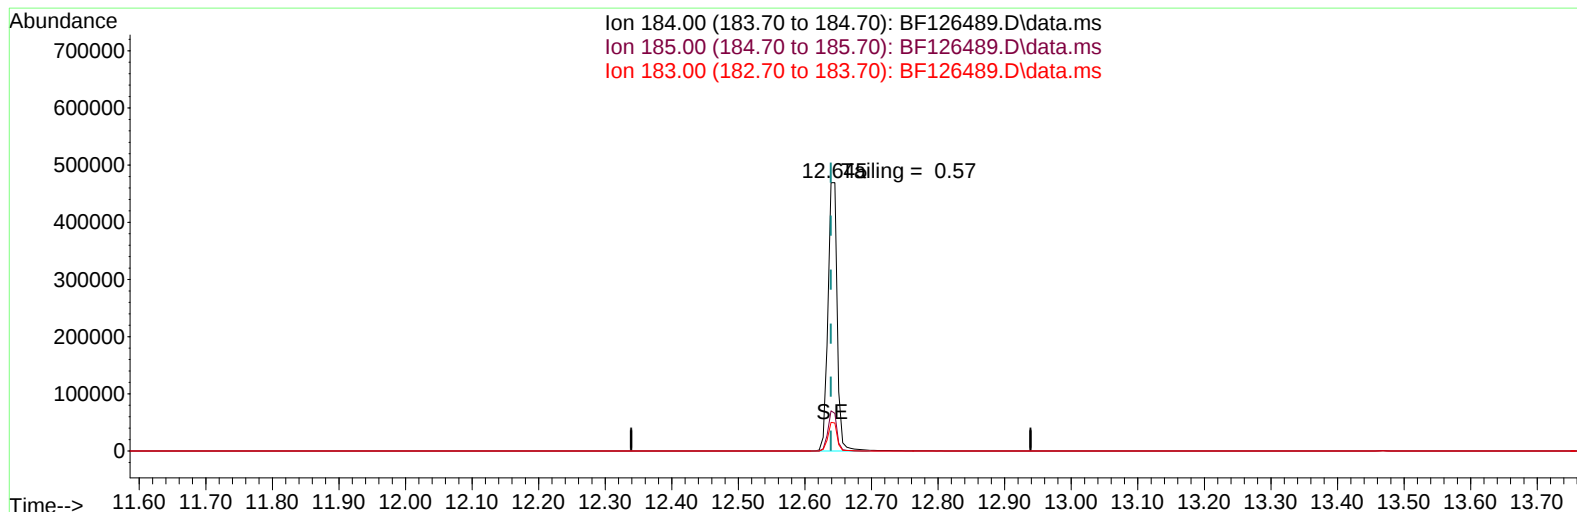

TIC: BF126489.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 0.00 ng




response 458242

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.05
183.00	10.20	10.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010522\
Data File : BF126489.D
Acq On : 5 Jan 2022 11:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 06 02:21:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 01:57:07 2022
Response via : Initial Calibration

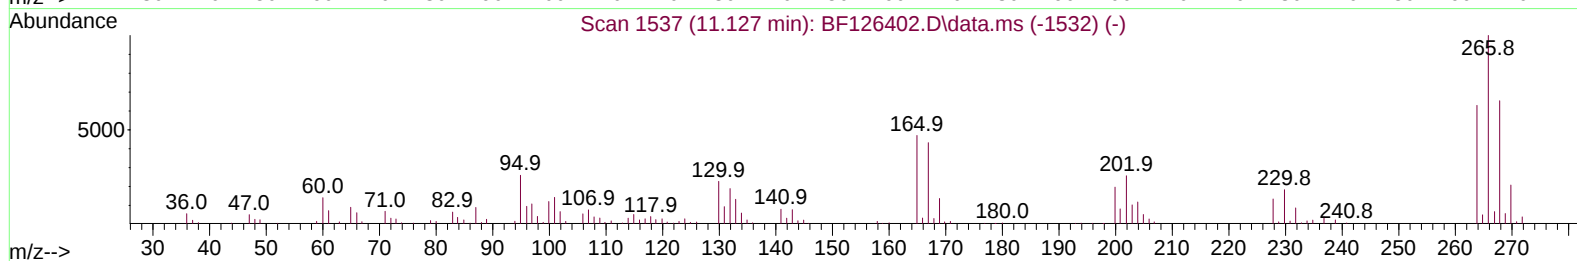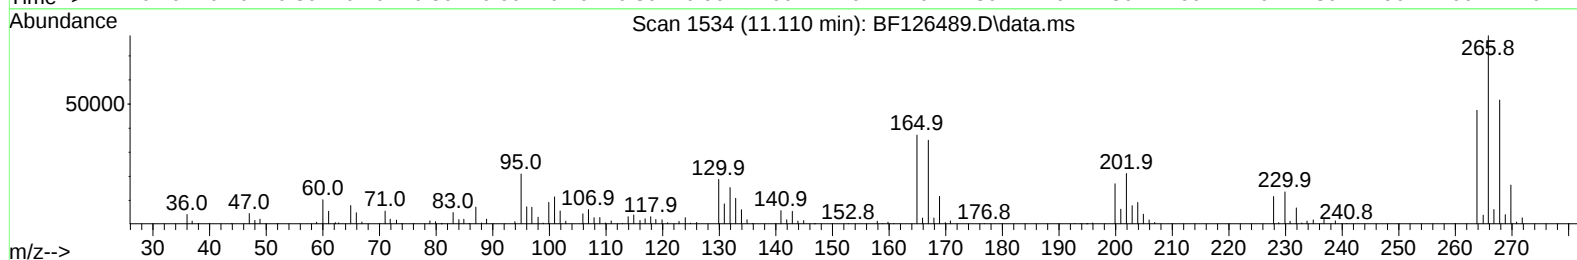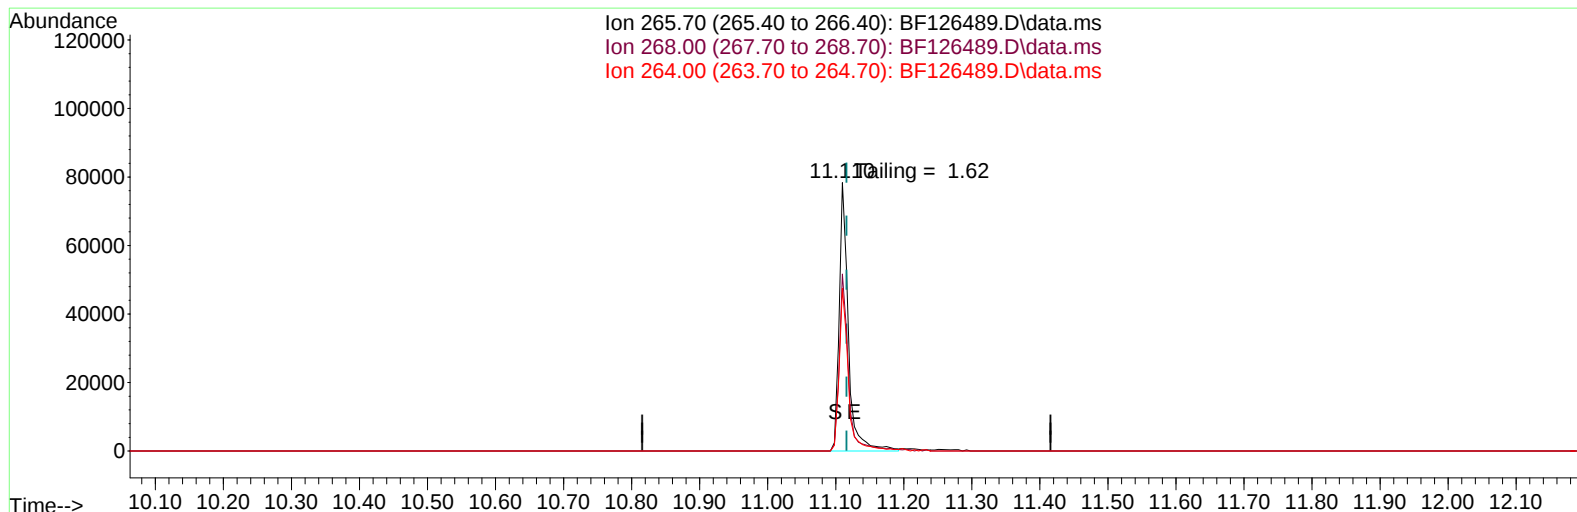

TIC: BF126489.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.006) 85282.01 ng

response 73607

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	65.96
264.00	63.00	60.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/5/2022	BNA_F	<u>BF126489.D</u>
Compound Name	Response	Retention Time
DDT	165899	13.468
DDD	2355	13.168
DDE	0	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2355	168254	1.40

Instrument :
BNA_F
ClientSampleId :
DFTPP