
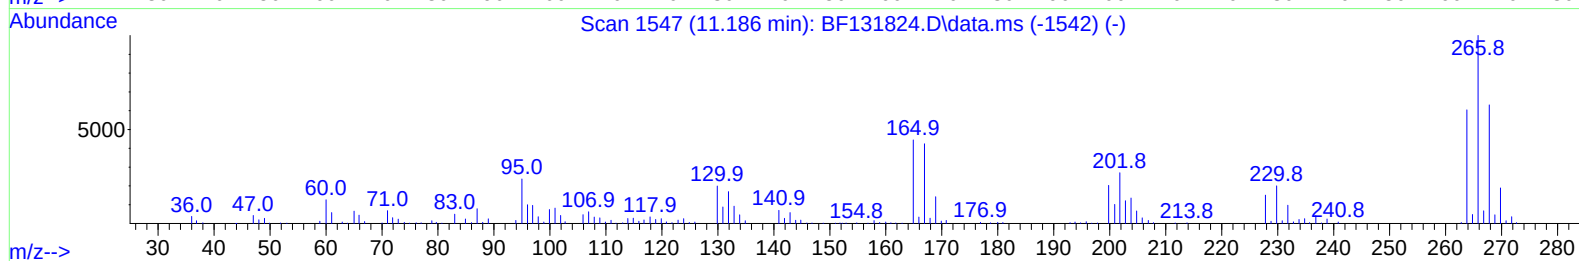
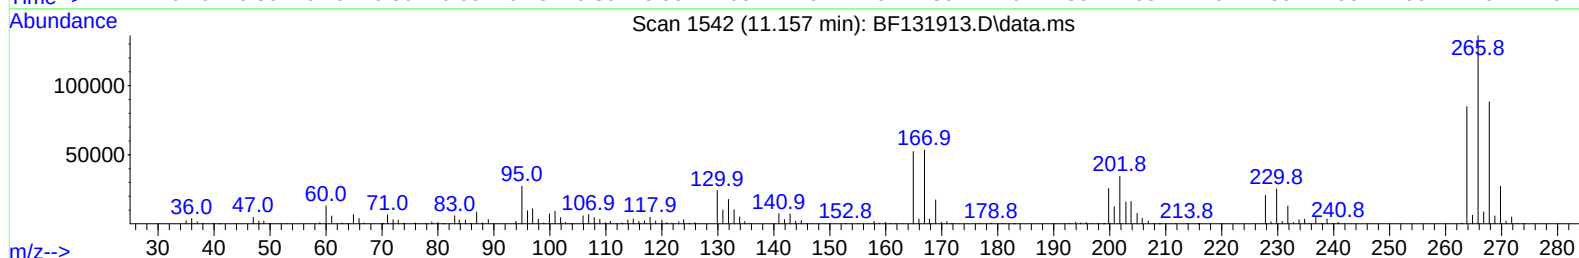


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010523\
Data File : BF131913.D
Acq On : 05 Jan 2023 13:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 01:22:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 30 02:06:40 2022
Response via : Initial Calibration

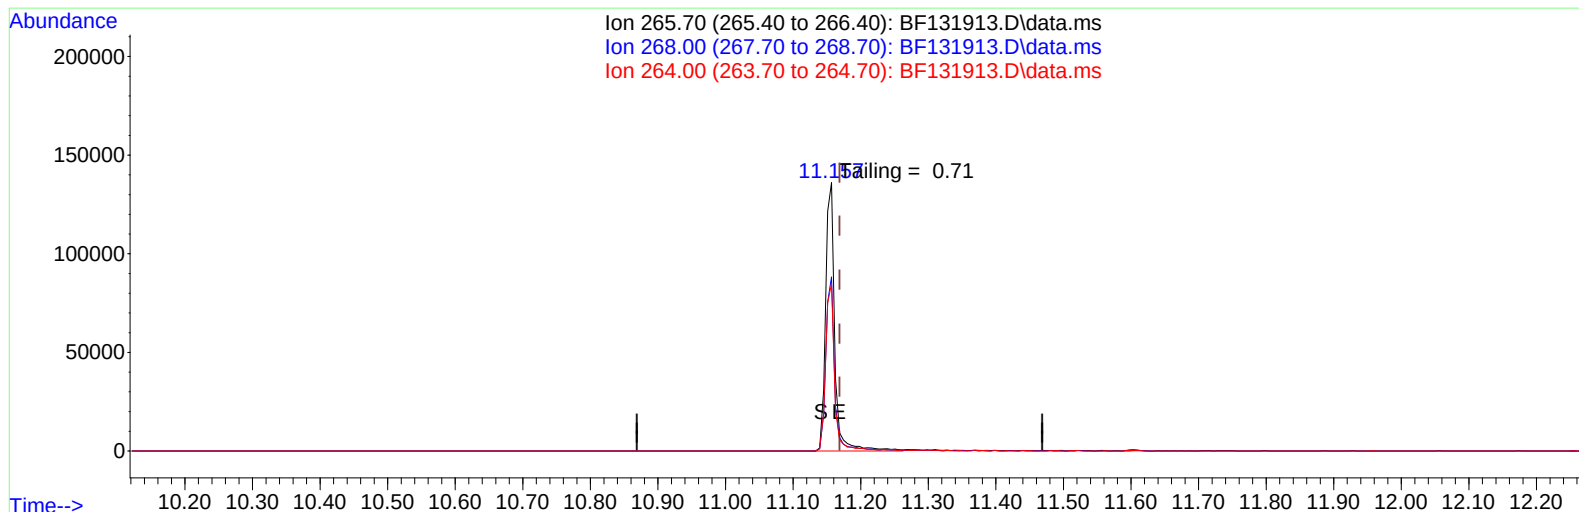

TIC: BF131913.D\data.ms

(70) Pentachlorophenol (C)




11.157min (-0.012) 152640.31 ng

response 128860

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.90
264.00	60.40	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010523\
Data File : BF131913.D
Acq On : 05 Jan 2023 13:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 01:22:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 30 02:06:40 2022
Response via : Initial Calibration

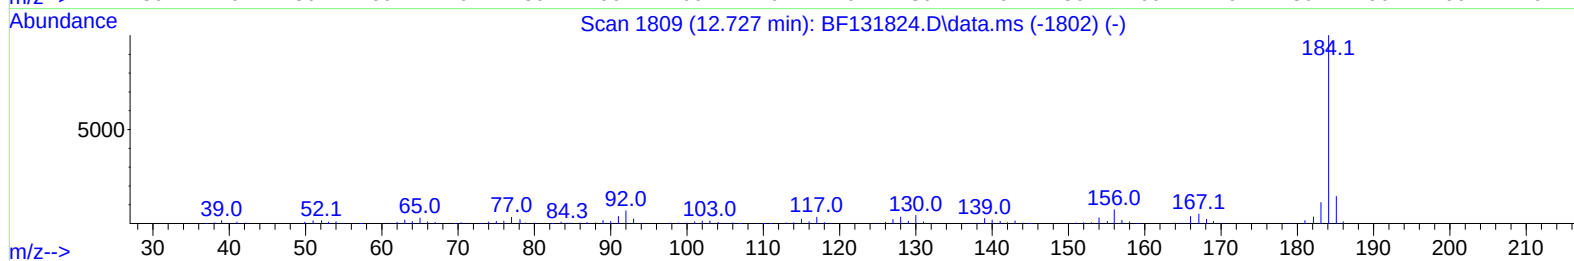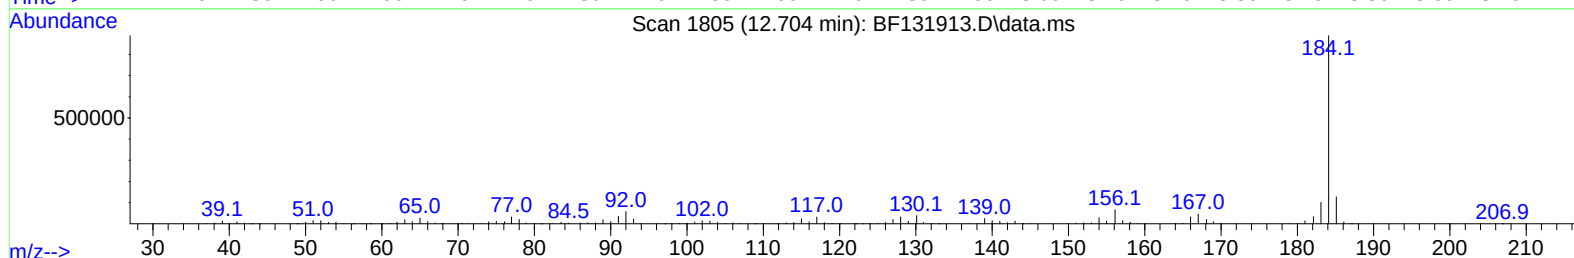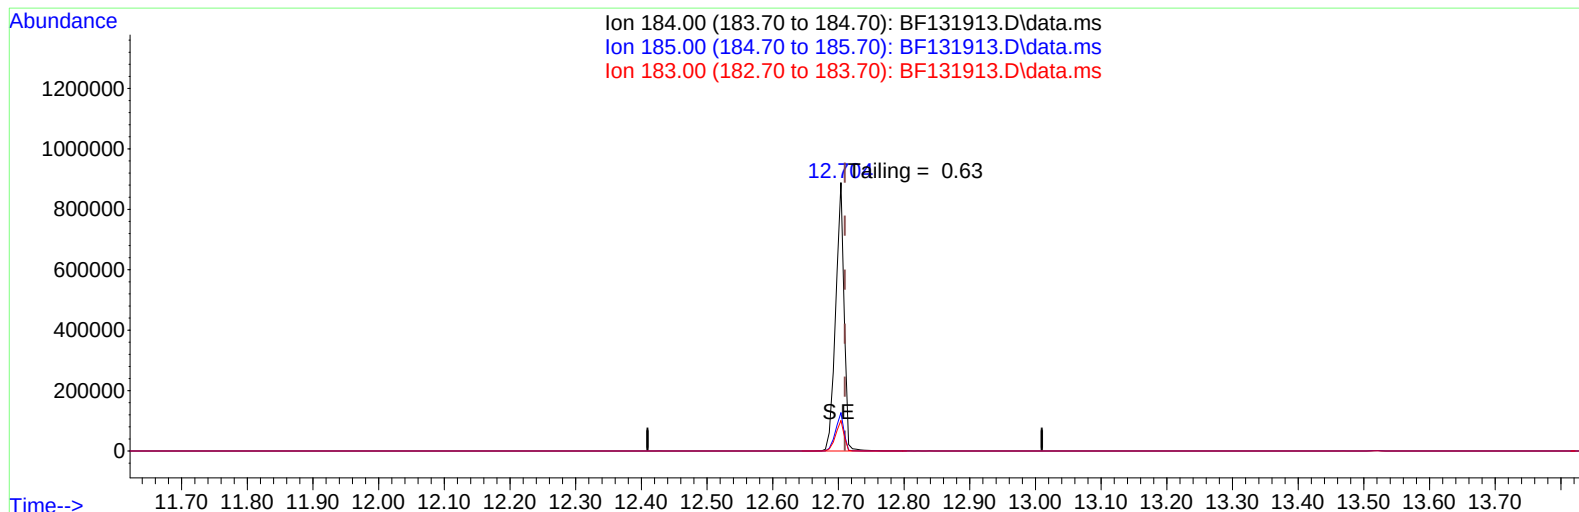

TIC: BF131913.D\data.ms

(77) Benzidine

12.704min (-0.006) 249499.83 ng

response 795438

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.32
183.00	11.20	11.42
0.00	0.00	0.00