
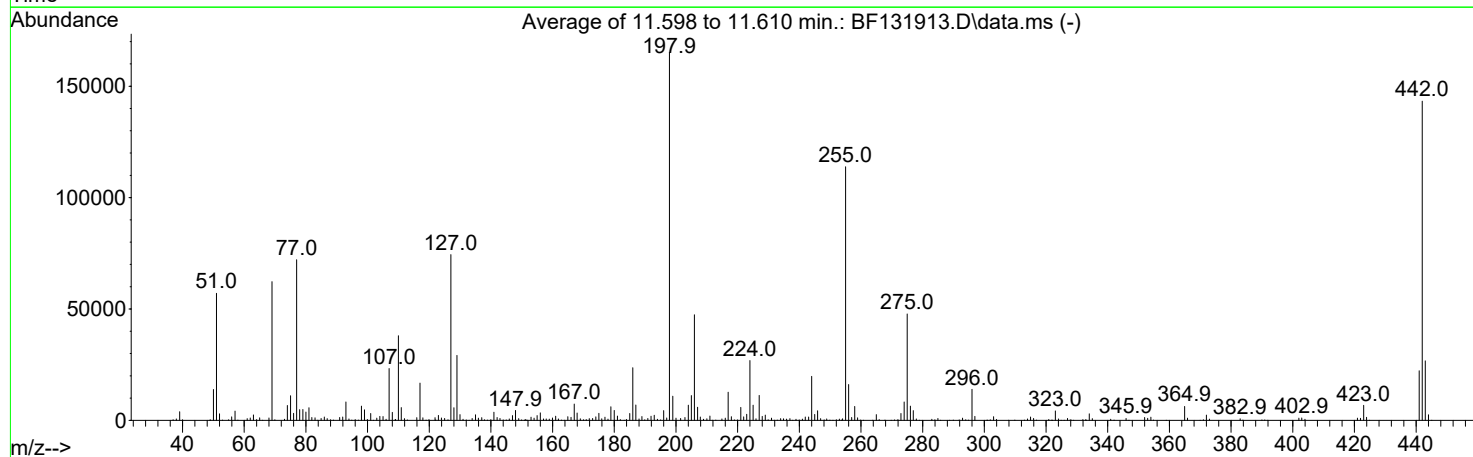


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010523\
Data File : BF131913.D
Acq On : 05 Jan 2023 13:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 06 03:02:38 2023

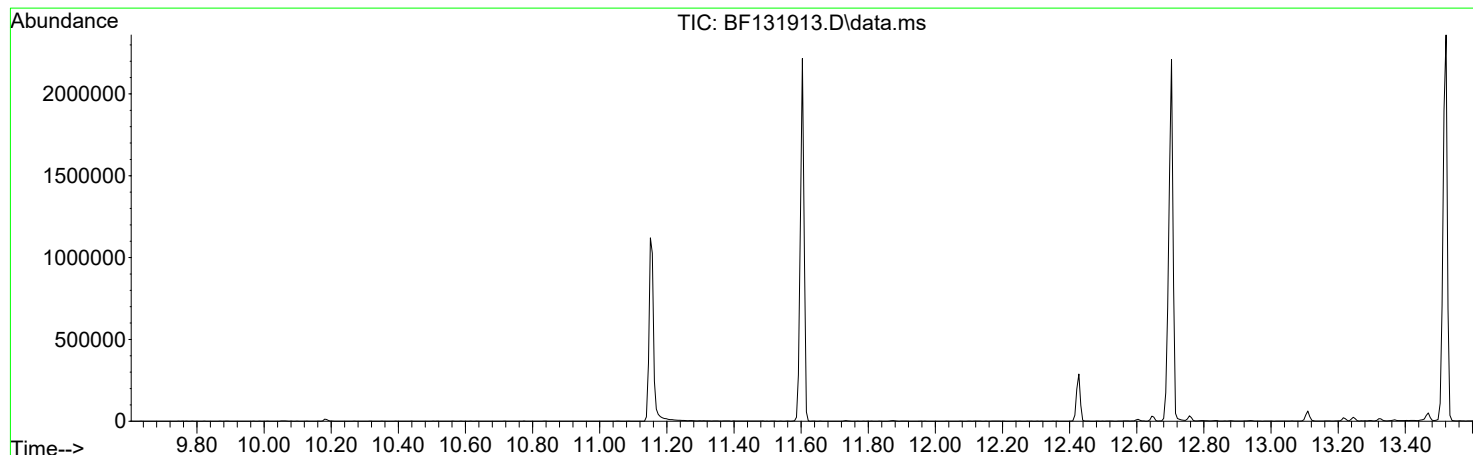

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	57045	PASS
68	69	0.00	2	1.8	1115	PASS
69	198	0.00	100	37.7	62264	PASS
70	69	0.00	2	0.5	281	PASS
127	198	10	80	45.0	74387	PASS
197	198	0.00	2	0.6	1051	PASS
198	198	100	100	100.0	165133	PASS
199	198	5	9	6.6	10871	PASS
275	198	10	60	28.9	47757	PASS
365	198	1	100	3.8	6284	PASS
441	198	0.01	100	13.5	22241	PASS
442	442	50	100	100.0	143275	PASS
443	442	15	24	18.7	26746	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
1/5/2023	BNA_F	<u>BF131913.D</u>
Compound Name	Response	Retention Time
DDT	403712	13.521
DDD	7925	13.216
DDE	614	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8539	412251	2.07

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010523\
Data File : BF131913.D
Acq On : 05 Jan 2023 13:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 06 01:22:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 30 02:06:40 2022
Response via : Initial Calibration

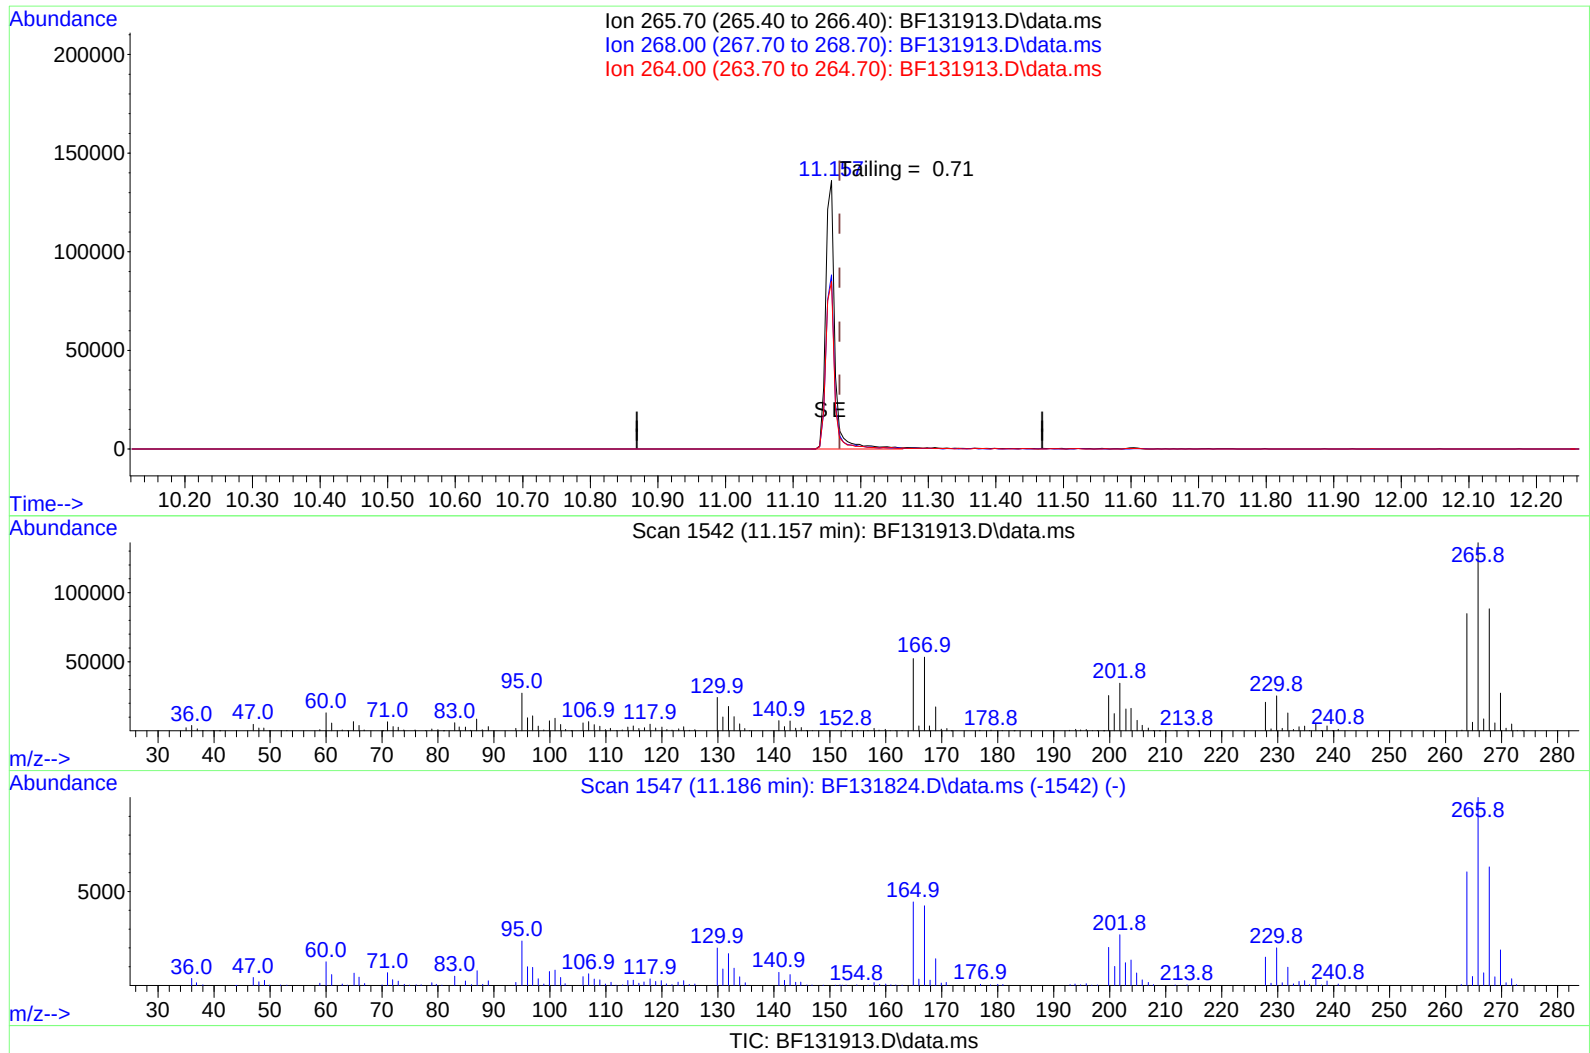

(70) Pentachlorophenol (C)

11.157min (-0.012) 152640.31 ng




response 128860

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.90
264.00	60.40	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010523\
Data File : BF131913.D
Acq On : 05 Jan 2023 13:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 06 01:22:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 30 02:06:40 2022
Response via : Initial Calibration

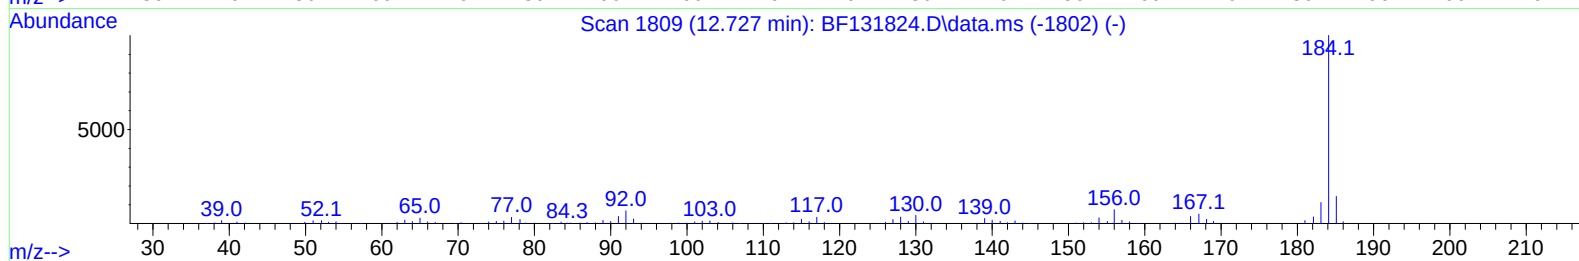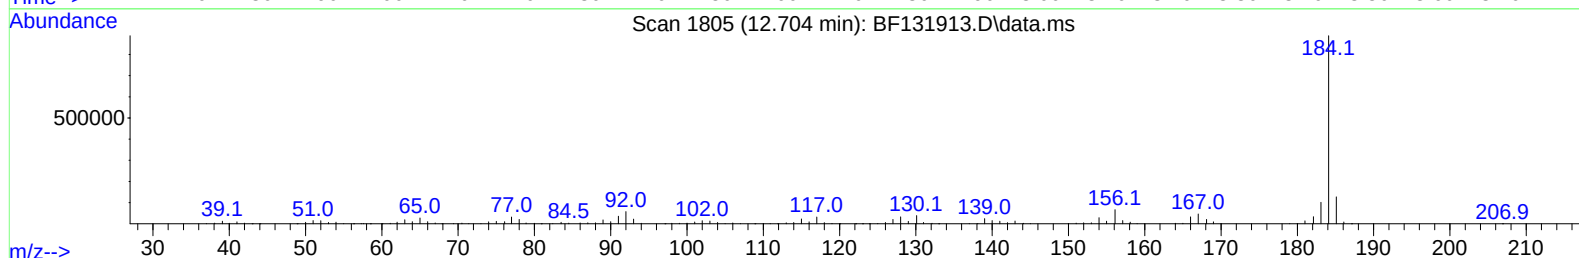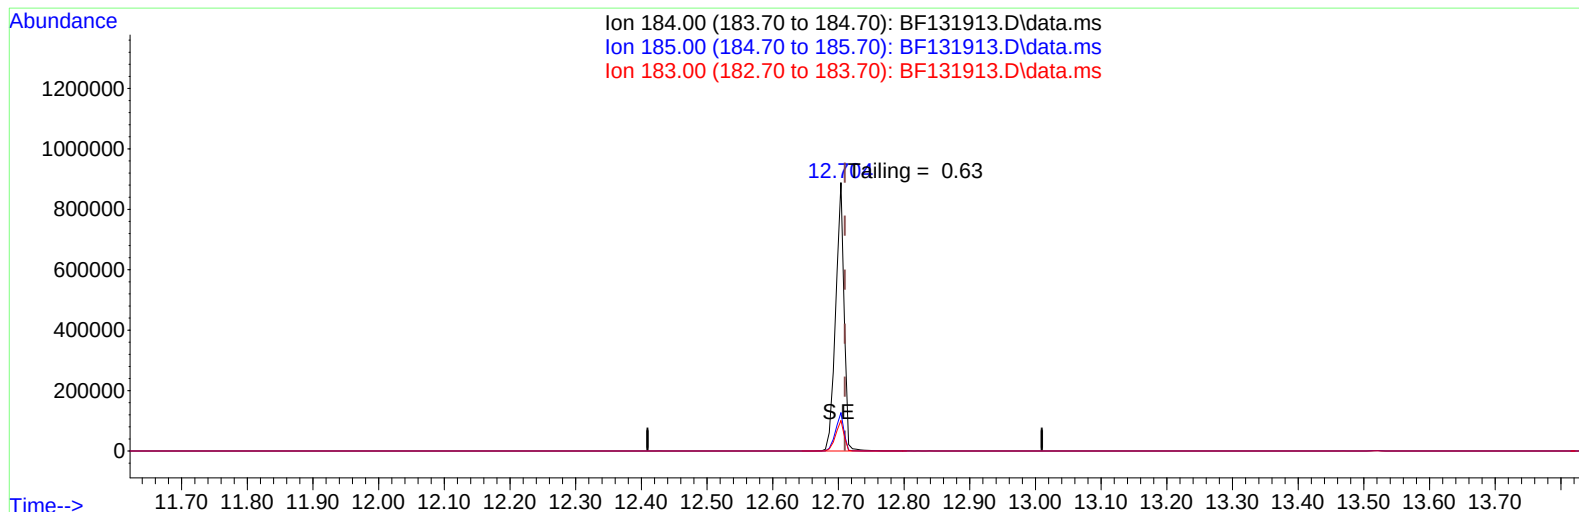

TIC: BF131913.D\data.ms

(77) Benzidine

12.704min (-0.006) 249499.83 ng

response 795438

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.32
183.00	11.20	11.42
0.00	0.00	0.00