


Data Path : Z:\HPCHEM1\BNA_F\Data\BF010615\
 Data File : BF076751.D
 Acq On : 6 Jan 2015 9:46
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 26 13:50:53 2014

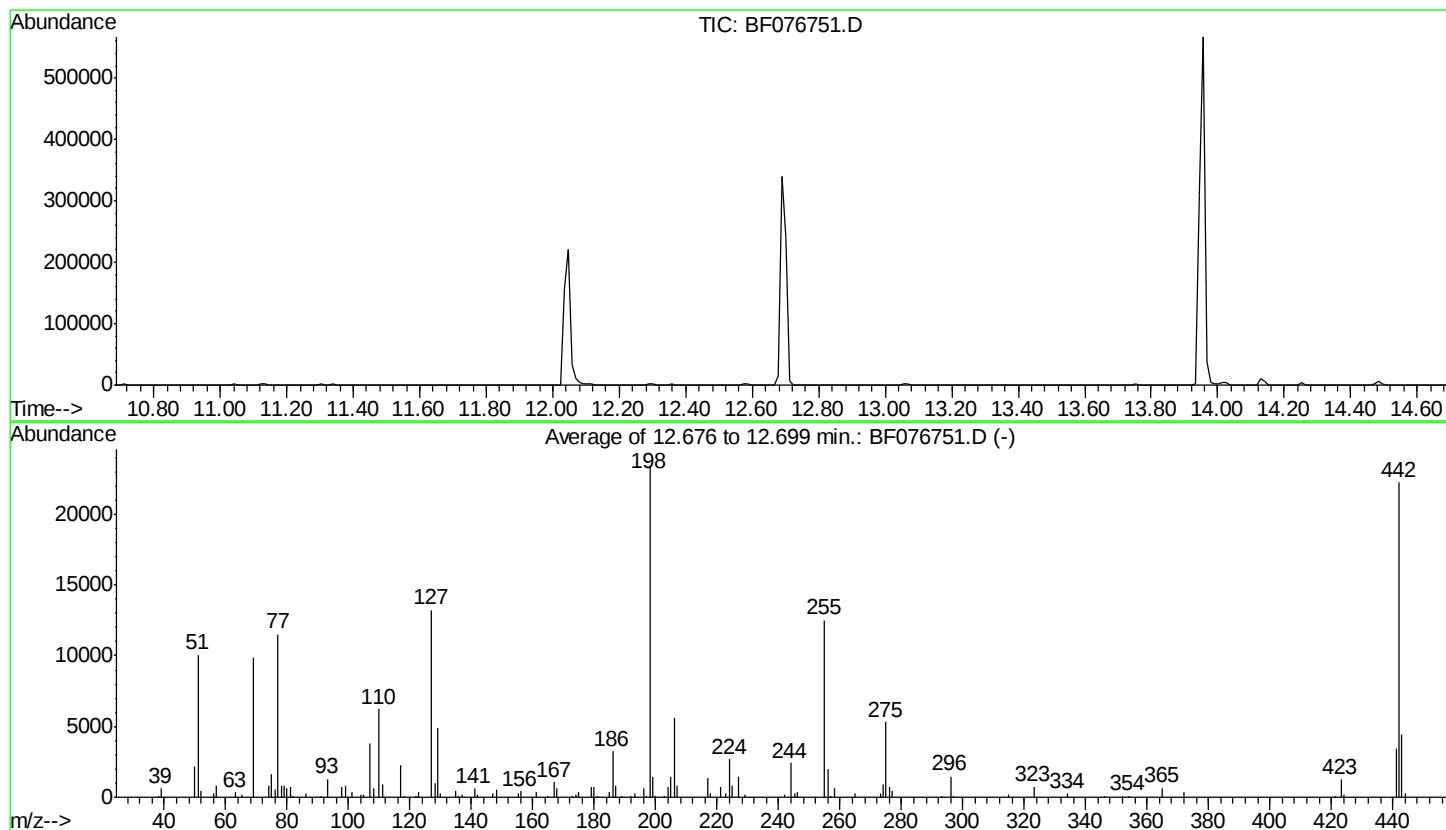

AutoFind: Scans 1014, 1015, 1016; Background Corrected with Scan 1011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	10082	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.2	9886	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.4	13218	PASS
197	198	0.00	2	0.4	104	PASS
198	198	100	100	100.0	23435	PASS
199	198	5	9	6.1	1432	PASS
275	198	10	60	22.7	5320	PASS
365	198	1	100	2.8	666	PASS
441	442	0.01	24	15.6	3469	PASS
442	198	50	100	94.9	22247	PASS
443	442	15	24	19.9	4437	PASS