


Data Path : Z:\HPCHEM1\BNA F\Data\BF010617\
 Data File : BF092108.D
 Acq On : 6 Jan 2017 10:42
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

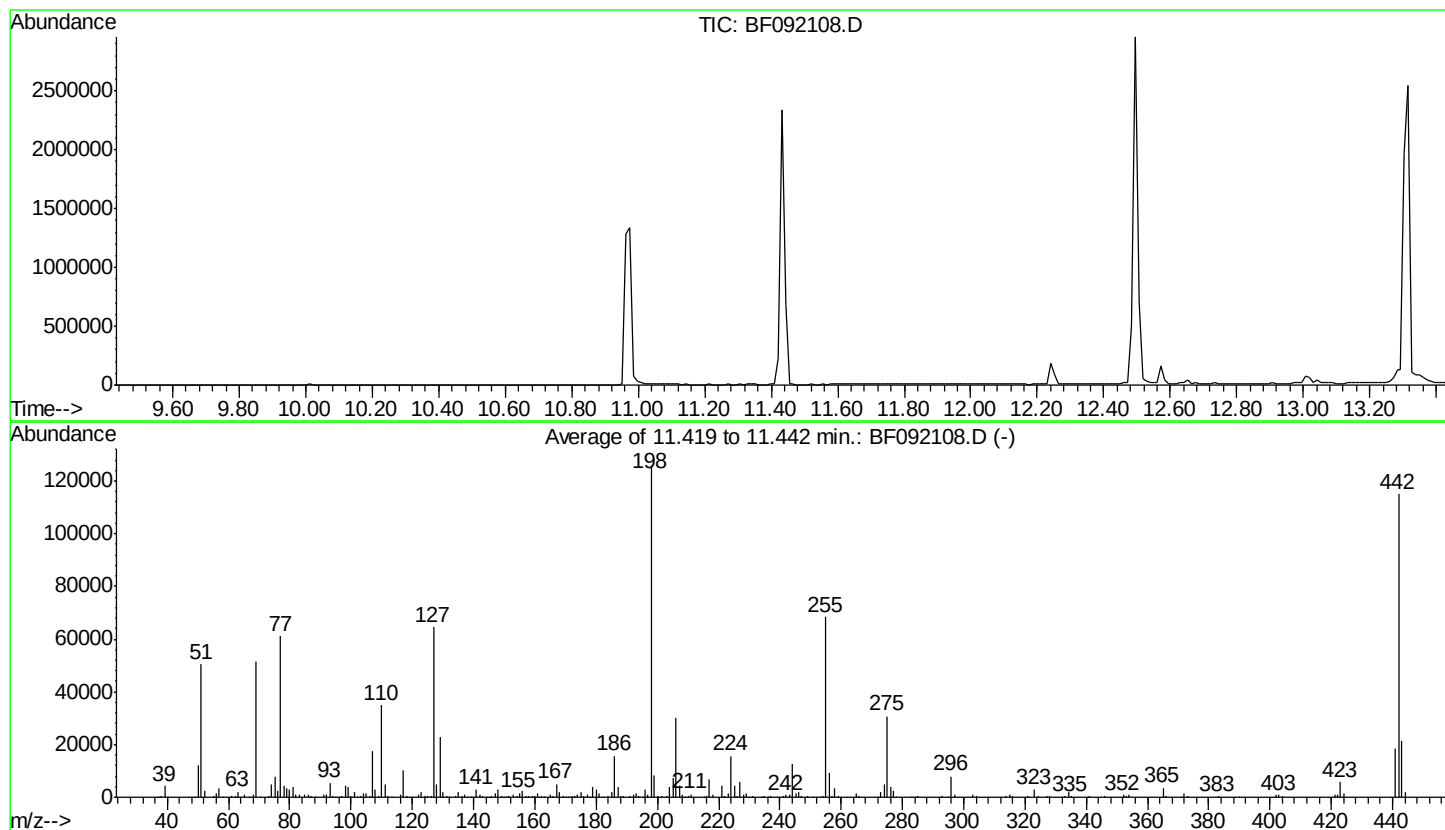

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	50469	PASS
68	69	0.00	2	1.6	816	PASS
69	198	0.00	100	40.8	51363	PASS
70	69	0.00	2	0.4	208	PASS
127	198	10	80	51.3	64506	PASS
197	198	0.00	2	0.7	834	PASS
198	198	100	100	100.0	125840	PASS
199	198	5	9	6.6	8349	PASS
275	198	10	60	24.4	30693	PASS
365	198	1	100	2.8	3533	PASS
441	442	0.01	24	15.9	18306	PASS
442	198	50	100	91.4	115052	PASS
443	442	15	24	18.8	21573	PASS