
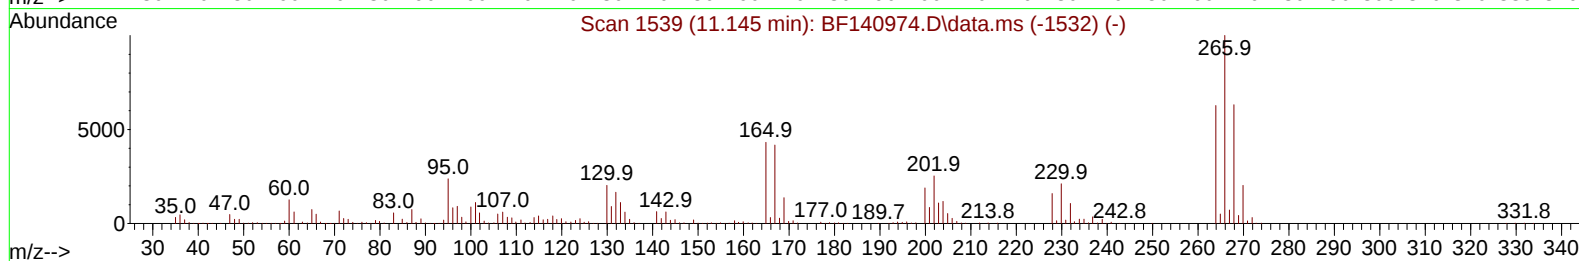
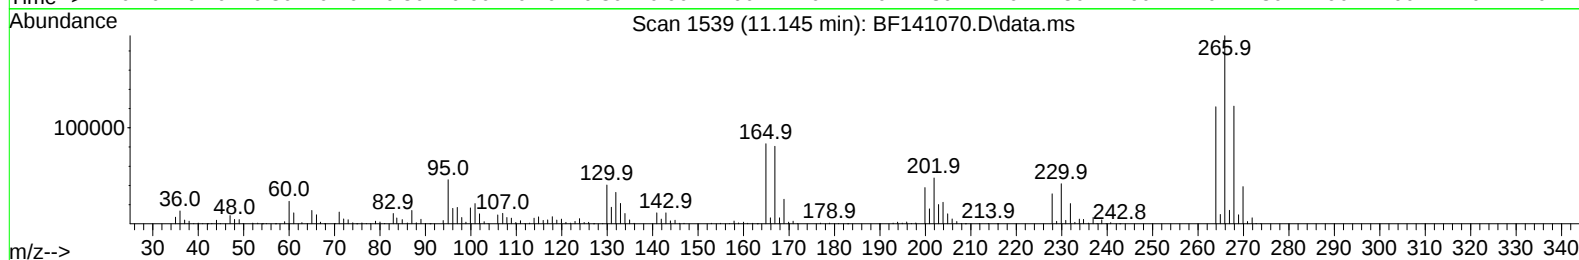


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010625\
Data File : BF141070.D
Acq On : 06 Jan 2025 12:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 13:32:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

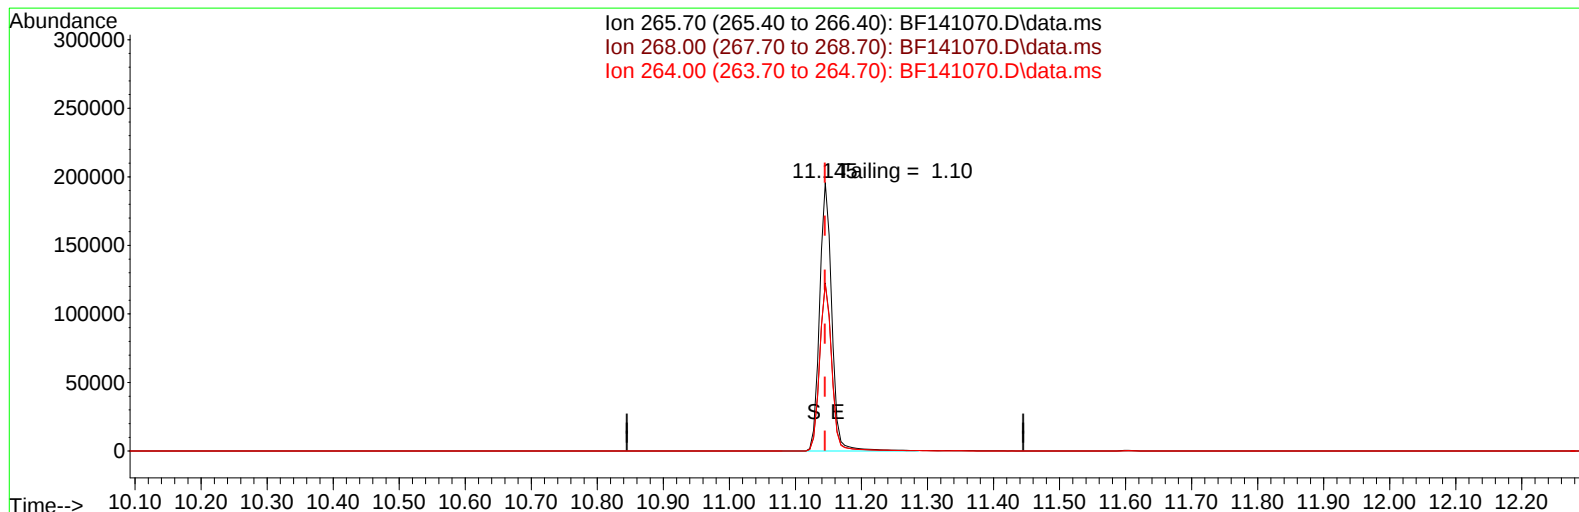

TIC: BF141070.D\data.ms

(70) Pentachlorophenol (C)




11.145min (+ 0.000) 56863.29 ng

response 251094

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.56
264.00	62.80	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010625\
Data File : BF141070.D
Acq On : 06 Jan 2025 12:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 13:32:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

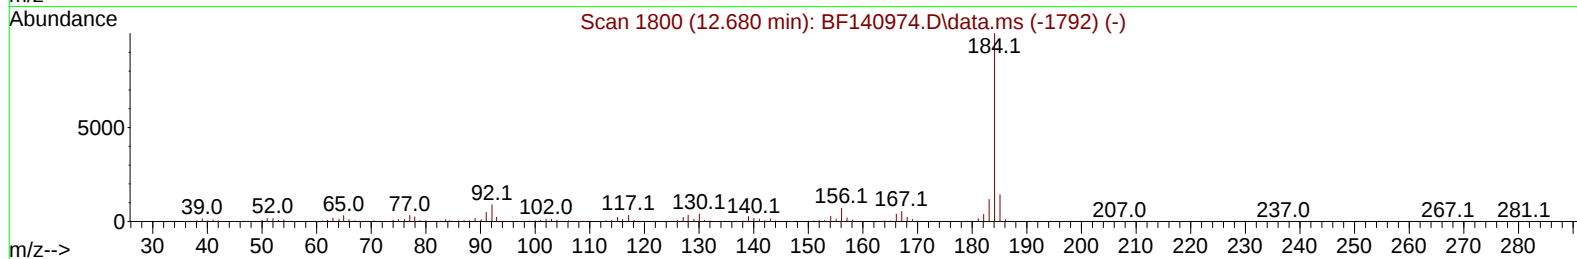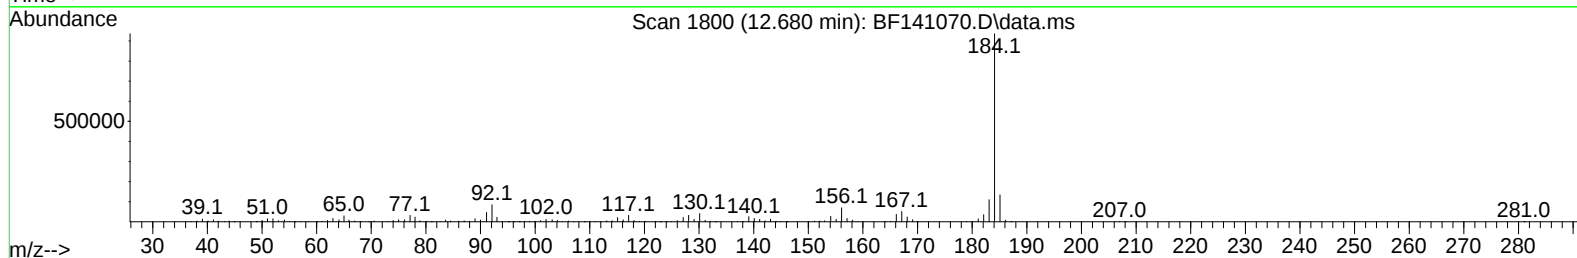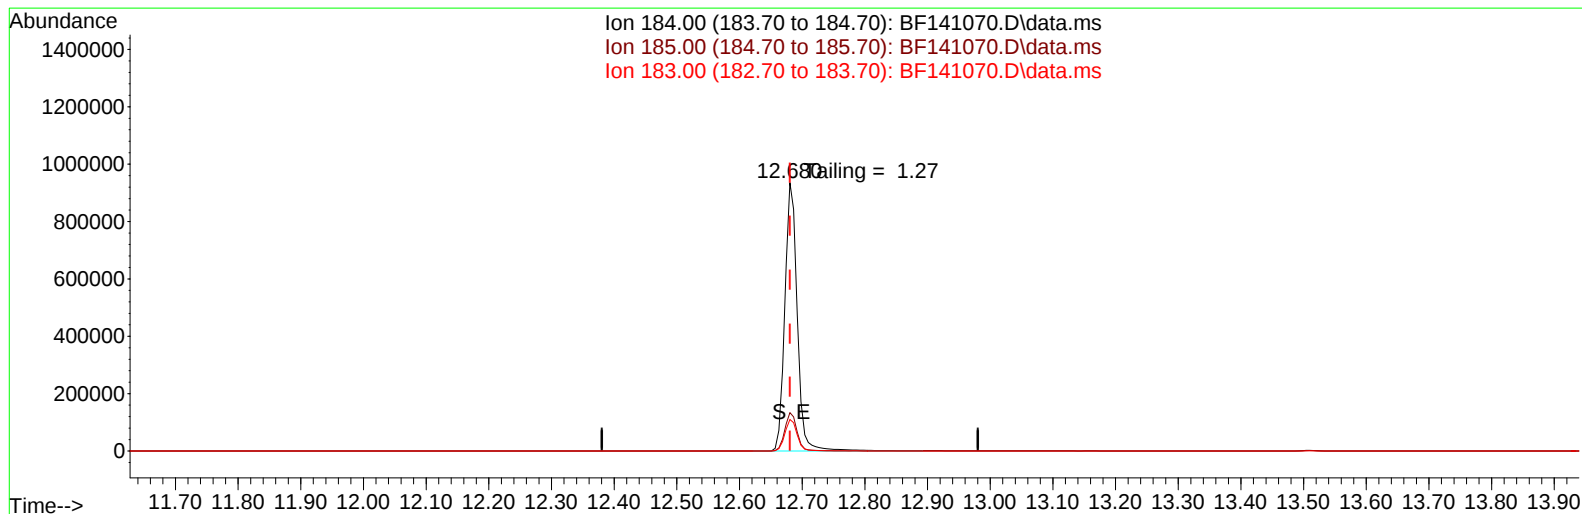

TIC: BF141070.D\data.ms

(77) Benzidine**12.680min (+ 0.000) 173264.14 ng****response 1296265**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.34
183.00	11.70	11.78
0.00	0.00	0.00