


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010625\
Data File : BF141070.D
Acq On : 06 Jan 2025 12:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 27 00:31:16 2024

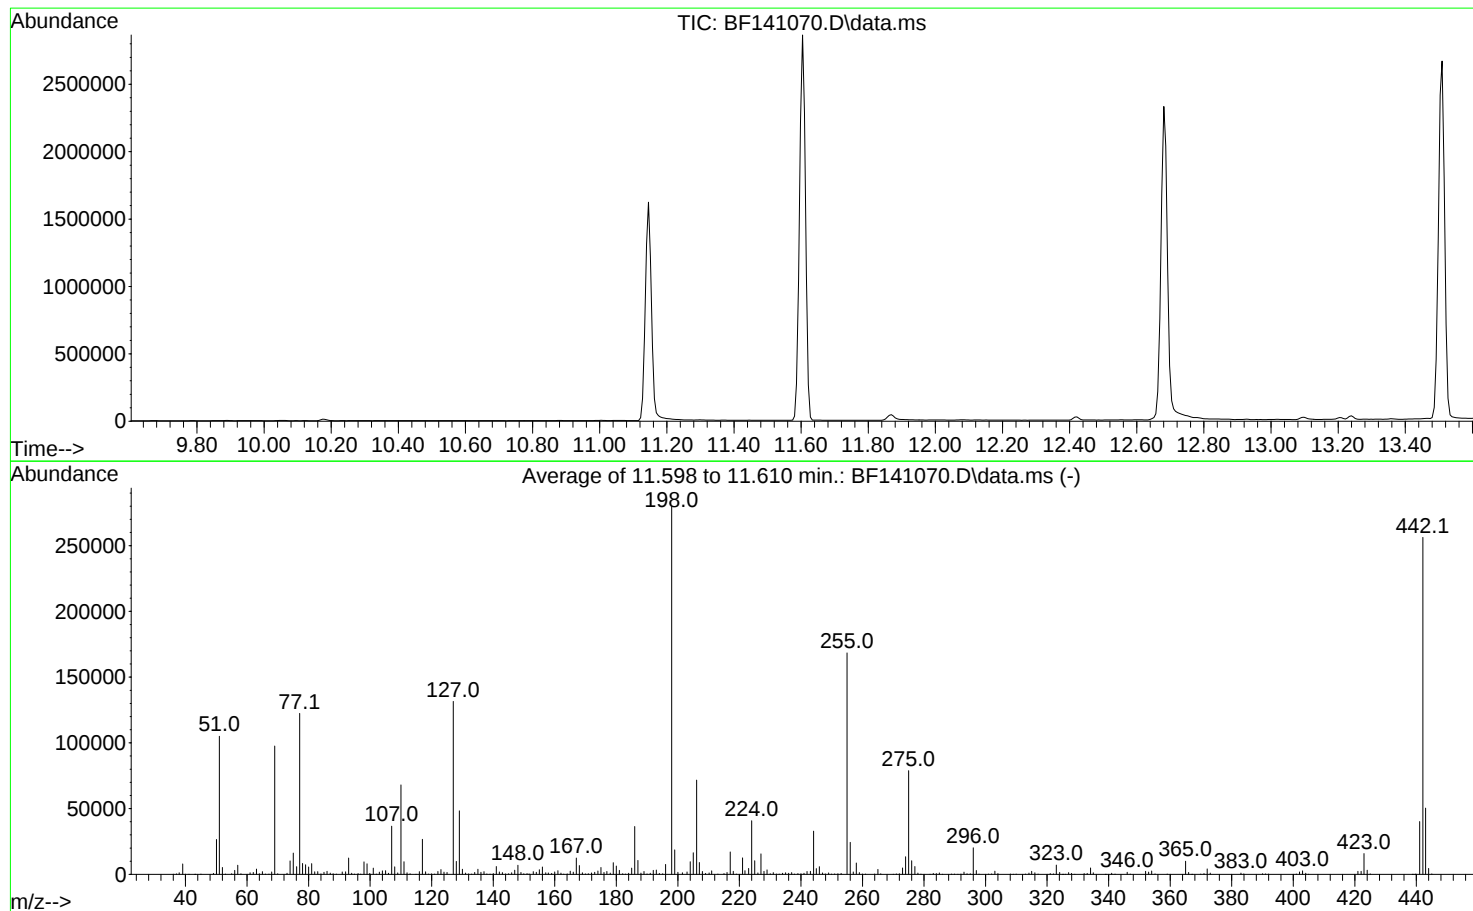

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	104963	PASS
68	69	0.00	2	1.9	1822	PASS
69	198	0.00	100	34.9	97613	PASS
70	69	0.00	2	0.6	559	PASS
127	198	10	80	47.0	131493	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	279765	PASS
199	198	5	9	6.7	18664	PASS
275	198	10	60	28.2	78829	PASS
365	198	1	100	3.6	10039	PASS
441	198	0.01	100	14.4	40219	PASS
442	442	50	100	100.0	256256	PASS
443	442	15	24	19.7	50381	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/6/2025	BNA_F	<u>BF141070.D</u>
Compound Name	Response	Retention Time
DDT	588704	13.51
DDD	8476	13.239
DDE	560	12.875
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9036	597740	1.51

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010625\
Data File : BF141070.D
Acq On : 06 Jan 2025 12:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 06 13:32:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

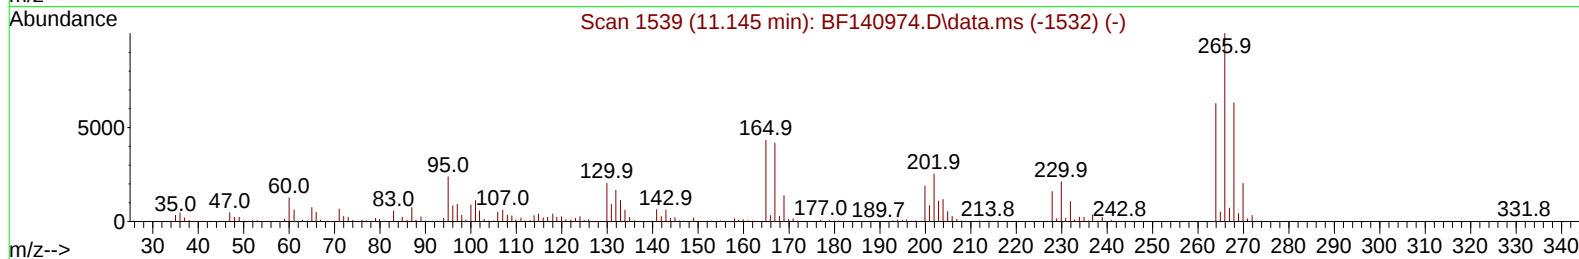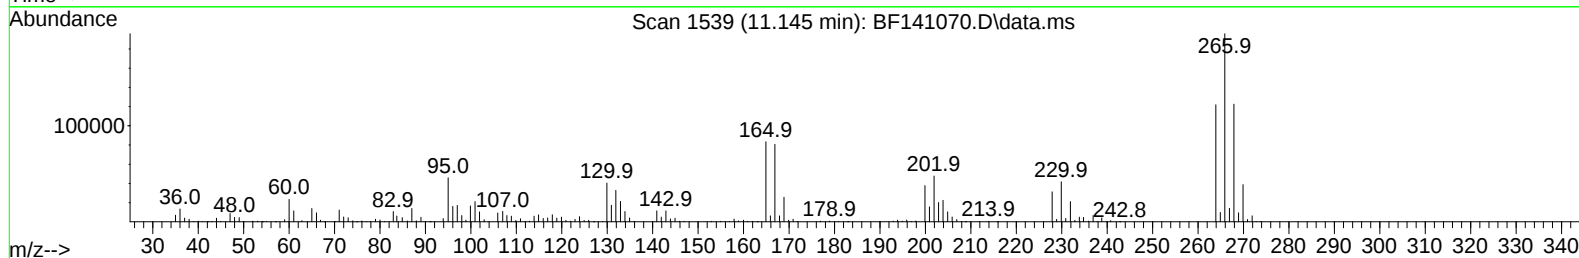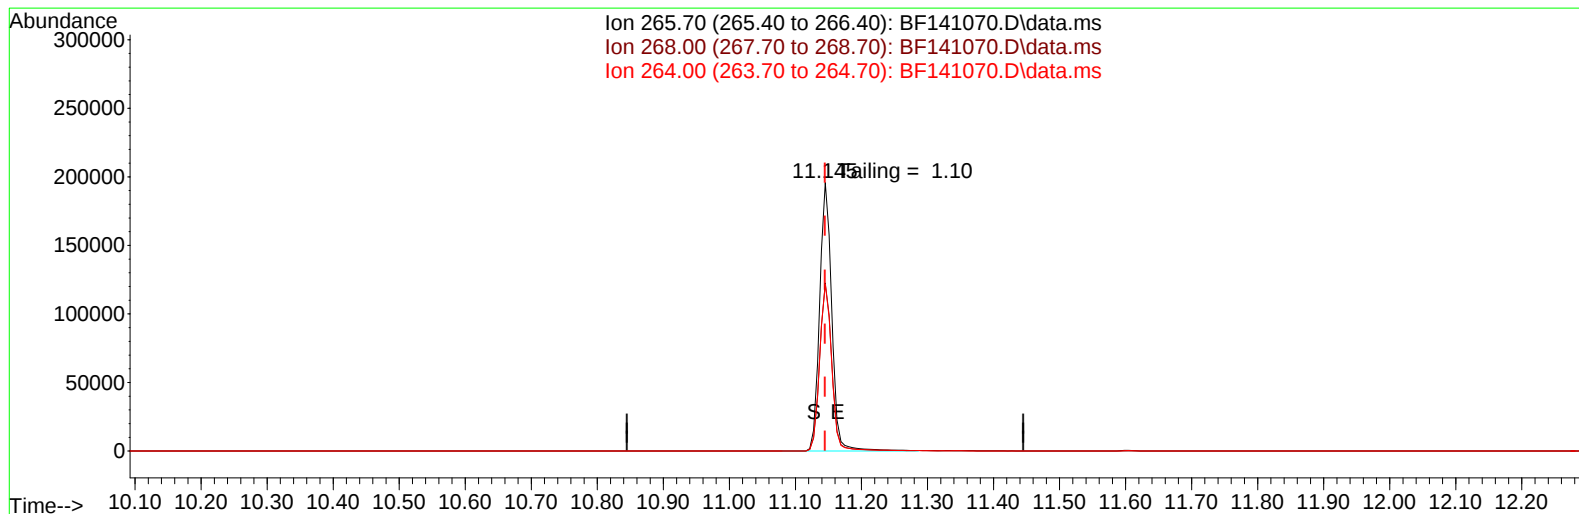

TIC: BF141070.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.000) 56863.29 ng




response 251094

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.56
264.00	62.80	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010625\
Data File : BF141070.D
Acq On : 06 Jan 2025 12:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 06 13:32:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

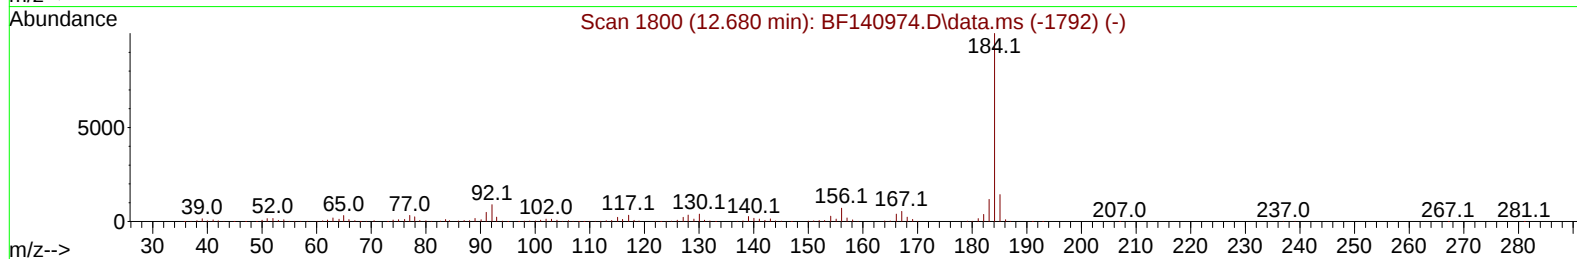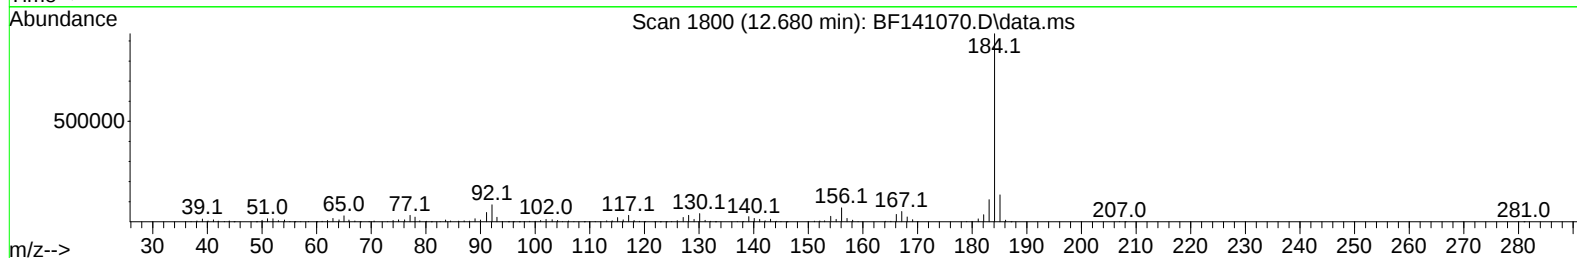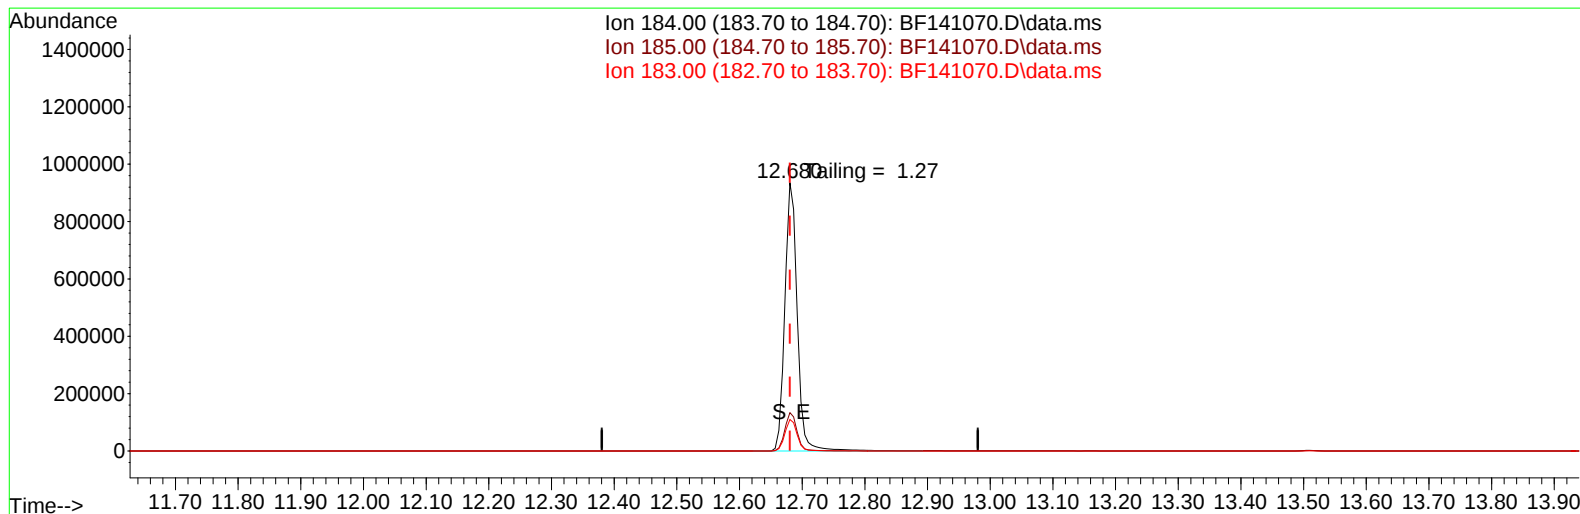

TIC: BF141070.D\data.ms

(77) Benzidine

12.680min (+ 0.000) 173264.14 ng

response 1296265

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.34
183.00	11.70	11.78
0.00	0.00	0.00